
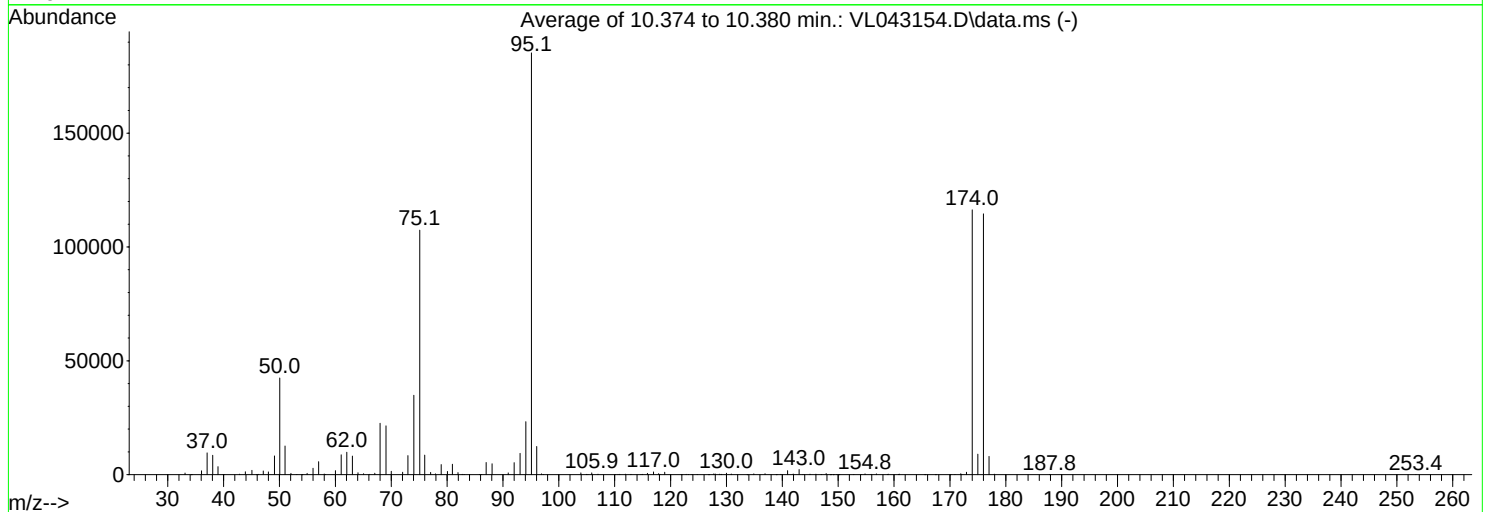


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110625\
Data File : VL043154.D
Acq On : 06 Nov 2025 06:24
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Oct 15 02:12:58 2025

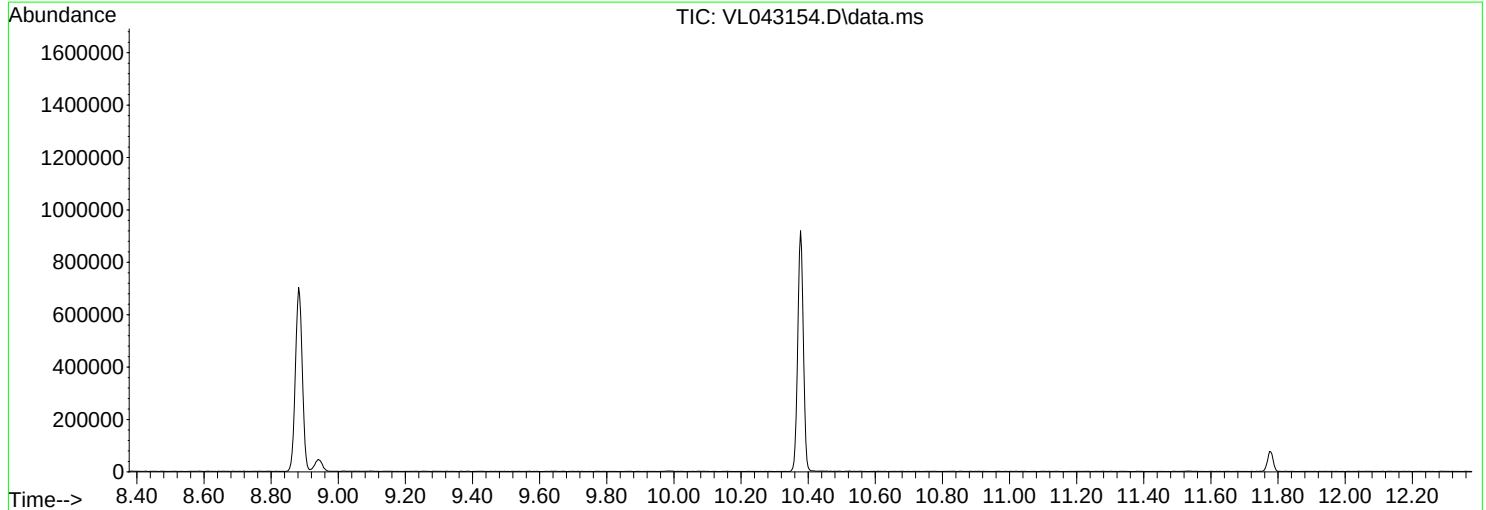

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.9	42440	PASS
75	95	30	66	58.0	107403	PASS
95	95	100	100	100.0	185280	PASS
96	95	5	9	6.7	12391	PASS
173	174	0.00	2	0.9	1086	PASS
174	95	50	120	62.8	116309	PASS
175	174	4	9	7.7	9002	PASS
176	174	93	101	98.5	114536	PASS
177	176	5	9	7.0	7990	PASS

Average of 10.374 to 10.380 min.: VL043154.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	718	46.20	126	57.00	5713	68.00	2254
34.20	24	47.10	1637	58.00	315	69.05	2145
36.05	1715	48.00	1200	58.20	85	70.00	150
37.05	9540	49.10	8233	60.00	1761	72.05	105
38.05	8532	50.05	42440	61.05	8689	73.00	8397
39.00	3502	51.00	12600	62.05	9808	74.05	34856
39.90	19	52.05	587	63.05	8134	75.10	107403
42.85	221	53.10	53	64.05	829	76.00	8608
43.90	1283	54.00	39	65.05	447	77.05	986
45.05	1927	54.95	553	66.05	120	77.90	359
45.90	28	56.00	2809	67.05	607	78.95	4459

Average of 10.374 to 10.380 min.: VL043154.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.05	1432	92.00	5302	107.00	255	118.10	164
80.95	4586	93.05	9365	110.10	82	118.95	1070
81.95	933	94.10	23259	110.60	59	121.90	28
82.70	141	95.10	185280	110.90	119	122.80	114
83.05	97	96.05	12391	111.90	202	123.20	46
84.00	62	96.90	336	112.90	183	123.85	61
85.80	84	97.20	111	114.70	103	124.75	72
86.10	47	103.95	774	115.00	169	126.80	22
87.00	5371	104.95	170	115.85	564	127.75	323
88.05	4817	105.20	46	116.95	1222	128.00	314
90.95	761	105.90	771	117.85	404	128.80	213

Average of 10.374 to 10.380 min.: VL043154.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.10	118	143.70	86	152.80	51	170.00	25
130.00	635	143.95	86	154.10	73	170.90	95
130.85	264	144.95	226	154.80	348	171.90	371
133.70	30	146.00	204	155.90	147	172.10	212
134.90	352	147.00	84	156.85	337	172.95	1086
136.90	447	147.85	475	158.80	94	174.00	116309
138.90	24	148.60	35	158.95	215	175.00	9002
139.75	156	148.80	65	160.80	139	176.00	114536
140.95	1770	149.10	30	160.95	190	177.00	7990
141.95	305	149.75	89	165.50	19	177.95	237
143.00	2233	150.10	30	167.40	21	187.85	75

Average of 10.374 to 10.380 min.: VL043154.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
253.40	44						

Instrument :

MSVOA_L

ClientSampleId :

BFB