
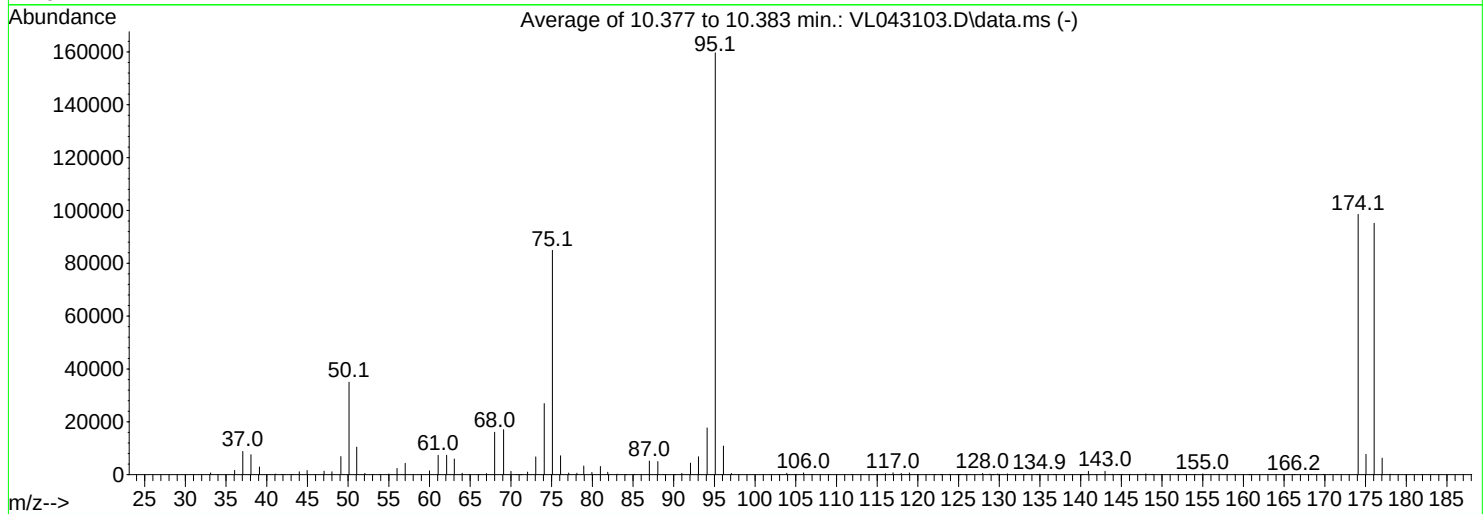


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL101425\
Data File : VL043103.D
Acq On : 14 Oct 2025 08:42
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Oct 15 02:12:58 2025

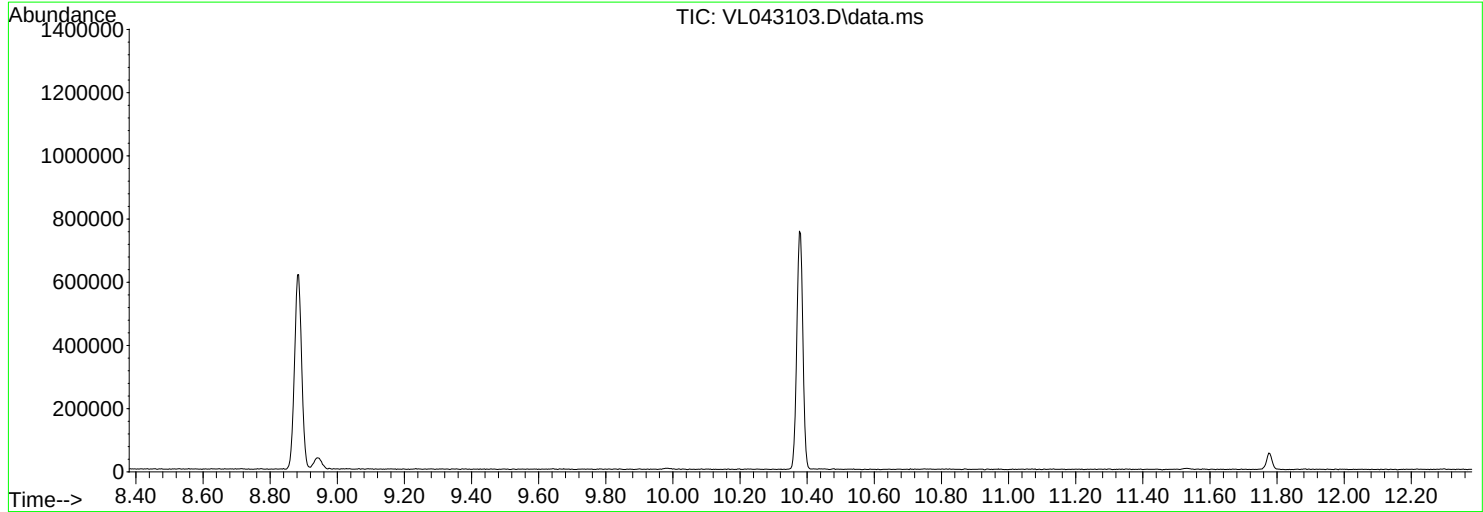

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3159

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.9	35021	PASS
75	95	30	66	53.2	84899	PASS
95	95	100	100	100.0	159660	PASS
96	95	5	9	6.8	10862	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	61.7	98536	PASS
175	174	4	9	7.8	7669	PASS
176	174	93	101	96.5	95125	PASS
177	176	5	9	6.6	6237	PASS

Average of 10.377 to 10.383 min.: VL043103.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	678	45.90	92	57.00	4329	69.10	1705
36.05	1649	47.05	1356	58.05	156	70.00	125
37.05	8803	48.00	1116	60.00	1471	70.70	4
38.05	7582	49.10	6864	61.05	7364	70.90	6
39.10	2897	50.10	35021	62.10	7323	71.20	30
41.10	216	51.05	10411	63.05	5960	72.05	989
41.85	155	52.05	464	64.00	555	73.05	6713
42.20	51	53.05	99	64.90	107	74.10	26912
43.20	141	53.90	66	66.00	21	75.10	84899
44.00	1066	55.00	227	67.00	401	76.10	7154
44.95	1561	56.00	2392	68.00	16058	77.10	609

Average of 10.377 to 10.383 min.: VL043103.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.10	547	88.80	66	104.90	96	116.95	731
78.95	3267	90.10	23	105.10	98	117.95	489
79.95	849	91.00	470	105.95	658	118.95	646
81.00	3075	92.05	4394	106.95	133	122.15	88
81.90	894	93.05	6769	109.15	79	122.80	36
83.05	174	94.10	17698	110.00	104	123.95	104
84.10	11	95.10	159660	111.90	140	124.80	48
85.15	151	96.10	10862	113.05	117	125.10	22
86.00	122	97.10	451	115.00	138	125.80	25
87.00	5156	102.90	75	115.60	71	127.95	496
88.05	4968	103.90	541	116.00	350	128.85	219

Average of 10.377 to 10.383 min.: VL043103.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.20	37	141.90	157	152.85	142	171.50	128
129.80	225	143.00	1303	154.05	106	172.05	103
130.00	213	143.90	121	155.00	312	174.10	98536
131.00	303	144.75	83	157.00	199	175.05	7669
133.10	19	145.10	42	158.95	159	176.05	95125
134.60	38	146.05	150	160.70	27	177.05	6237
134.95	203	147.00	115	160.90	91	178.05	186
136.70	112	148.00	286	166.20	19		
136.90	134	148.80	100	168.35	50		
140.10	20	149.95	150	169.80	113		
140.95	1257	152.00	23	170.65	62		

Instrument :

MSVOA_L

ClientSampleId :

BFB