

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110625\
 Data File : VL043164.D
 Acq On : 06 Nov 2025 13:17
 Operator : SY/MD
 Sample : Q3557-02
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 141-IA-1

Quant Time: Nov 07 00:21:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Wed Oct 15 02:12:58 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	115366	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	342427	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.881	117	290452	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.377	95	237353	10.513	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	105.100%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.499	85	24649	1.503	ppbv	96
3) Chlorodifluoromethane	1.476	51	11497	0.648	ppbv #	79
4) Chloromethane	1.534	50	2908	0.448	ppbv	96
8) Dichlorotetrafluoroethane	1.499	85	24649	1.859	ppbv #	21
9) Propene	1.560	41	45237	5.748	ppbv	98
10) Heptane	4.985	43	1712	0.076	ppbv #	27
11) Trichlorofluoromethane	1.884	101	5366	0.334	ppbv	94
12) 1,1,2-Trichlorotrifluoro...	2.146	101	1035	0.080	ppbv	91
13) Ethanol	1.722	45	76195	26.173	ppbv	100
15) Acetone	1.839	43	138148	8.884	ppbv	92
16) 1,3-Butadiene	1.602	39	1714	0.231	ppbv #	13
17) tert-Butyl alcohol	2.046	59	1651	0.077	ppbv #	72
19) Isopropyl Alcohol	1.887	45	9578	0.989	ppbv #	1
20) Methylene Chloride	2.065	84	97396	15.846	ppbv	93
21) Allyl Chloride	2.081	41	3894	0.340	ppbv #	1
23) Vinyl Acetate	2.479	43	43597	1.914	ppbv #	50
25) Ethyl Acetate	2.829	43	86024	2.231	ppbv #	80
26) Hexane	2.832	57	122149	6.875	ppbv #	42
27) Carbon Disulfide	2.156	76	508	0.031	ppbv #	1
29) Chloroform	2.852	83	1705	0.066	ppbv #	75
30) Cyclohexane	3.865	84	3316	0.214	ppbv #	79
34) 2-Butanone	2.560	43	34716	1.508	ppbv	99
36) Benzene	3.661	78	12305	0.382	ppbv	98
37) 1,2-Dichloroethane	3.224	62	1623	0.087	ppbv #	94
39) 1,2-Dichloropropane	3.962	63	85408	7.244	ppbv #	24
41) Tetrahydrofuran	3.237	42	2049	0.159	ppbv #	63
44) 2,2,4-Trimethylpentane	4.641	57	17870	0.328	ppbv #	78
51) 2-Hexanone	7.441	43	5610	0.235	ppbv #	53
53) Toluene	6.936	91	22705	0.593	ppbv	97
58) Ethyl Benzene	9.360	91	2883	0.058	ppbv	94
59) m/p-Xylene	9.535	91	15295	0.385	ppbv	99
60) o-Xylene	9.969	91	5758	0.147	ppbv	94
73) 1,3,5-Trimethylbenzene	11.209	105	1713	0.043	ppbv #	81
74) 1,2,4-Trimethylbenzene	11.539	105	5751	0.129	ppbv #	55
79) Naphthalene	13.516	128	6044	0.130	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 07 00:21:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 26 06:05:16 2022
QLast Update : Wed Oct 15 02:12:58 2025
Response via : Initial Calibration









#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.790 min Scan# 835
Delta R.T. 0.000 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17




Instrument :
MSVOA_L
ClientSampleId :
141-IA-1


Tgt Ion: 49 Resp: 115366
Ion Ratio Lower Upper
49 100
128 48.9 24.4 73.4
130 62.7 31.0 93.0

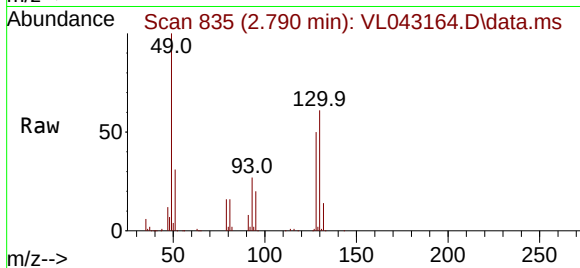

#2
Dichlorodifluoromethane
Concen: 1.503 ppbv
RT: 1.499 min Scan# 436
Delta R.T. -0.000 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17

Tgt Ion: 85 Resp: 24649
Ion Ratio Lower Upper
85 100
87 29.5 25.3 37.9




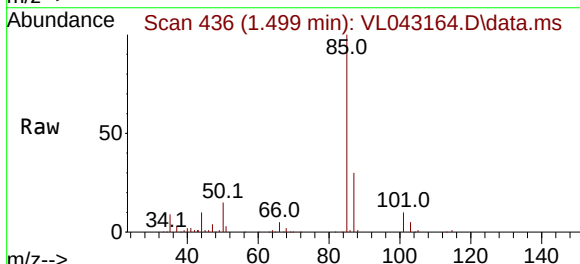




#3
Chlorodifluoromethane
Concen: 0.648 ppbv
RT: 1.476 min Scan# 41
Delta R.T. -0.000 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17




Instrument :
MSVOA_L
ClientSampleId :
141-IA-1


Tgt Ion: 51 Resp: 11497
Ion Ratio Lower Upper
51 100
67 9.5 15.1 22.7#

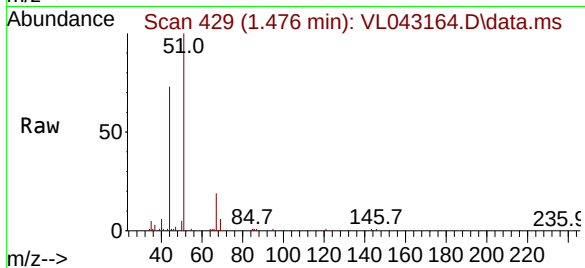

#4
Chloromethane
Concen: 0.448 ppbv
RT: 1.534 min Scan# 447
Delta R.T. -0.000 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17

Tgt Ion: 50 Resp: 2908
Ion Ratio Lower Upper
50 100
52 33.9 25.2 37.8




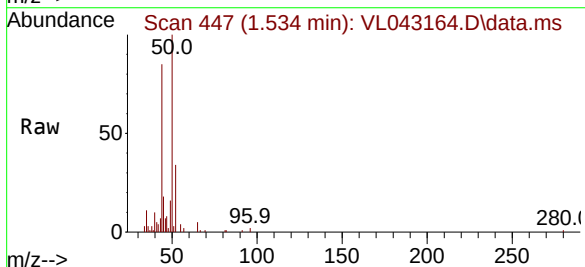




#8
 Dichlorotetrafluoroethane
 Concen: 1.859 ppbv
 RT: 1.499 min Scan# 41
 Delta R.T. -0.059 min
 Lab File: VL043164.D
 Acq: 06 Nov 2025 13:17




Instrument :
 MSVOA_1
 ClientSampleId :
 141-IA-1


Tgt Ion: 85 Resp: 24649
 Ion Ratio Lower Upper
 85 100
 135 0.6 48.2 72.4#

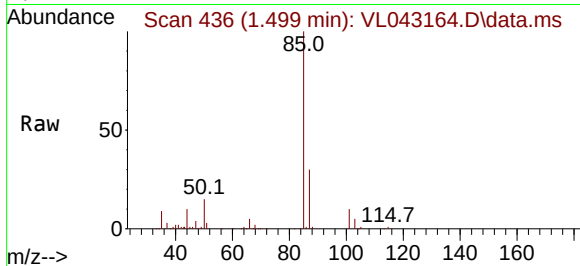

#9
 Propene
 Concen: 5.748 ppbv
 RT: 1.560 min Scan# 455
 Delta R.T. 0.077 min
 Lab File: VL043164.D
 Acq: 06 Nov 2025 13:17

Tgt Ion: 41 Resp: 45237
 Ion Ratio Lower Upper
 41 100
 42 70.2 55.1 82.7




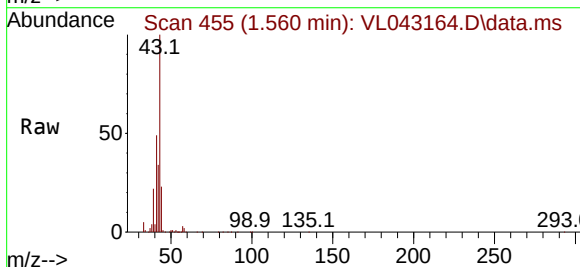




#10
Heptane
Concen: 0.076 ppbv
RT: 4.985 min Scan# 11
Delta R.T. -0.000 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17




Instrument :
MSVOA_L
ClientSampleId :
141-IA-1


Tgt Ion: 43 Resp: 1712
Ion Ratio Lower Upper
43 100
57 0.0 40.8 61.2#

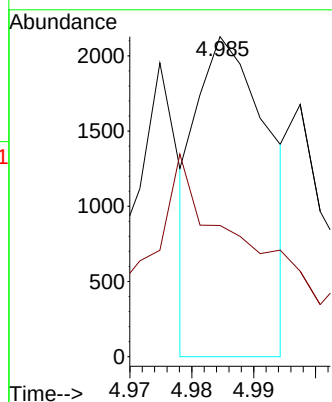

#11
Trichlorofluoromethane
Concen: 0.334 ppbv
RT: 1.884 min Scan# 555
Delta R.T. 0.003 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17

Tgt Ion:101 Resp: 5366
Ion Ratio Lower Upper
101 100
103 56.9 49.3 73.9



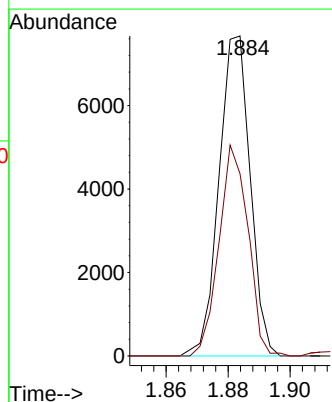





#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.080 ppbv
 RT: 2.146 min Scan# 61
 Delta R.T. 0.003 min
 Lab File: VL043164.D
 Acq: 06 Nov 2025 13:17




Instrument :
 MSVOA_1
 ClientSampleId :
 141-IA-1


Tgt Ion:101 Resp: 1035
 Ion Ratio Lower Upper
 101 100
 151 61.2 54.7 82.1

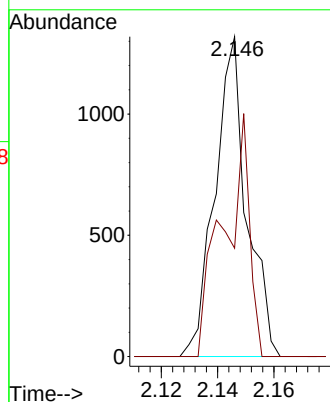

#13
 Ethanol
 Concen: 26.173 ppbv
 RT: 1.722 min Scan# 505
 Delta R.T. -0.000 min
 Lab File: VL043164.D
 Acq: 06 Nov 2025 13:17

Tgt Ion: 45 Resp: 76195
 Ion Ratio Lower Upper
 45 100
 46 36.8 14.7 58.9



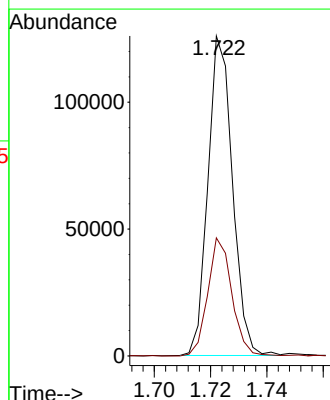





#15
Acetone
Concen: 8.884 ppbv
RT: 1.839 min Scan# 541
Delta R.T. 0.003 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17




Instrument :
MSVOA_L
ClientSampleId :
141-IA-1


Tgt Ion: 43 Resp: 138148
Ion Ratio Lower Upper
43 100
58 30.2 20.8 31.2

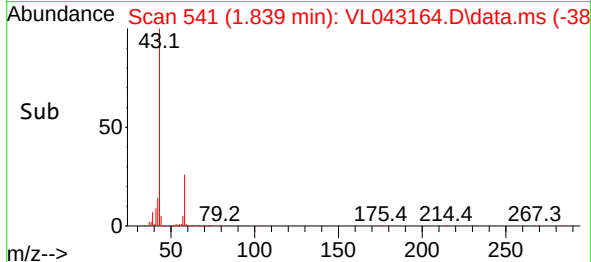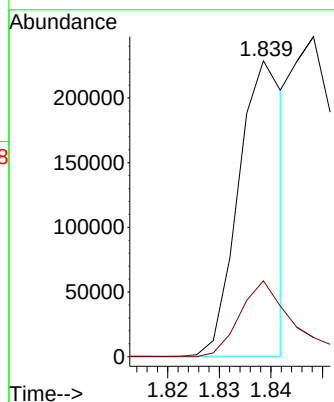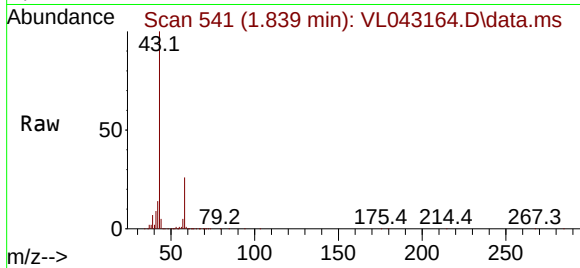

#16
1,3-Butadiene
Concen: 0.231 ppbv
RT: 1.602 min Scan# 468
Delta R.T. -0.010 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17

Tgt Ion: 39 Resp: 1714
Ion Ratio Lower Upper
39 100
54 0.0 59.0 88.4#

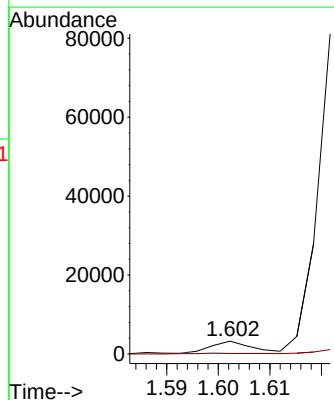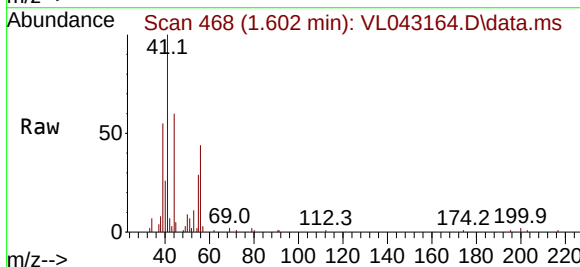



#17

tert-Butyl alcohol

Concen: 0.077 ppbv

RT: 2.046 min Scan# 604

Delta R.T. 0.003 min

Lab File: VL043164.D

Acq: 06 Nov 2025 13:17

Instrument :

MSVOA_1

ClientSampleId :





141-IA-1

Tgt Ion: 59 Resp: 1651

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.4#

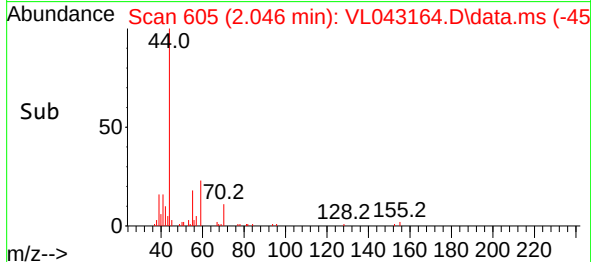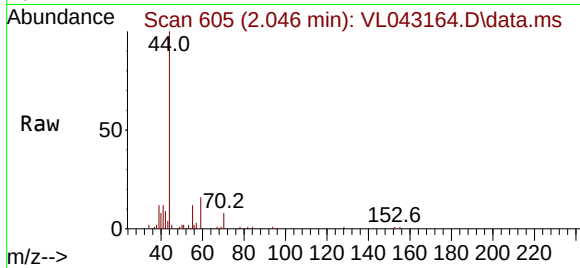

#19

Isopropyl Alcohol

Concen: 0.989 ppbv

RT: 1.887 min Scan# 556

Delta R.T. -0.000 min

Lab File: VL043164.D




Acq: 06 Nov 2025 13:17


Tgt Ion: 45 Resp: 9578

Ion Ratio Lower Upper

45 100

58 434.7 31.3 46.9#

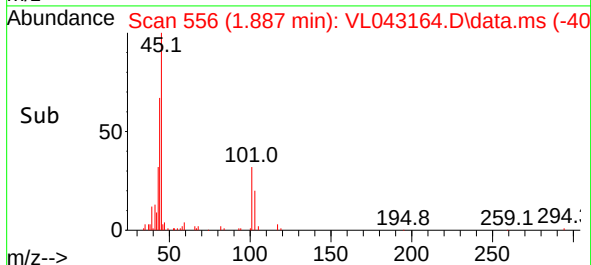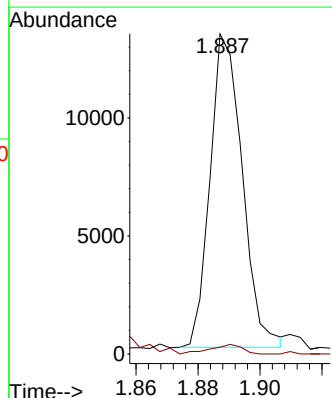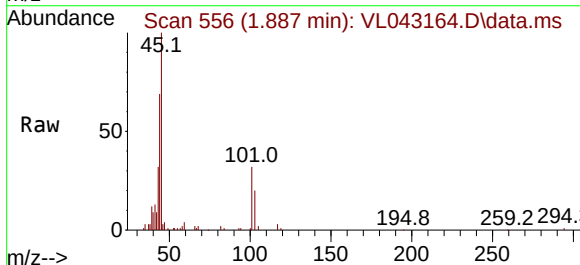



#20

Methylene Chloride

Concen: 15.846 ppbv

RT: 2.065 min Scan# 611

Delta R.T. -0.000 min

Lab File: VL043164.D

Acq: 06 Nov 2025 13:17

Instrument :

MSVOA_L

ClientSampleId :

141-IA-1

Tgt Ion: 84 Resp: 97396





Ion Ratio Lower Upper

84 100

49 152.0 116.6 175.0

51 47.2 34.8 52.2

86 66.6 46.2 69.4

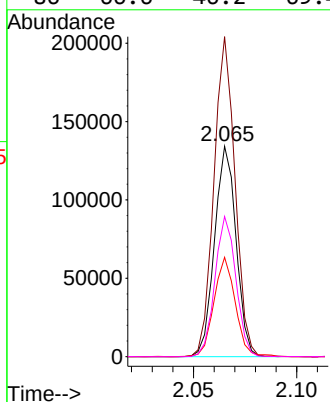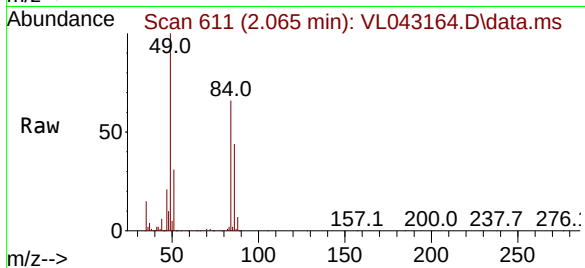

#21

Allyl Chloride

Concen: 0.340 ppbv

RT: 2.081 min Scan# 616

Delta R.T. -0.016 min

Lab File: VL043164.D

Acq: 06 Nov 2025 13:17




Tgt Ion: 41 Resp: 3894


Ion Ratio Lower Upper

41 100

76 0.0 21.5 32.3#

39 181.7 60.8 91.2#



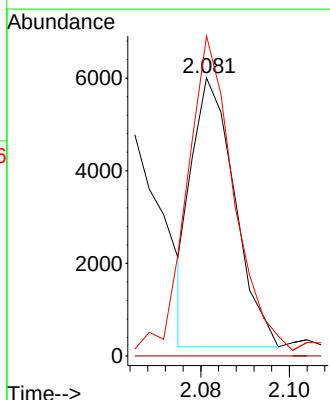
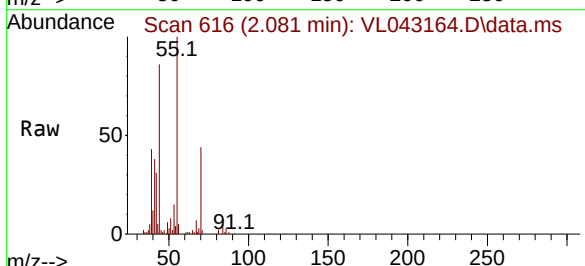




#23
 Vinyl Acetate
 Concen: 1.914 ppbv
 RT: 2.479 min Scan# 71
 Delta R.T. 0.013 min
 Lab File: VL043164.D
 Acq: 06 Nov 2025 13:17




Instrument :
 MSVOA_1
 ClientSampleId :
 141-IA-1


Tgt Ion:	43	Resp:	43597
Ion	Ratio	Lower	Upper
43	100		
86	4.2	6.2	9.2#
42	48.7	7.6	11.4#
44	2.9	4.2	6.4#

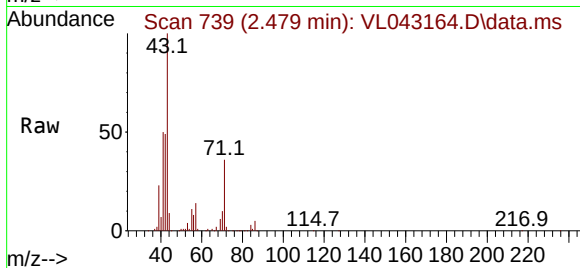

#25
 Ethyl Acetate
 Concen: 2.231 ppbv
 RT: 2.829 min Scan# 847
 Delta R.T. -0.010 min
 Lab File: VL043164.D
 Acq: 06 Nov 2025 13:17

Tgt Ion:	43	Resp:	86024
Ion	Ratio	Lower	Upper
43	100		
45	2.0	7.8	11.8#
61	0.8	7.0	10.6#
70	2.2	6.9	10.3#



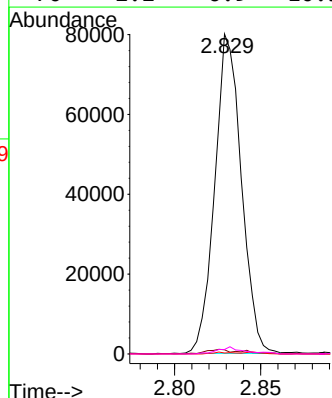
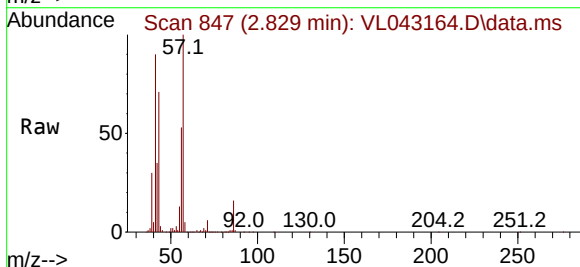




#26
Hexane
Concen: 6.875 ppbv
RT: 2.832 min Scan# 847
Delta R.T. 0.003 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17




Instrument :
MSVOA_L
ClientSampleId :
141-IA-1


Tgt Ion: 57 Resp: 122149
Ion Ratio Lower Upper
57 100
41 90.6 71.4 107.0
43 71.8 178.5 267.7#
56 56.2 42.2 63.4

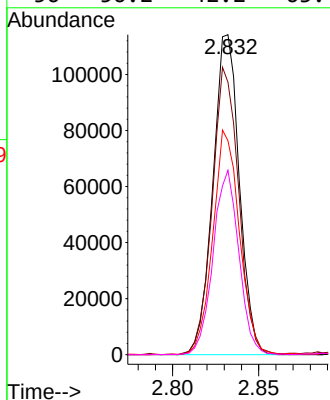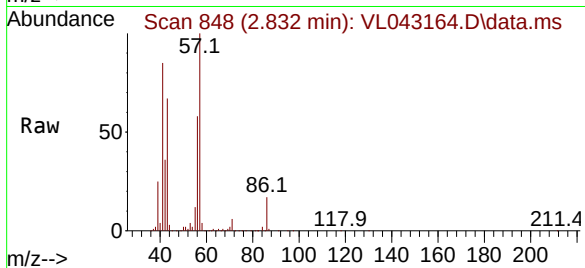

#27
Carbon Disulfide
Concen: 0.031 ppbv
RT: 2.156 min Scan# 639
Delta R.T. 0.003 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17

Tgt Ion: 76 Resp: 508
Ion Ratio Lower Upper
76 100
44 6293.9 16.7 25.1#
78 11.2 9.3 13.9

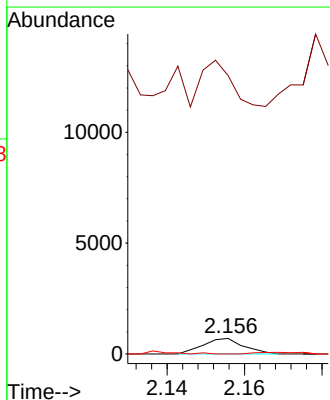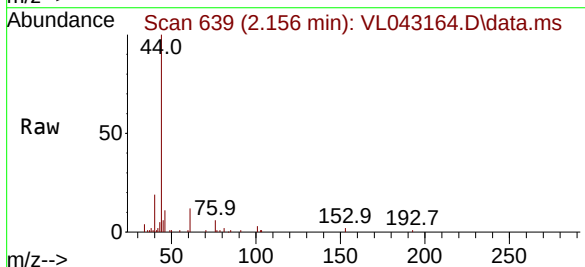



#29

Chloroform

Concen: 0.066 ppbv

RT: 2.852 min Scan# 81

Delta R.T. -0.000 min

Lab File: VL043164.D

Acq: 06 Nov 2025 13:17

Instrument :

MSVOA_L

ClientSampleId :





141-IA-1

Tgt Ion: 83 Resp: 1705

Ion Ratio Lower Upper

83 100

85 84.5 51.8 77.6#

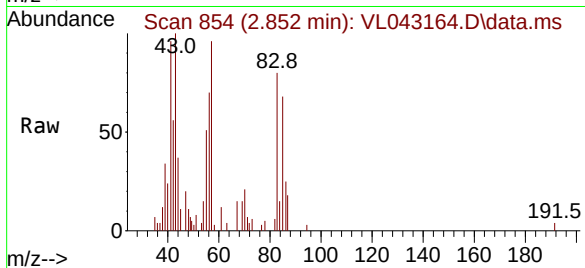

#30

Cyclohexane

Concen: 0.214 ppbv

RT: 3.865 min Scan# 1167

Delta R.T. 0.003 min

Lab File: VL043164.D

Acq: 06 Nov 2025 13:17




Tgt Ion: 84 Resp: 3316


Ion Ratio Lower Upper

84 100

56 140.3 100.9 151.3

41 109.4 63.8 95.6#




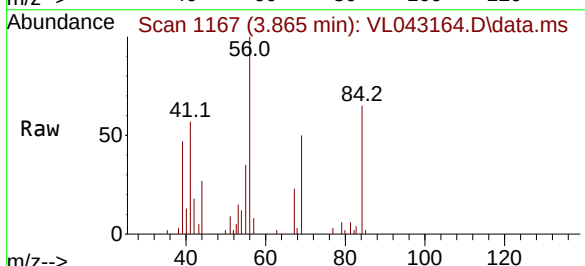




#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 3.962 min Scan# 1197
 Delta R.T. -0.000 min
 Lab File: VL043164.D
 Acq: 06 Nov 2025 13:17




Instrument :
 MSVOA_L
 ClientSampleId :
 141-IA-1


Tgt Ion:114 Resp: 342427
 Ion Ratio Lower Upper
 114 100
 63 25.1 19.3 28.9
 88 17.2 13.9 20.9

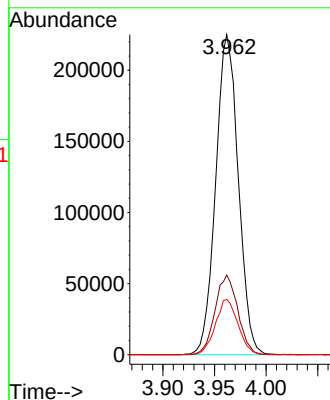

#34
 2-Butanone
 Concen: 1.508 ppbv
 RT: 2.560 min Scan# 764
 Delta R.T. 0.003 min
 Lab File: VL043164.D
 Acq: 06 Nov 2025 13:17

Tgt Ion: 43 Resp: 34716
 Ion Ratio Lower Upper
 43 100
 72 22.4 18.4 27.6



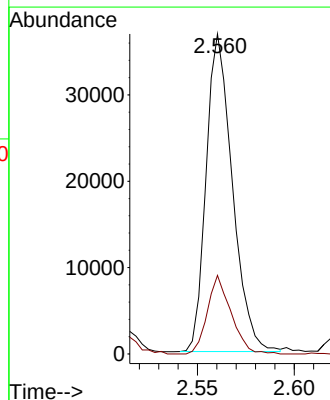
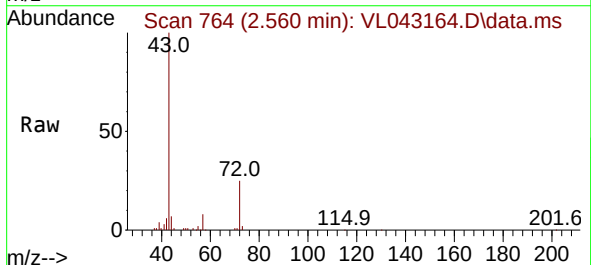




#36
Benzene
Concen: 0.382 ppbv
RT: 3.661 min Scan# 1104
Delta R.T. -0.000 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17




Instrument :
MSVOA_1
ClientSampleId :
141-IA-1


Tgt Ion: 78 Resp: 12305
Ion Ratio Lower Upper
78 100
77 23.2 17.0 25.6
50 18.0 14.6 22.0

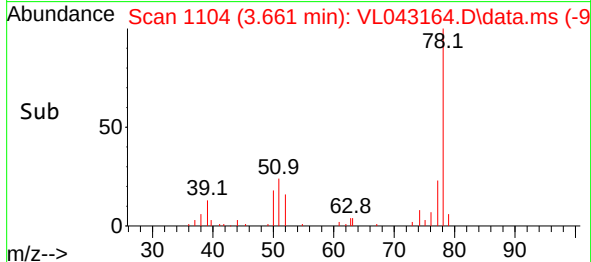

#37
1,2-Dichloroethane
Concen: 0.087 ppbv
RT: 3.224 min Scan# 969
Delta R.T. 0.003 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17

Tgt Ion: 62 Resp: 1623
Ion Ratio Lower Upper
62 100
98 9.3 5.8 8.6

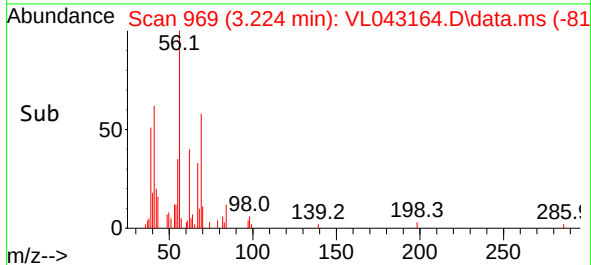



#39

1,2-Dichloropropane

Concen: 7.244 ppbv

RT: 3.962 min Scan# 1197

Delta R.T. -0.353 min

Lab File: VL043164.D

Acq: 06 Nov 2025 13:17

Instrument :

MSVOA_L

ClientSampleId :

141-IA-1





Tgt Ion: 63 Resp: 85408

Ion Ratio Lower Upper

63 100

41 0.0 58.0 87.0#

62 15.2 54.7 82.1#

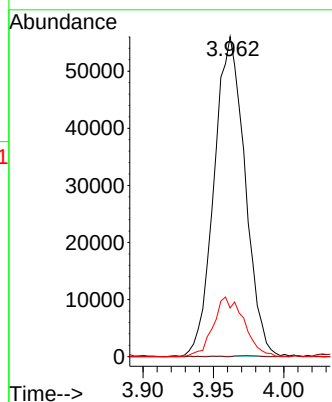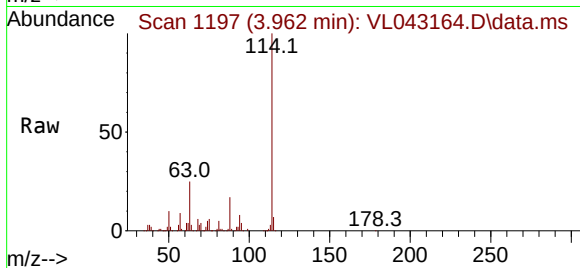

#41

Tetrahydrofuran

Concen: 0.159 ppbv

RT: 3.237 min Scan# 973

Delta R.T. 0.181 min

Lab File: VL043164.D

Acq: 06 Nov 2025 13:17




Tgt Ion: 42 Resp: 2049


Ion Ratio Lower Upper

42 100

72 16.7 31.3 46.9#

71 15.5 30.4 45.6#

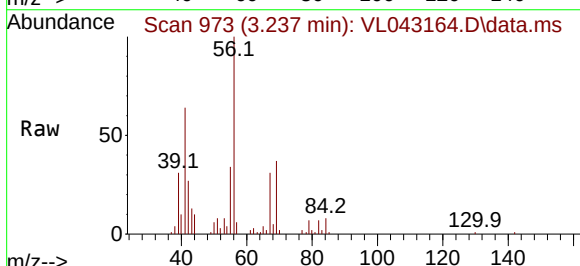



#44

2,2,4-Trimethylpentane

Concen: 0.328 ppbv

RT: 4.641 min Scan# 1408

Delta R.T. -0.004 min

Lab File: VL043164.D

Acq: 06 Nov 2025 13:17

Instrument :

MSVOA_1

ClientSampleId :

141-IA-1





Tgt Ion: 57 Resp: 17870

Ion Ratio Lower Upper

57 100

41 45.5 26.3 39.5#

56 44.3 25.9 38.9#

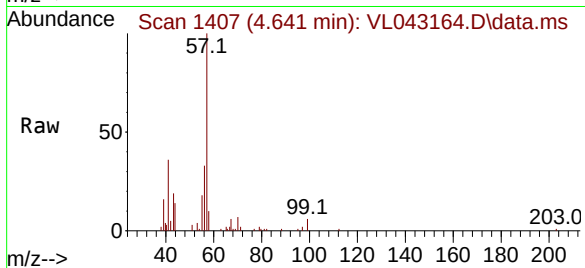

#51

2-Hexanone

Concen: 0.235 ppbv

RT: 7.441 min Scan# 2272

Delta R.T. 0.003 min

Lab File: VL043164.D

Acq: 06 Nov 2025 13:17




Tgt Ion: 43 Resp: 5610


Ion Ratio Lower Upper

43 100

58 83.3 40.4 60.6#

98 0.0 0.1 0.1#


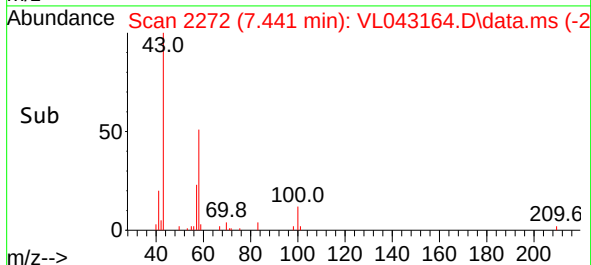
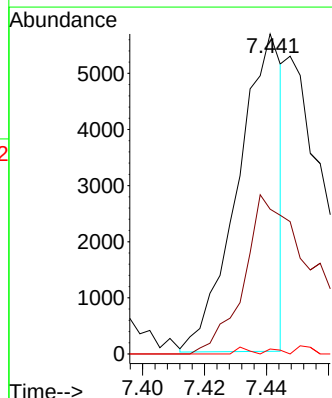
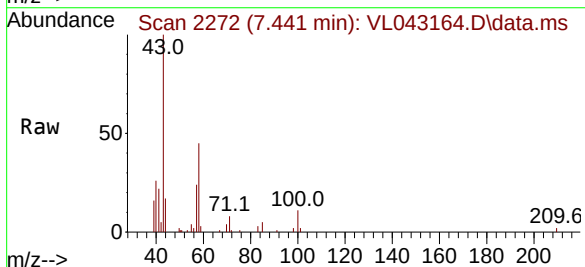




#53
Toluene
Concen: 0.593 ppbv
RT: 6.936 min Scan# 2117
Delta R.T. -0.004 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17




Instrument :
MSVOA_1
ClientSampleId :
141-IA-1


Tgt Ion: 91 Resp: 22705
Ion Ratio Lower Upper
91 100
92 63.0 48.8 73.2



#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.881 min Scan# 2717
Delta R.T. -0.004 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17

Tgt Ion: 117 Resp: 290452
Ion Ratio Lower Upper
117 100
82 66.0 53.8 80.8
119 32.3 25.4 38.0









#58
Ethyl Benzene
Concen: 0.058 ppbv
RT: 9.360 min Scan# 2864
Delta R.T. 0.003 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17




Instrument :
MSVOA_1
ClientSampleId :
141-IA-1


Tgt Ion: 91 Resp: 2883
Ion Ratio Lower Upper
91 100
106 27.8 24.8 37.2



#59
m/p-Xylene
Concen: 0.385 ppbv
RT: 9.535 min Scan# 2919
Delta R.T. -0.000 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17

Tgt Ion: 91 Resp: 15295
Ion Ratio Lower Upper
91 100
106 46.5 38.0 57.0









#60
o-Xylene
Concen: 0.147 ppbv
RT: 9.969 min Scan# 3053
Delta R.T. -0.000 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17




Instrument :
MSVOA_1
ClientSampleId :
141-IA-1


Tgt Ion: 91 Resp: 5758
Ion Ratio Lower Upper
91 100
106 39.8 21.9 65.8

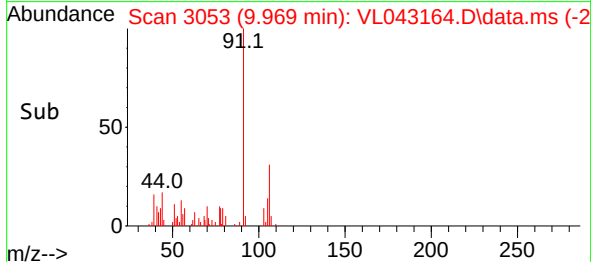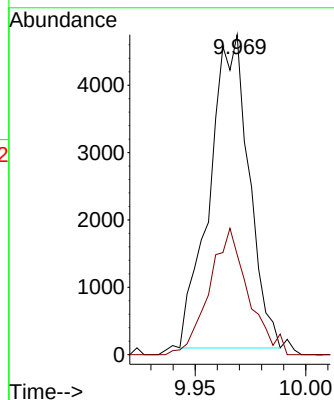

#68
1-Bromo-4-Fluorobenzene
Concen: 10.513 ppbv
RT: 10.377 min Scan# 3179
Delta R.T. -0.004 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17

Tgt Ion: 95 Resp: 237353
Ion Ratio Lower Upper
95 100
174 63.7 48.3 72.5
175 4.6 3.8 5.8



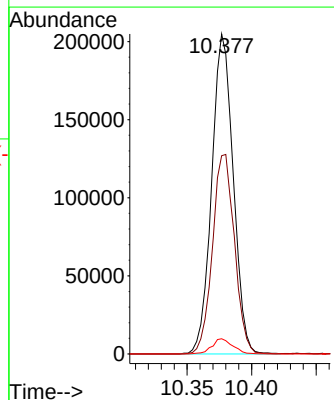
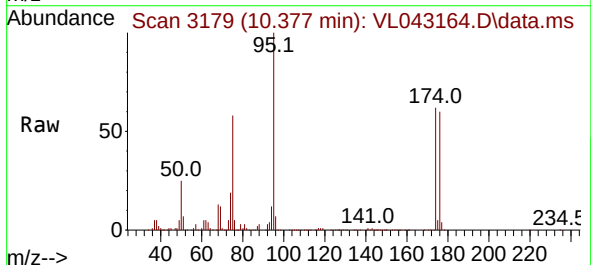




#73
1,3,5-Trimethylbenzene
Concen: 0.043 ppbv
RT: 11.209 min Scan# 3436
Delta R.T. 0.003 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17




Instrument :
MSVOA_L
ClientSampleId :
141-IA-1


Tgt Ion:105 Resp: 1713
Ion Ratio Lower Upper
105 100
120 35.9 39.0 58.6#

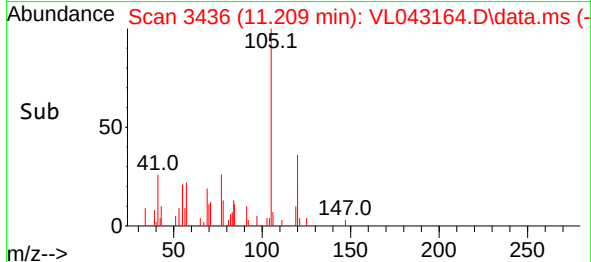

#74
1,2,4-Trimethylbenzene
Concen: 0.129 ppbv
RT: 11.539 min Scan# 3538
Delta R.T. -0.000 min
Lab File: VL043164.D
Acq: 06 Nov 2025 13:17

Tgt Ion:105 Resp: 5751
Ion Ratio Lower Upper
105 100
120 47.4 42.8 64.2
91 15.3 68.3 102.5#
77 19.7 23.4 35.0#

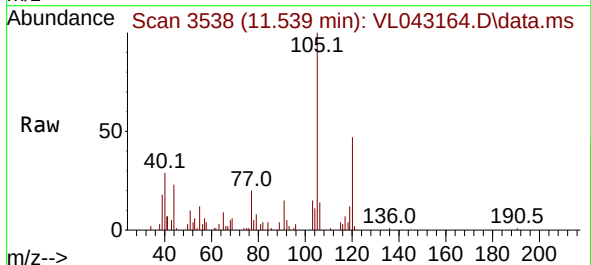



#79

Naphthalene

Concen: 0.130 ppbv

RT: 13.516 min Scan# 41

Delta R.T. -0.000 min

Lab File: VL043164.D


Acq: 06 Nov 2025 13:17

Instrument :

MSVOA_L

ClientSampleId :

141-IA-1



Tgt Ion:128 Resp: 6044

Ion Ratio Lower Upper

128 100

127 13.3 10.5 15.7

129 12.2 9.1 13.7

