
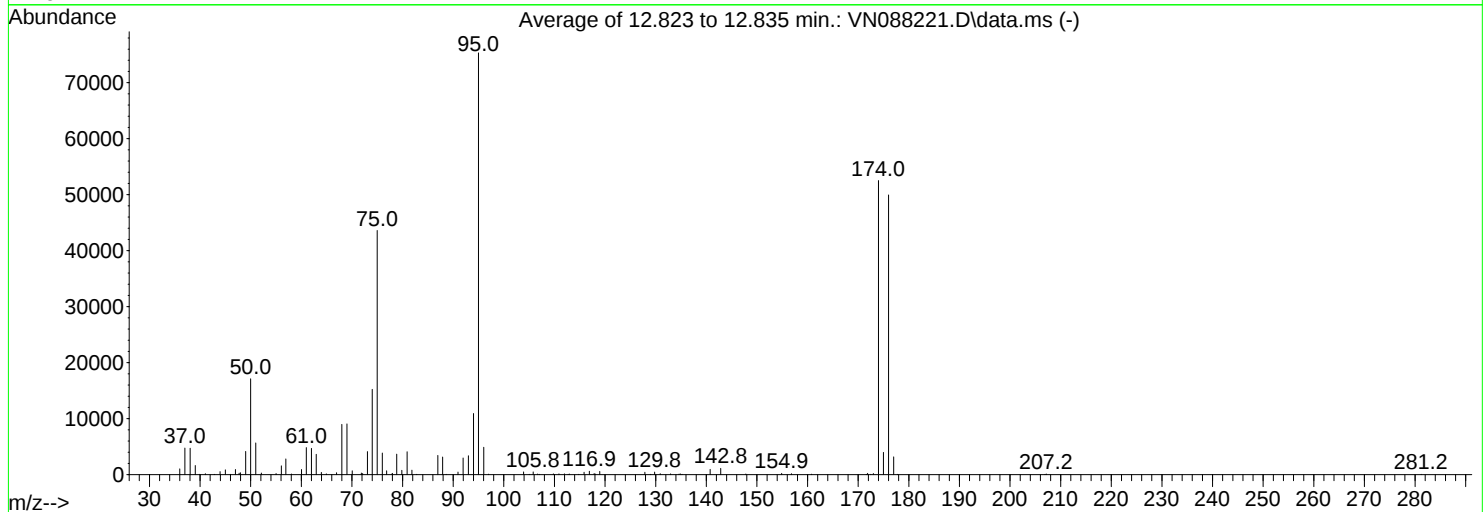


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110725\
Data File : VN088221.D
Acq On : 07 Nov 2025 09:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Title : SW846 8260
Last Update : Mon Nov 03 01:16:06 2025

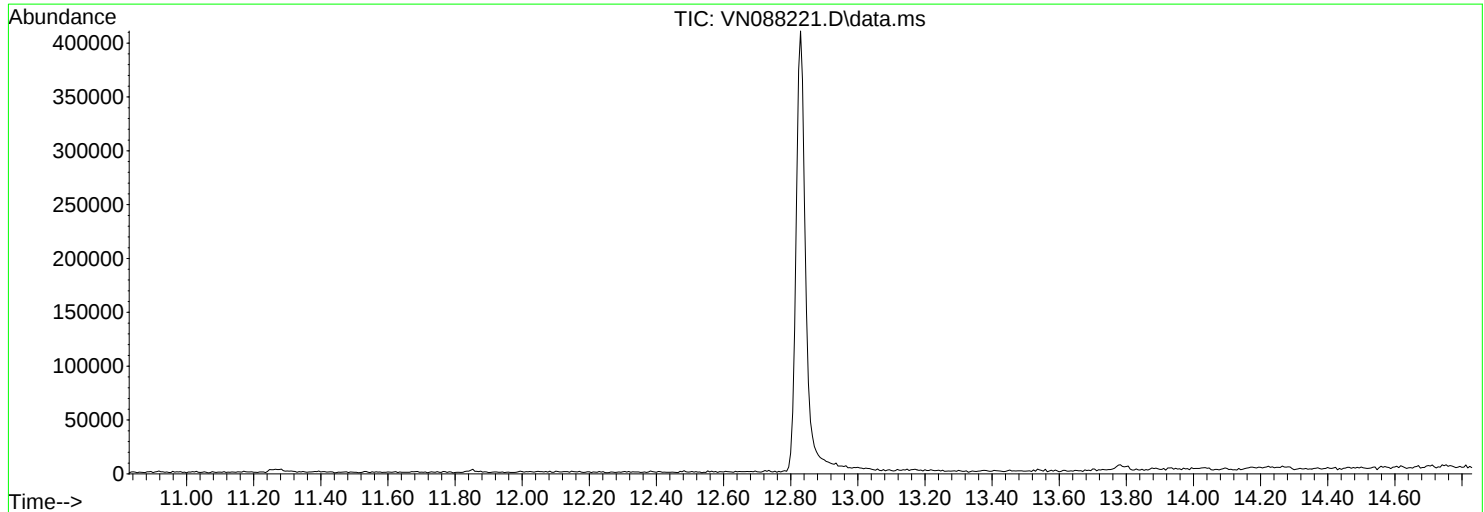

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1838

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.7	17120	PASS
75	95	30	60	57.9	43603	PASS
95	95	100	100	100.0	75336	PASS
96	95	5	9	6.5	4877	PASS
173	174	0.00	2	0.4	205	PASS
174	95	50	100	69.7	52515	PASS
175	174	5	9	7.6	3980	PASS
176	174	95	101	95.1	49944	PASS
177	176	5	9	6.4	3178	PASS

Average of 12.823 to 12.835 min.: VN088221.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	1042	47.70	263	61.00	4835	73.05	410
37.00	4745	47.95	347	62.00	4702	74.00	1523
38.05	4712	49.00	4138	62.95	3616	75.00	4360
39.05	1646	50.00	17120	63.95	399	76.00	387
39.95	68	51.00	5674	64.95	144	76.85	677
41.05	180	52.10	295	66.95	334	77.90	115
42.80	65	55.00	200	68.00	8969	78.00	239
43.95	545	56.05	1579	69.00	9075	78.85	3652
45.00	850	56.95	2808	70.05	685	79.85	772
46.00	69	58.05	126	71.85	289	80.90	4087
47.00	917	60.05	909	72.10	204	81.85	809

Average of 12.823 to 12.835 min.: VN088221.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
82.80	52	103.90	479	115.85	430	134.85	138
86.95	3421	105.00	56	116.90	599	135.20	62
87.90	3133	105.80	480	117.85	209	140.75	946
88.60	67	106.70	129	118.05	128	142.85	1123
90.95	467	107.00	61	118.95	565	147.80	122
91.95	2976	109.80	144	127.85	426	154.90	235
93.00	3375	110.90	148	129.00	74	156.80	164
94.00	10922	111.95	136	129.80	463	160.80	83
95.00	75336	112.70	50	130.90	167	171.60	65
96.05	4877	112.95	118	132.95	132	171.85	225
97.00	79	114.80	54	134.60	87	172.50	62

Average of 12.823 to 12.835 min.: VN088221.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.00	205						
174.00	52515						
175.00	3980						
176.00	49944						
177.00	3178						
177.80	53						
206.90	68						
207.15	126						
281.20	62						

Instrument :

MSVOA_N

ClientSampleId :

BFB