

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110725\
 Data File : VN088224.D
 Acq On : 07 Nov 2025 11:00
 Operator : JC\MD
 Sample : VN1107WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1107WBL01

Quant Time: Nov 08 01:53:44 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 03 01:16:06 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	218414	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.082	114	497944	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.847	117	470093	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	225246	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	228861	60.596	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	121.200%
35) Dibromofluoromethane	8.147	113	174482	52.159	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.320%
50) Toluene-d8	10.541	98	638940	49.570	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.140%
62) 4-Bromofluorobenzene	12.829	95	244496	53.710	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	107.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110725\
Data File : VN088224.D
Acq On : 07 Nov 2025 11:00
Operator : JC\MD
Sample : VN1107WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1107WBL01

Quant Time: Nov 08 01:53:44 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Quant Title : SW846 8260
QLast Update : Mon Nov 03 01:16:06 2025
Response via : Initial Calibration




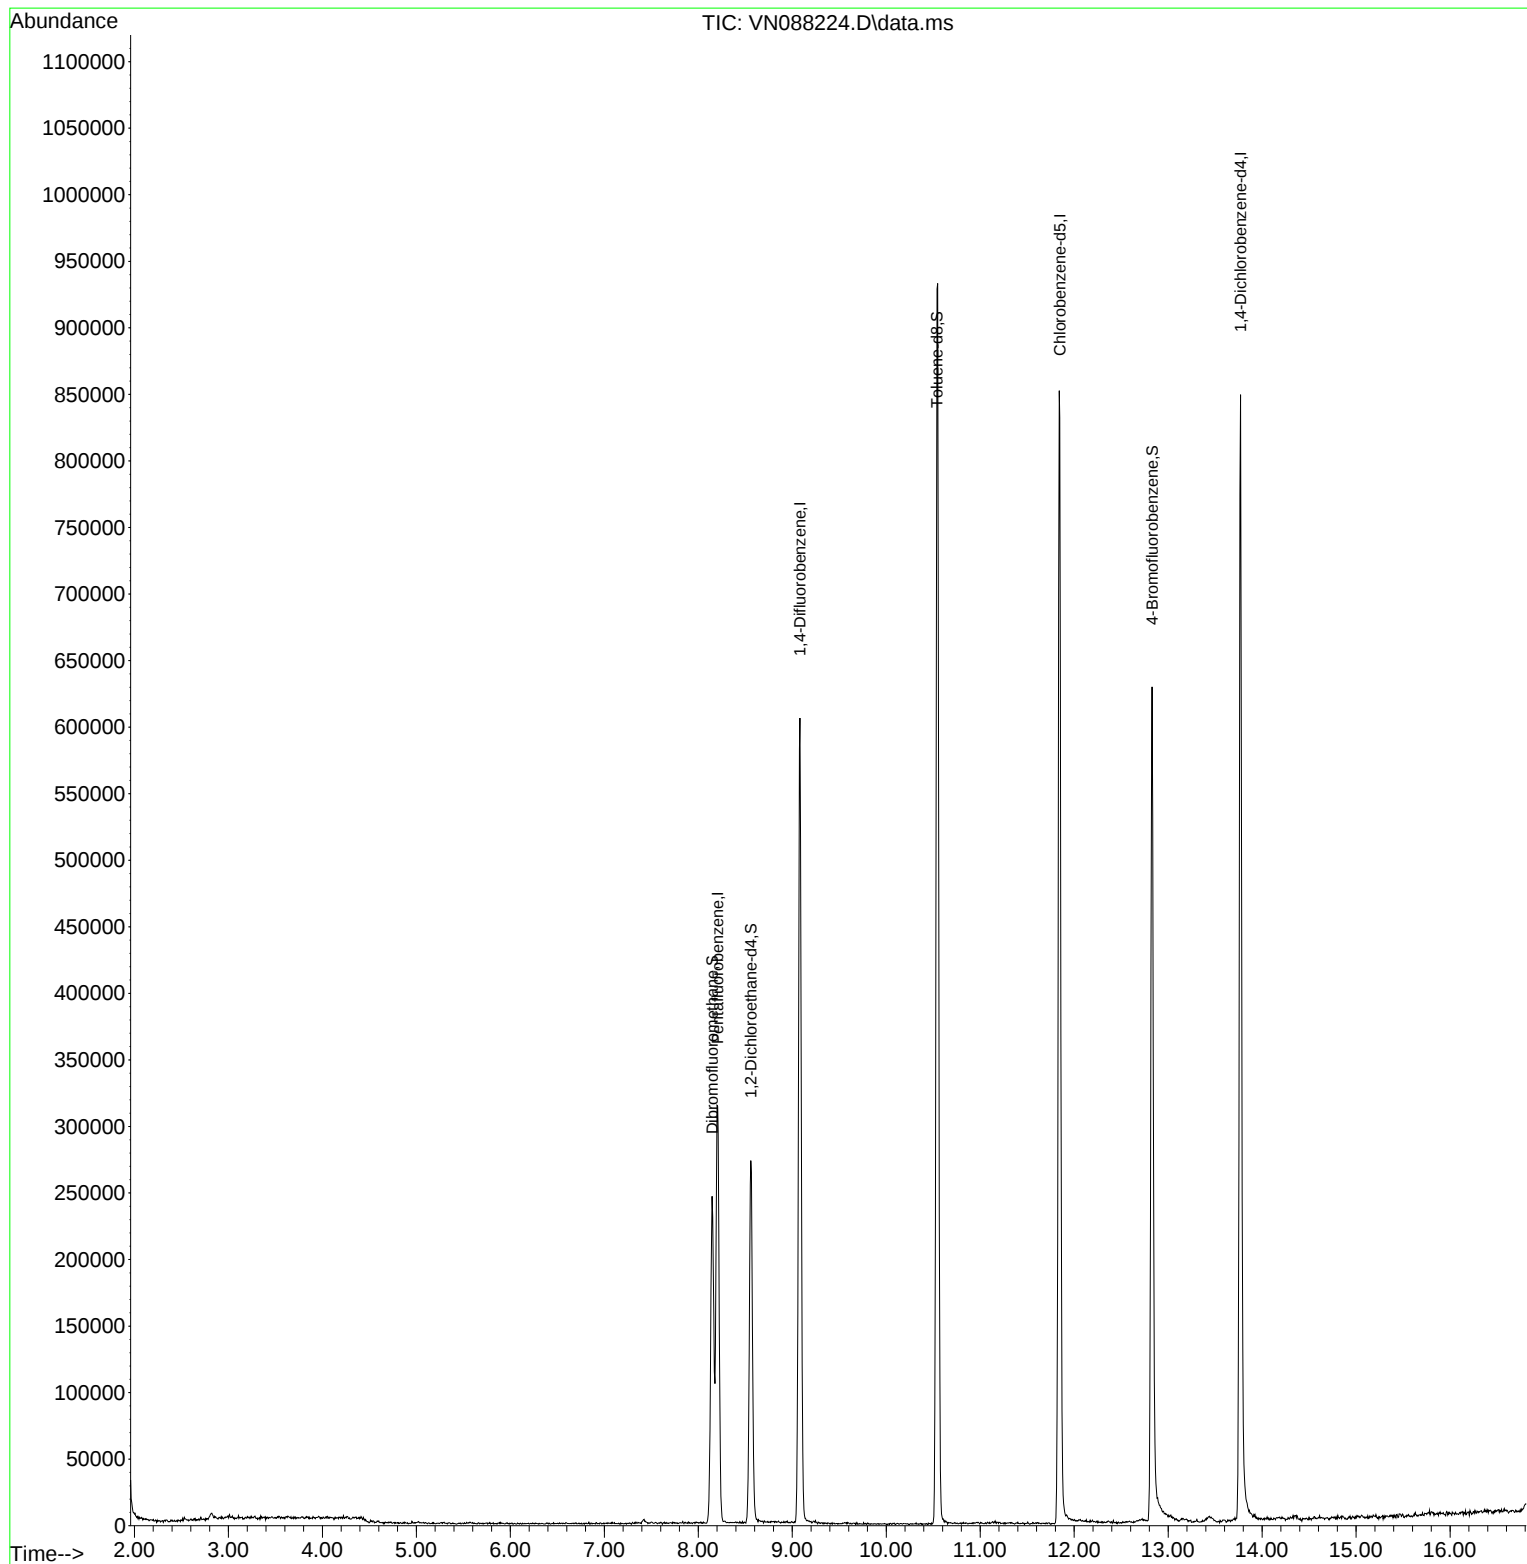


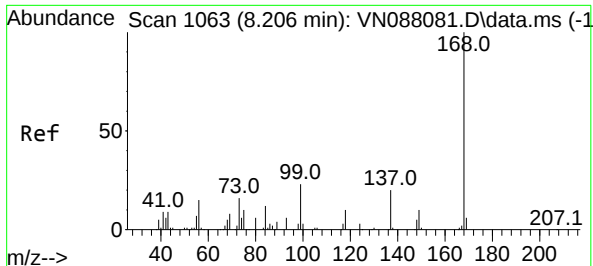

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1063
Delta R.T. -0.000 min
Lab File: VN088224.D
Acq: 07 Nov 2025 11:00




Instrument :
MSVOA_N
ClientSampleId :
VN1107WBL01


Tgt Ion:168 Resp: 218414
Ion Ratio Lower Upper
168 100
99 70.5 57.2 85.8

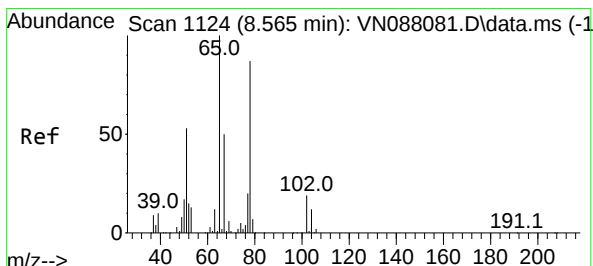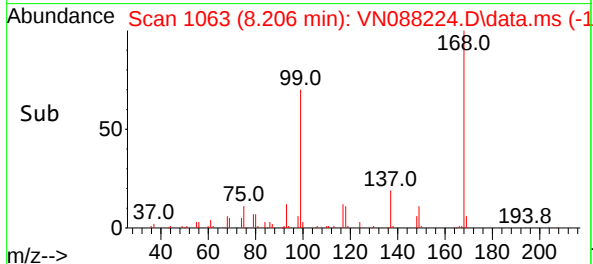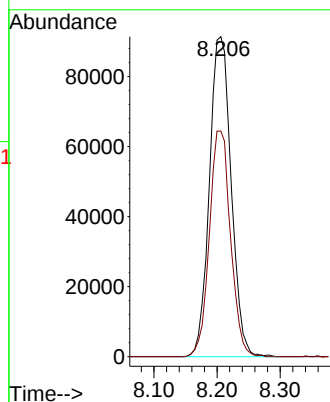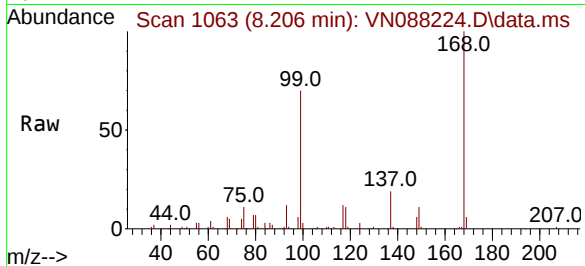

#33
1,2-Dichloroethane-d4
Concen: 60.596 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. -0.000 min
Lab File: VN088224.D
Acq: 07 Nov 2025 11:00

Tgt Ion: 65 Resp: 228861
Ion Ratio Lower Upper
65 100
67 50.6 0.0 100.0

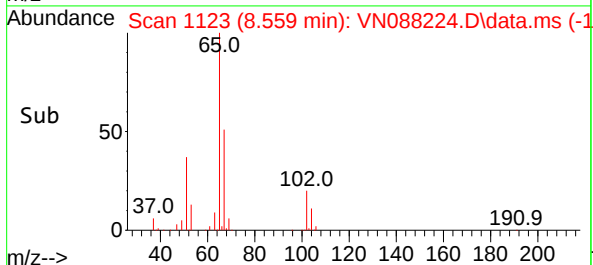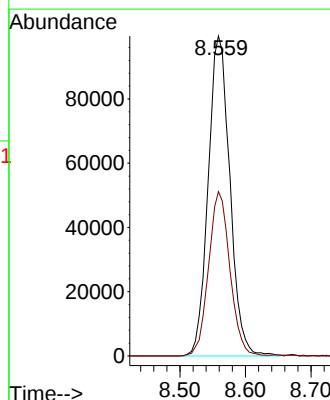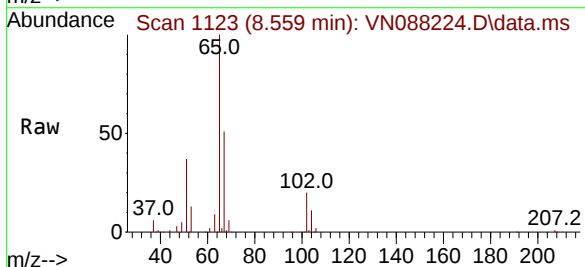

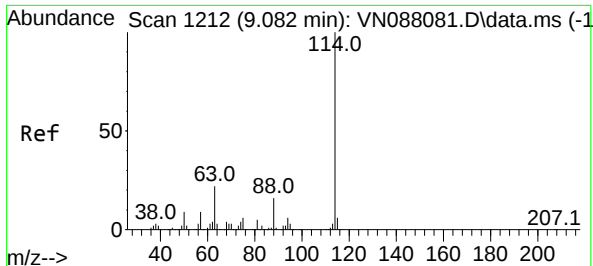

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.082 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN088224.D

Acq: 07 Nov 2025 11:00

Instrument :

MSVOA_N

ClientSampleId :

VN1107WBL01





Tgt Ion:114 Resp: 497944

Ion Ratio Lower Upper

114 100

63 22.2 0.0 45.2

88 17.3 0.0 33.4

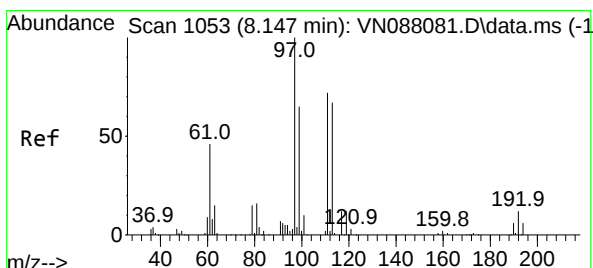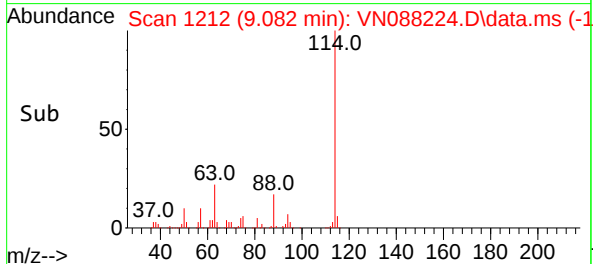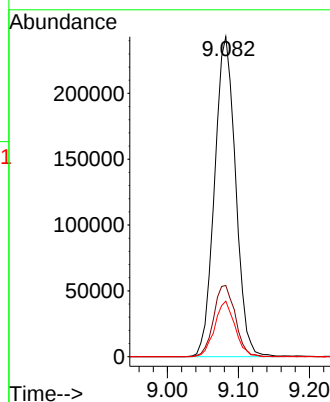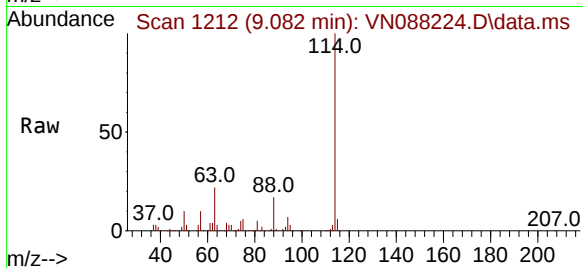

#35

Dibromofluoromethane

Concen: 52.159 ug/l

RT: 8.147 min Scan# 1053

Delta R.T. -0.006 min

Lab File: VN088224.D

Acq: 07 Nov 2025 11:00




Tgt Ion:113 Resp: 174482


Ion Ratio Lower Upper

113 100

111 101.7 82.8 124.2

192 16.2 12.8 19.2


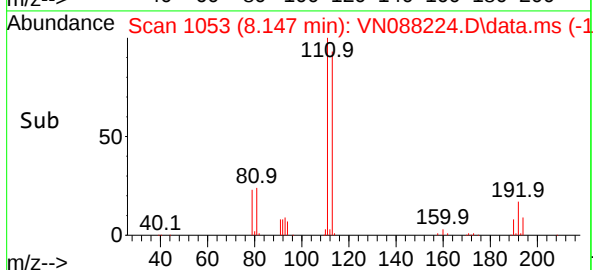
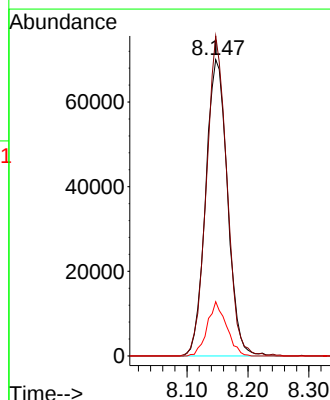
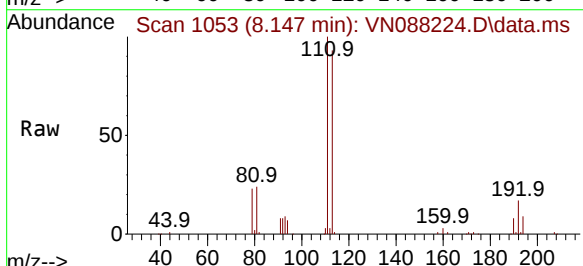


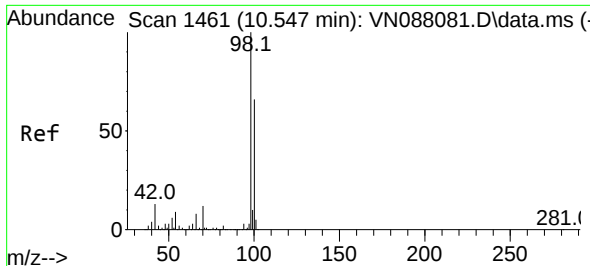

#50
Toluene-d8
Concen: 49.570 ug/l
RT: 10.541 min Scan# 1460
Delta R.T. -0.006 min
Lab File: VN088224.D
Acq: 07 Nov 2025 11:00




Instrument :
MSVOA_N
ClientSampleId :
VN1107WBL01


Tgt Ion: 98 Resp: 638940
Ion Ratio Lower Upper
98 100
100 64.9 52.8 79.2

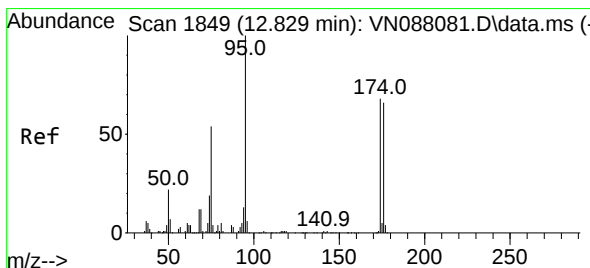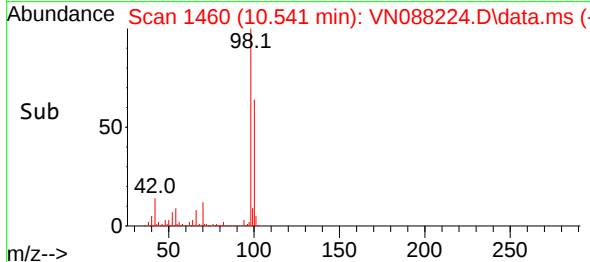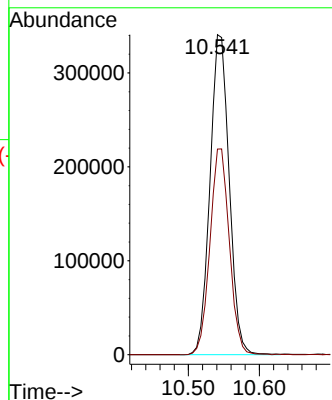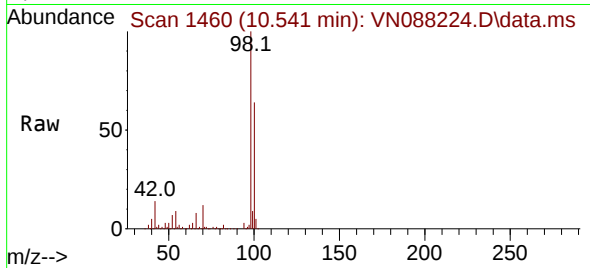

#62
4-Bromofluorobenzene
Concen: 53.710 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN088224.D
Acq: 07 Nov 2025 11:00

Tgt Ion: 95 Resp: 244496
Ion Ratio Lower Upper
95 100
174 69.1 0.0 138.4
176 64.1 0.0 132.6


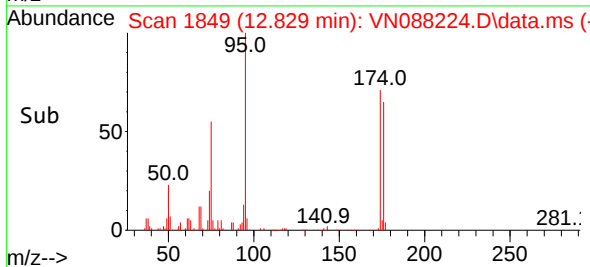
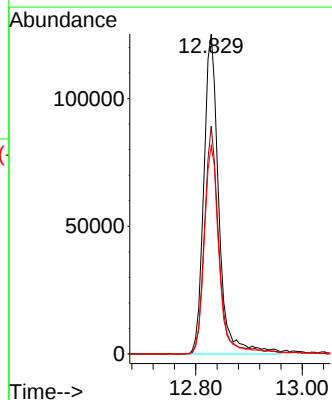
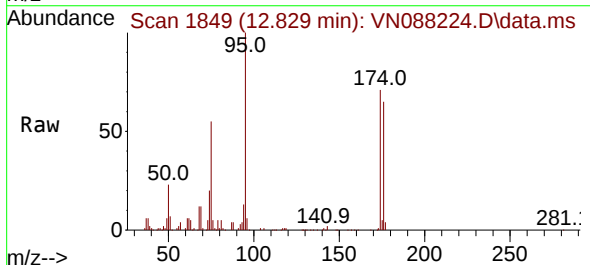


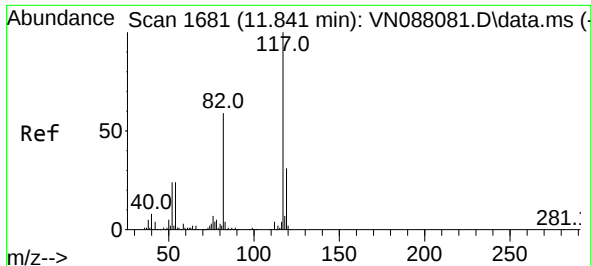

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.847 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN088224.D
Acq: 07 Nov 2025 11:00

Instrument :
MSVOA_N
ClientSampleId :
VN1107WBL01

Tgt Ion:117 Resp: 470093
Ion Ratio Lower Upper
117 100
82 58.5 47.4 71.2
119 30.7 24.3 36.5

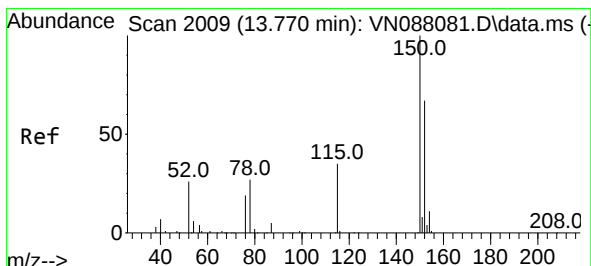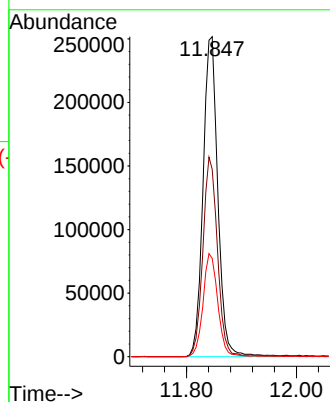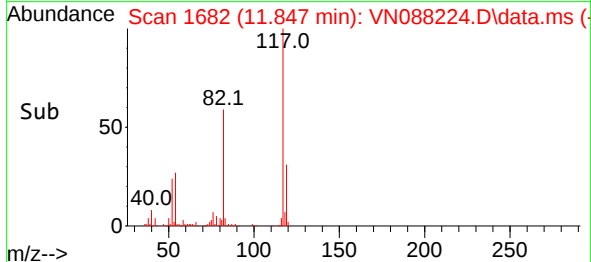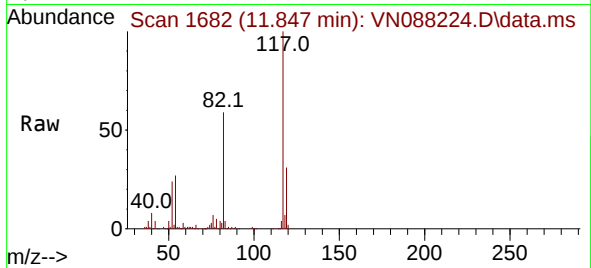

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.006 min
Lab File: VN088224.D
Acq: 07 Nov 2025 11:00

Tgt Ion:152 Resp: 225246
Ion Ratio Lower Upper
152 100
115 64.5 32.3 96.8
150 155.9 0.0 351.0

