


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110525\
Data File : BF144168.D
Acq On : 05 Nov 2025 12:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

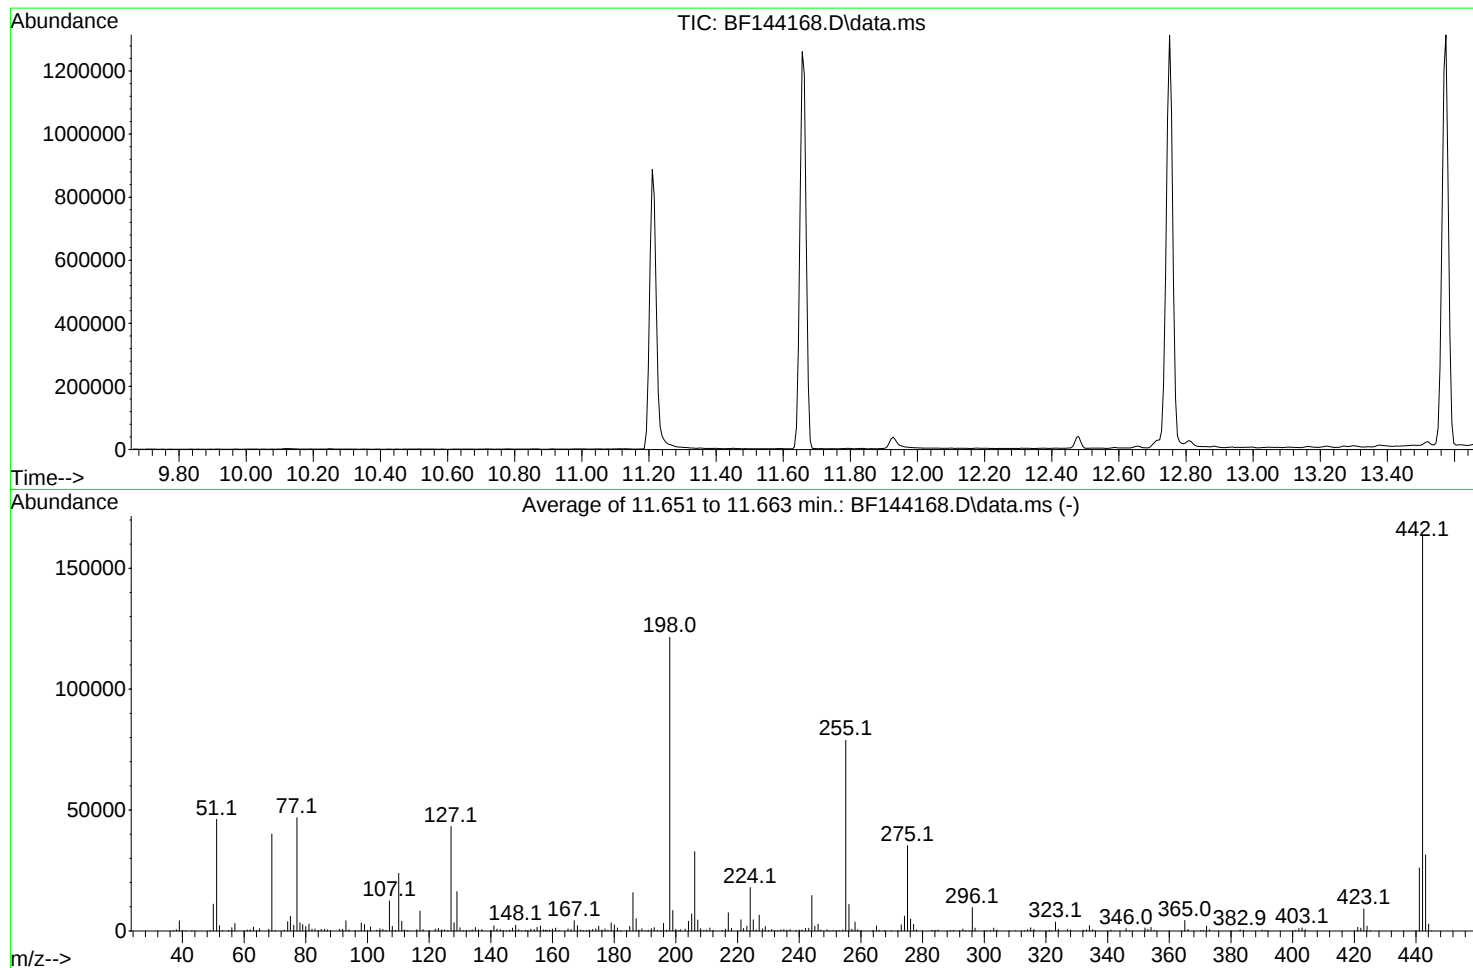




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	709	PASS
69	69	100	100	100.0	40048	PASS
70	69	0.00	2	0.6	222	PASS
197	198	0.00	2	0.3	378	PASS
198	198	100	100	100.0	121493	PASS
199	198	5	9	6.9	8441	PASS
365	198	1	100	3.6	4315	PASS
441	443	0.01	150	82.6	26027	PASS
442	442	100	100	100.0	163299	PASS
443	442	15	24	19.3	31501	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110525\
Data File : BF144168.D
Acq On : 05 Nov 2025 12:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 05 15:24:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 15:17:46 2025
Response via : Initial Calibration

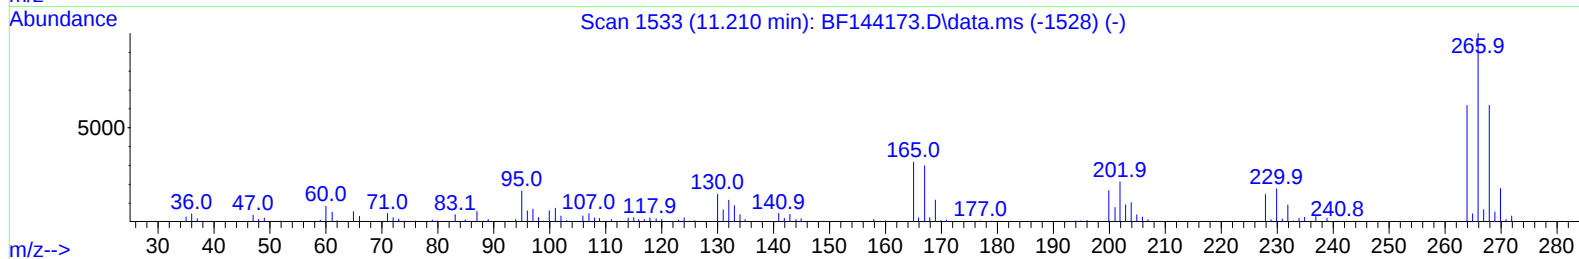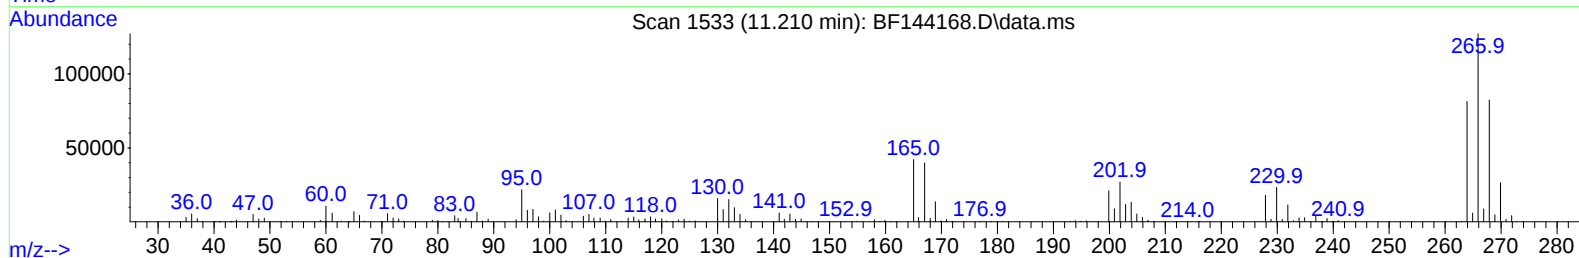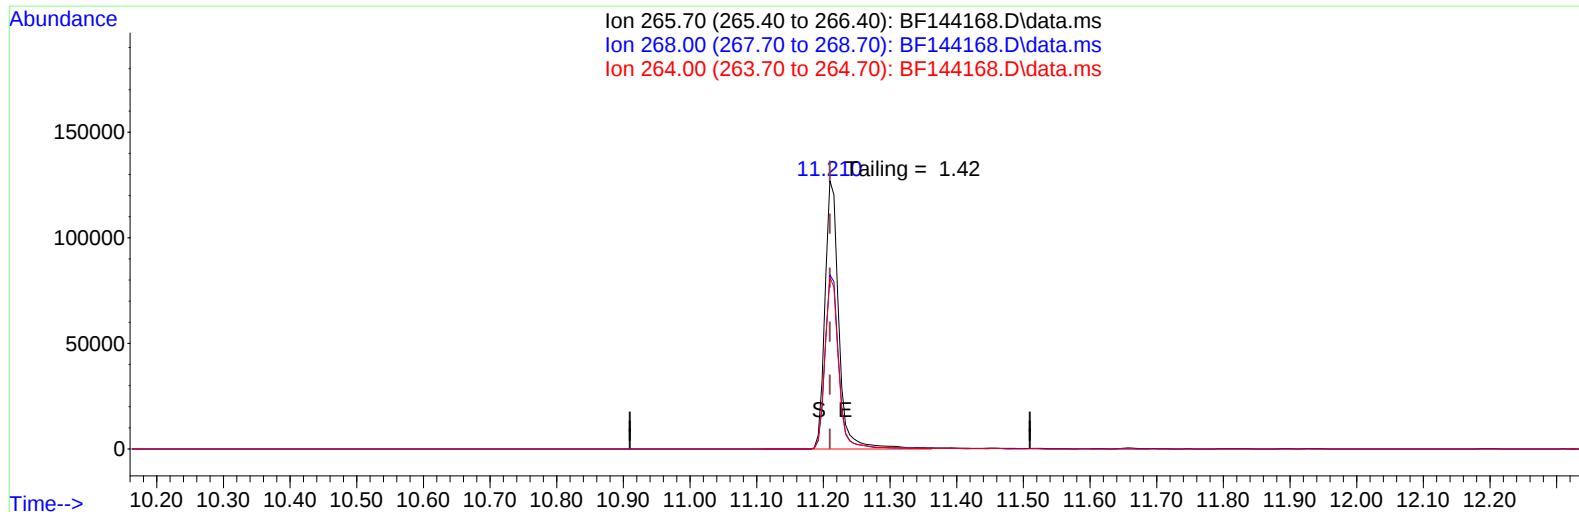

TIC: BF144168.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 39632.00 ng


response 182948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	64.79
264.00	61.80	64.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110525\
Data File : BF144168.D
Acq On : 05 Nov 2025 12:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 05 15:24:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 15:17:46 2025
Response via : Initial Calibration

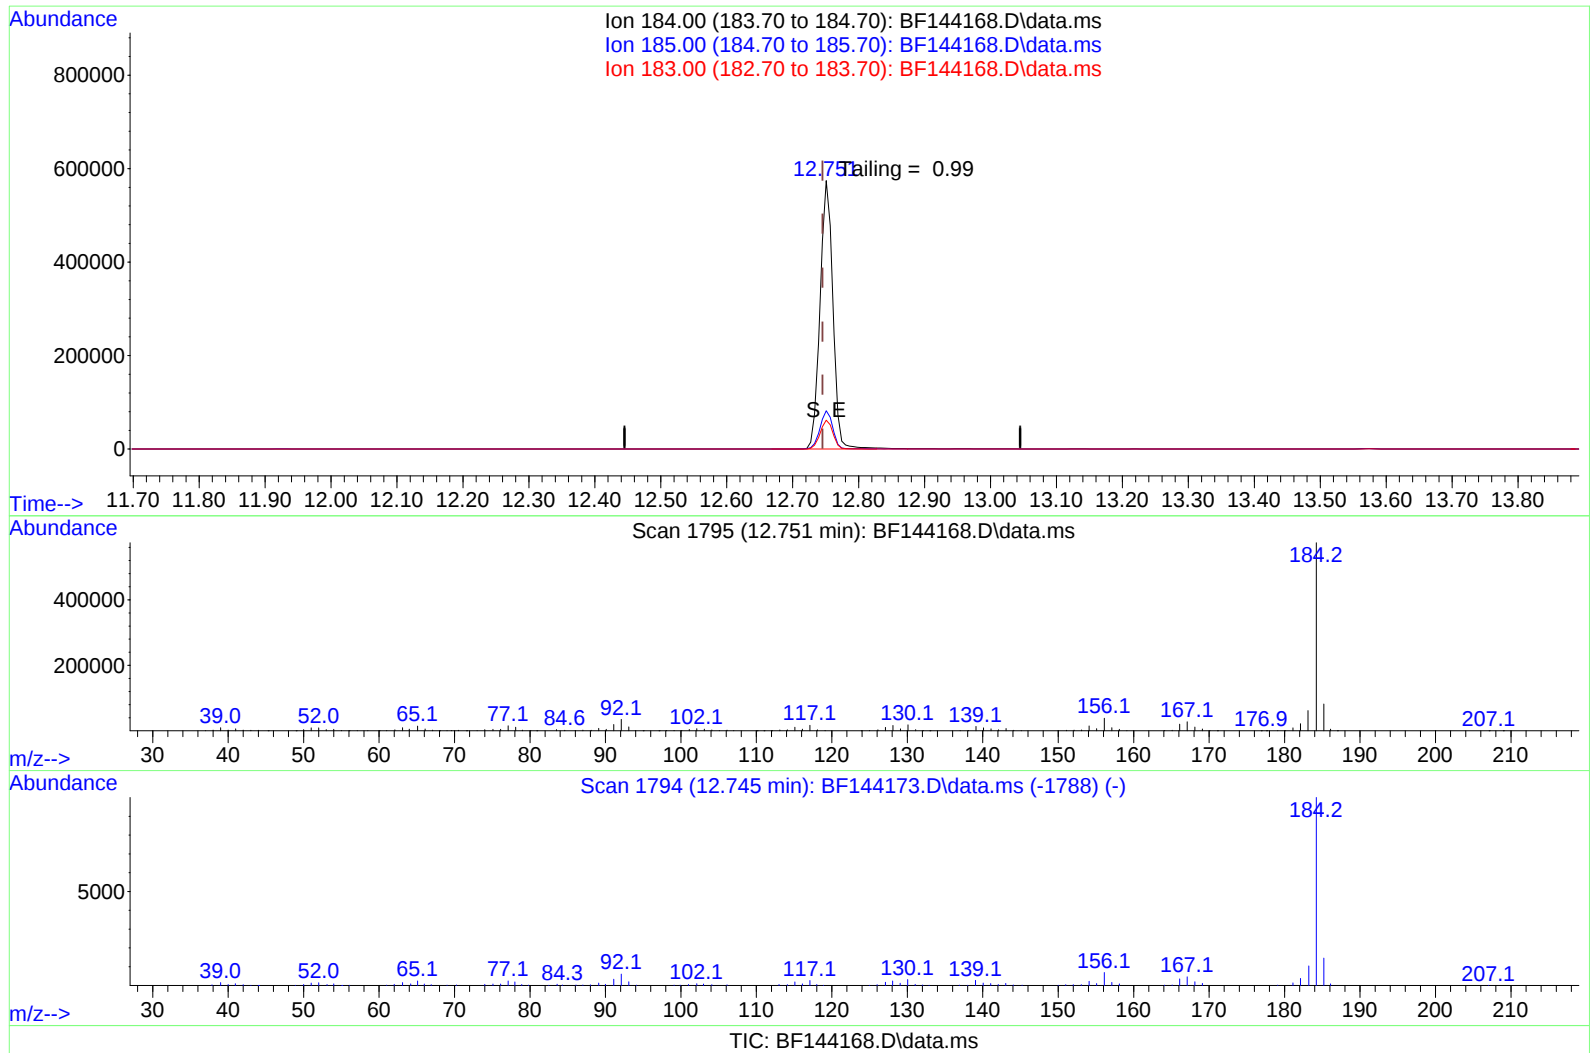

(77) Benzidine


12.751min (+ 0.006) 0.00 ng

response 777212

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.24
183.00	10.40	10.75
0.00	0.00	0.00

Hexachlorocyclopentadiene

Response Ratio

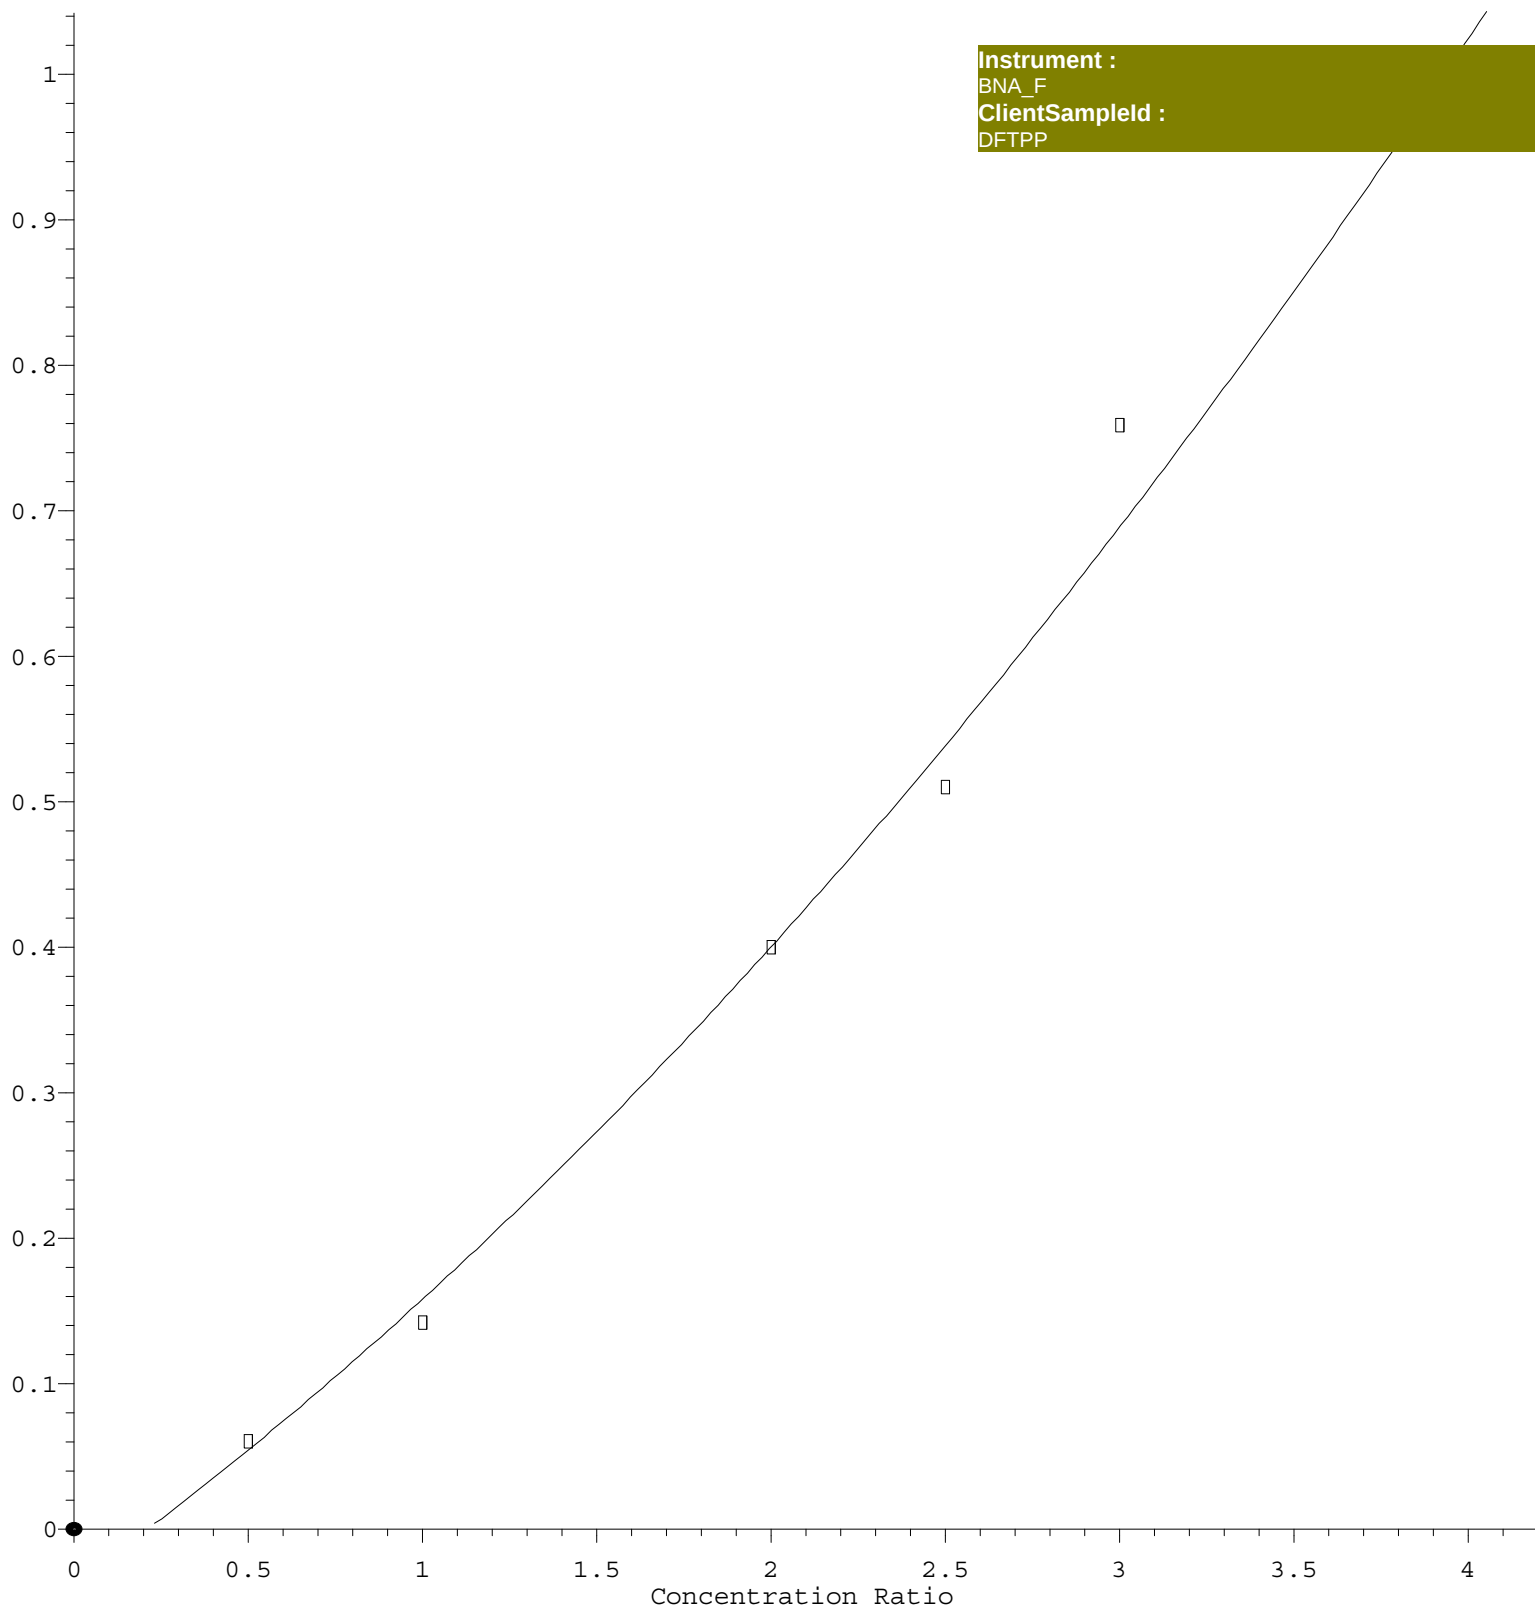

$R = 2.331e-002 A^2 + 1.722e-001 A - 3.751e-002$
Coef of Det (r^2) = 0.992660 Curve Fit: Quadratic w(1/a)
Method Name: Z:\svoasrv\HPCHEM1\BNA F\Methods\8270-BF110525.M
Calibration Table Last Updated: Wed Nov 05 18:37:33 2025