
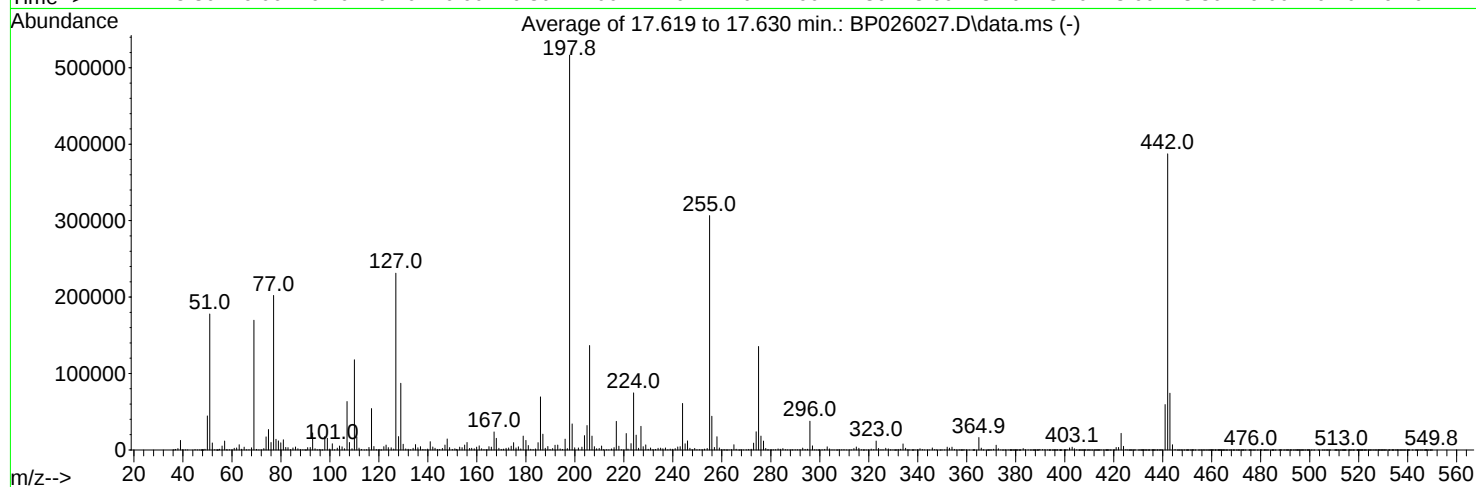


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102925\
Data File : BP026027.D
Acq On : 29 Oct 2025 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 30 11:51:34 2025

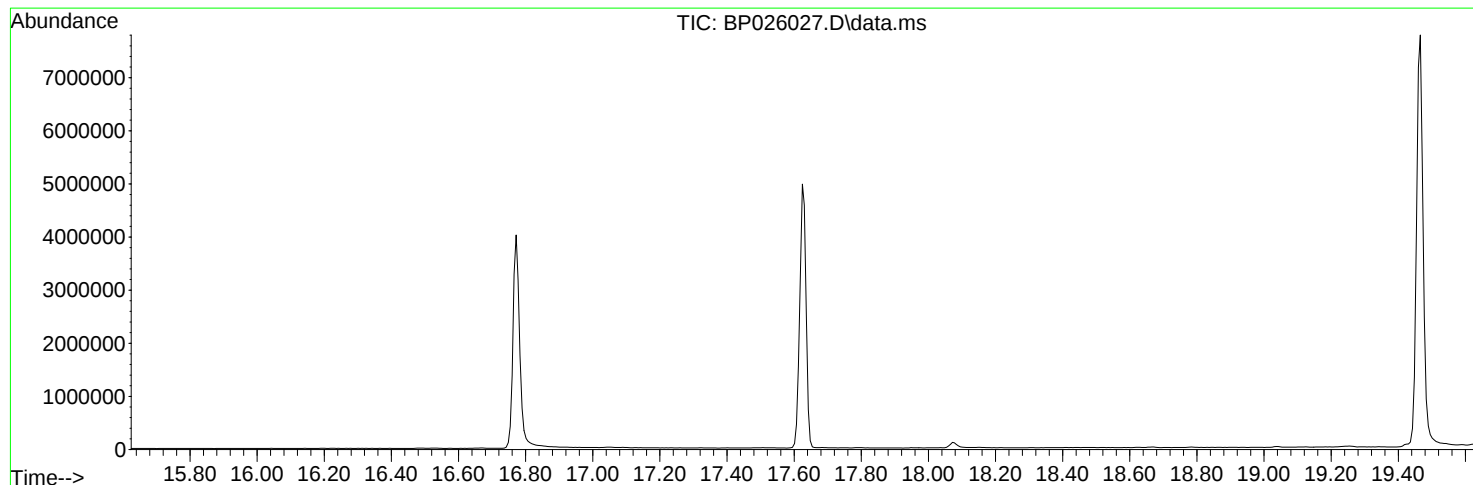




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2484

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	2792	PASS
69	69	100	100	100.0	169765	PASS
70	69	0.00	2	0.4	752	PASS
197	198	0.00	2	0.4	1827	PASS
198	198	100	100	100.0	516572	PASS
199	198	5	9	6.6	34035	PASS
365	198	1	100	3.1	16180	PASS
441	443	0.01	150	79.9	59342	PASS
442	442	100	100	100.0	387348	PASS
443	442	15	24	19.2	74271	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102925\
Data File : BP026027.D
Acq On : 29 Oct 2025 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 29 15:04:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 29 15:02:40 2025
Response via : Initial Calibration

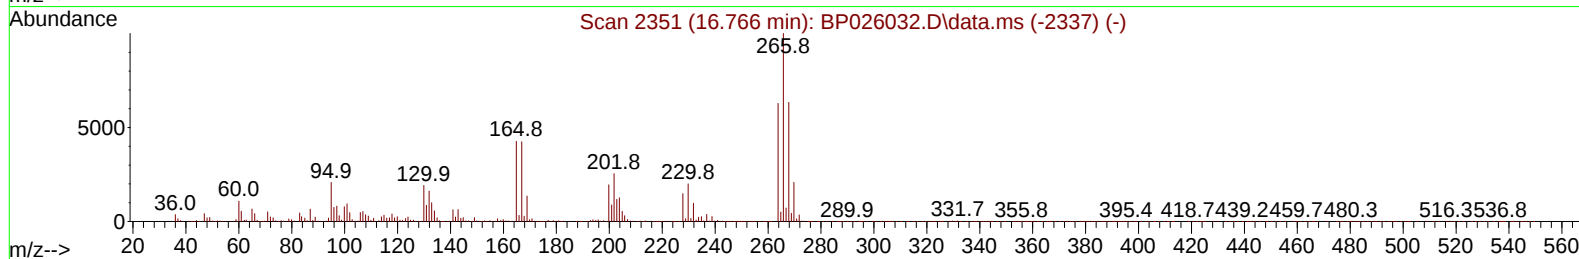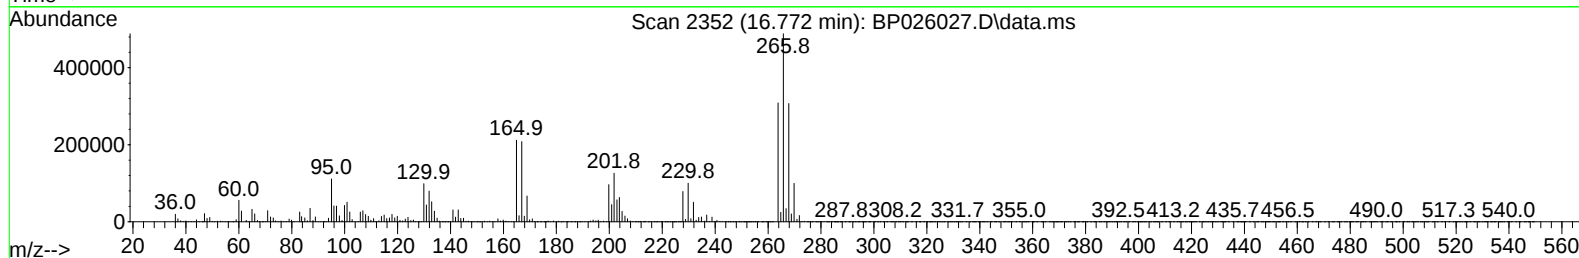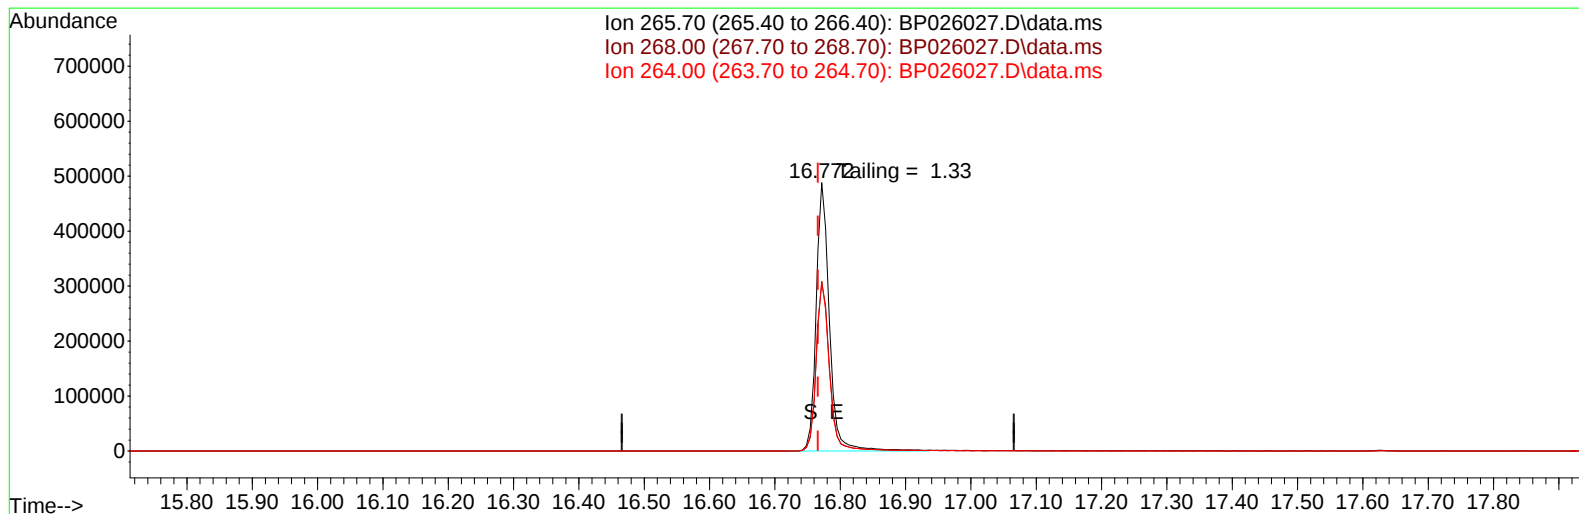

TIC: BP026027.D\data.ms

(70) Pentachlorophenol (C)

16.772min (+ 0.006) 52866.47 ng




response 688723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.93
264.00	62.80	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102925\
Data File : BP026027.D
Acq On : 29 Oct 2025 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 29 15:04:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 29 15:02:40 2025
Response via : Initial Calibration

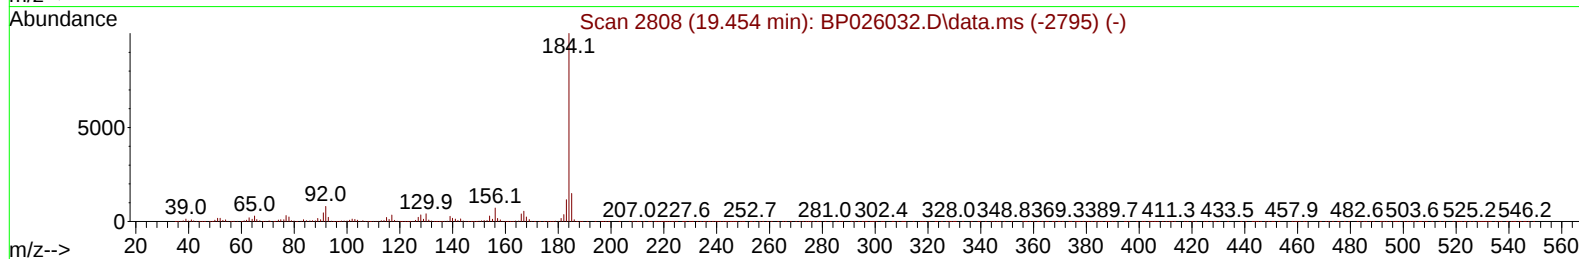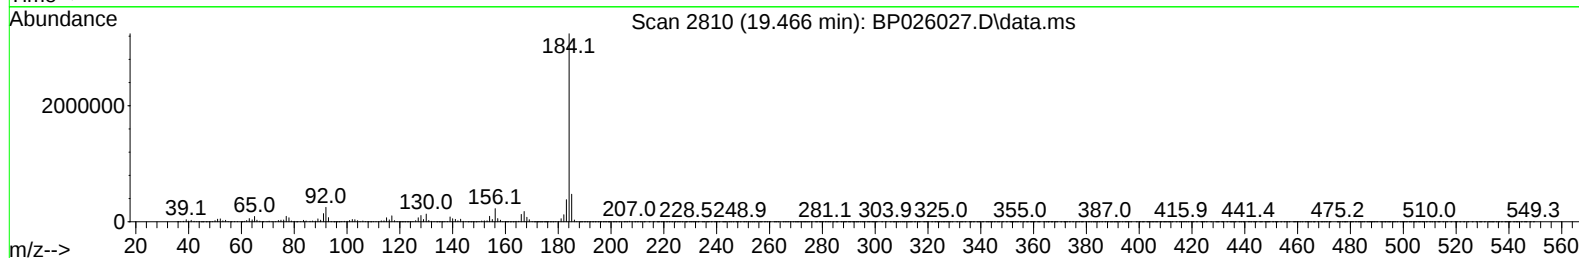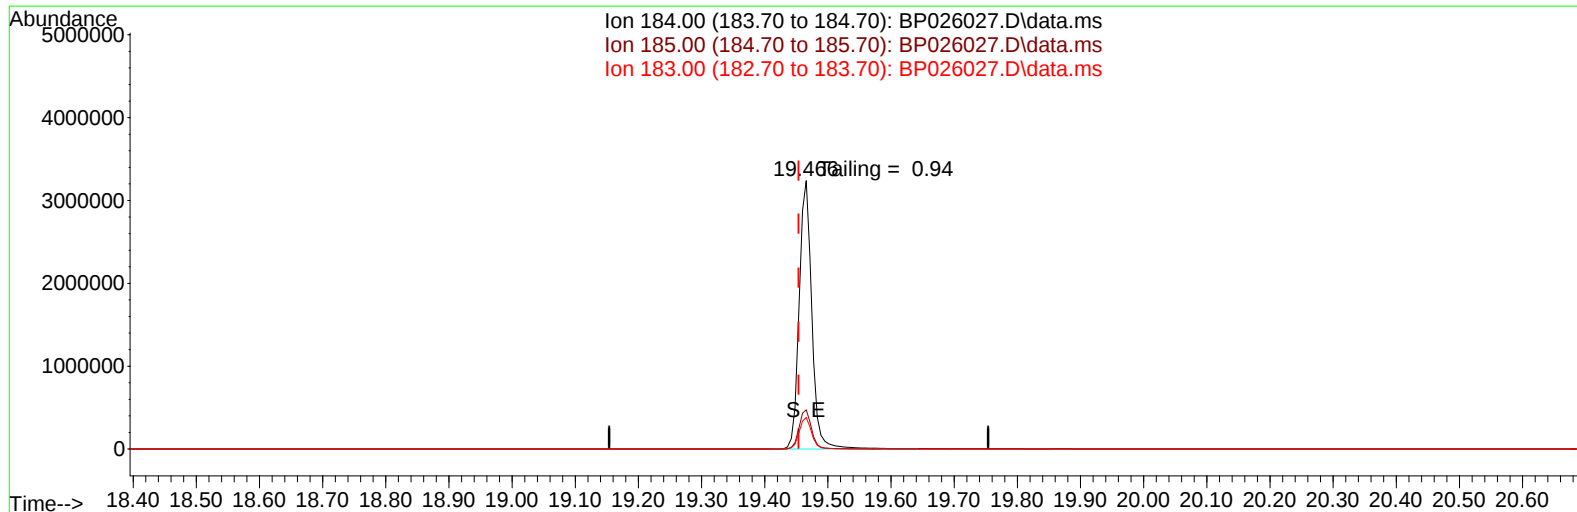

TIC: BP026027.D\data.ms

(77) Benzidine

19.466min (+ 0.012) 16317.24 ng

response 4546390

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.62
183.00	11.50	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/29/2025	BNA_P	<u>BP026027.D</u>
Compound Name	Response	Retention Time
DDT	1446445	20.766
DDD	18274	20.301
DDE	1074	19.866
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19348	1465793	1.32

Instrument :
BNA_P
ClientSampleId :
DFTPP