


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111125\
Data File : BP026089.D
Acq On : 11 Nov 2025 14:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 30 11:51:34 2025

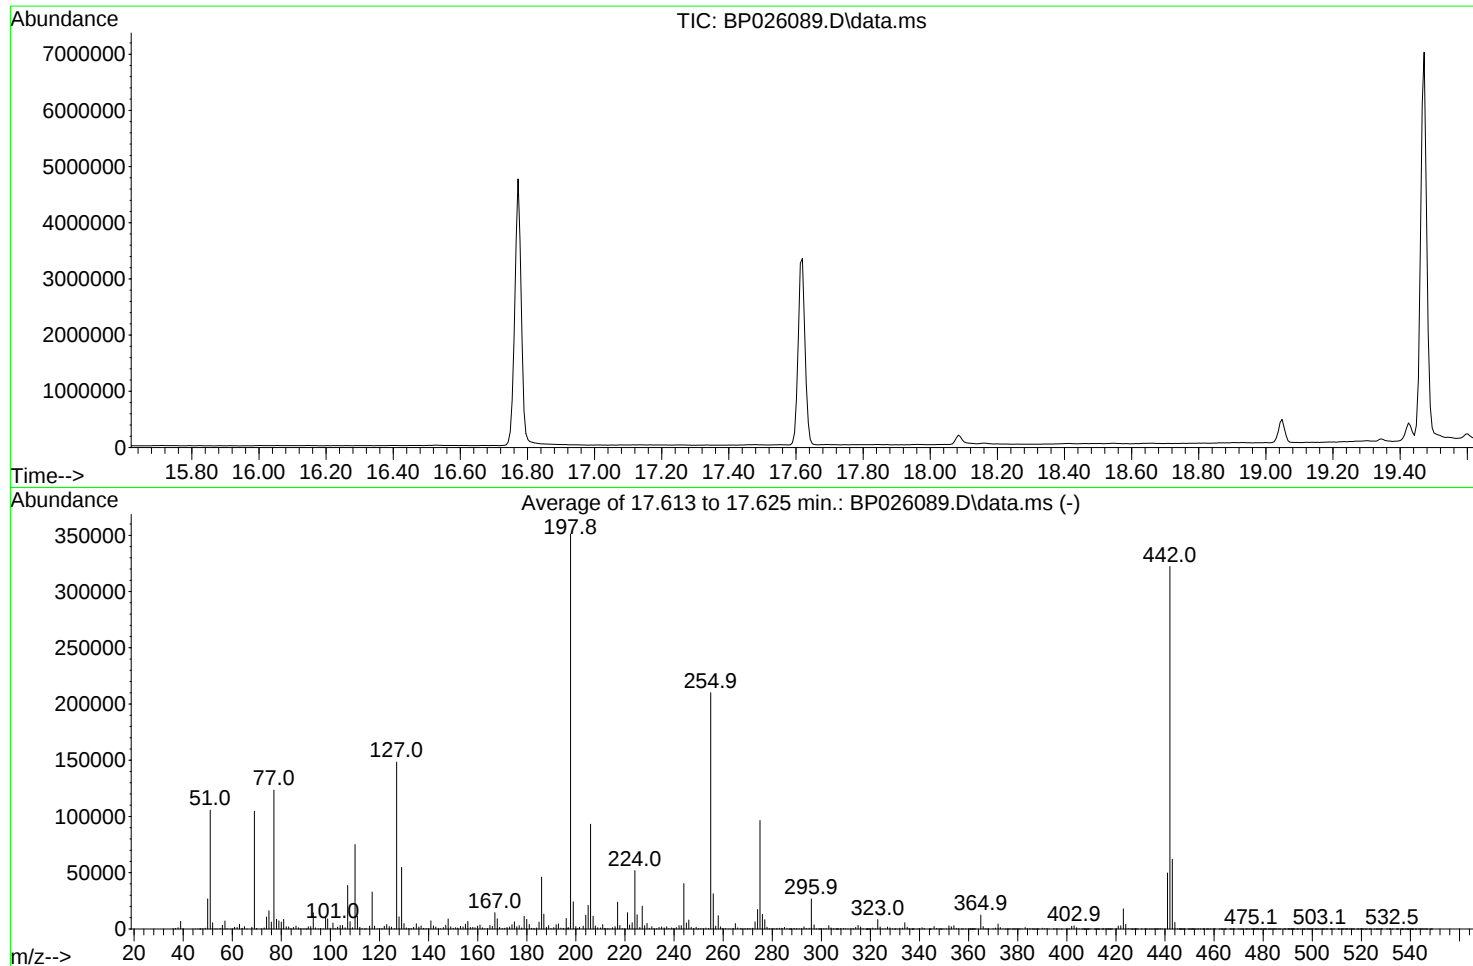


AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	1554	PASS
69	69	100	100	100.0	104622	PASS
70	69	0.00	2	0.3	304	PASS
197	198	0.00	2	0.3	1073	PASS
198	198	100	100	100.0	351105	PASS
199	198	5	9	6.9	24080	PASS
365	198	1	100	3.5	12262	PASS
441	443	0.01	150	80.2	49693	PASS
442	442	100	100	100.0	322318	PASS
443	442	15	24	19.2	61960	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111125\
Data File : BP026089.D
Acq On : 11 Nov 2025 14:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 11 15:18:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

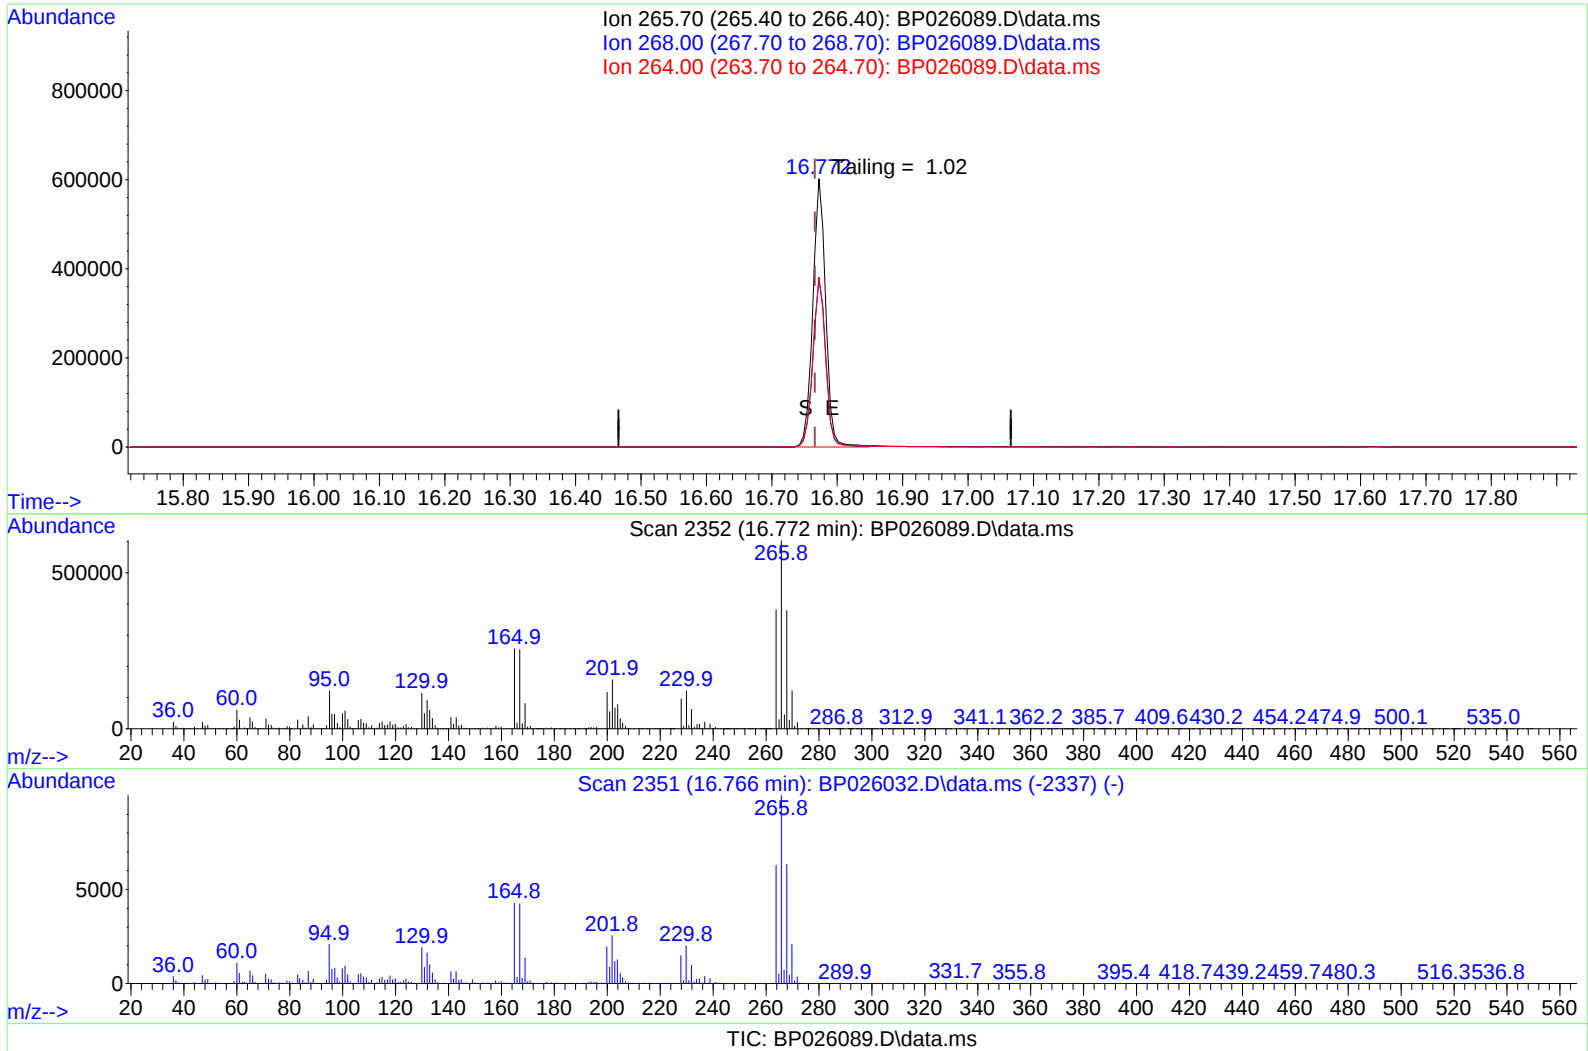

(70) Pentachlorophenol (C)

16.772min (+ 0.006) 1462042.63 ng




response 823223

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.80
264.00	62.80	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111125\
Data File : BP026089.D
Acq On : 11 Nov 2025 14:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 11 15:18:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

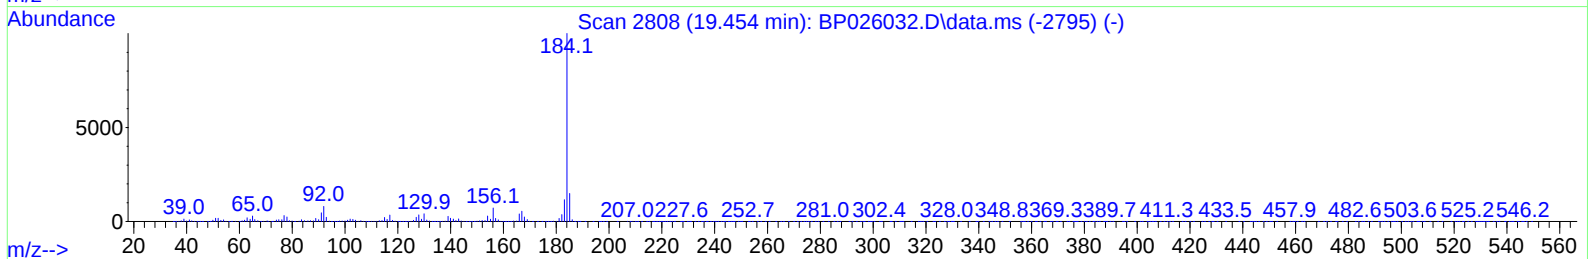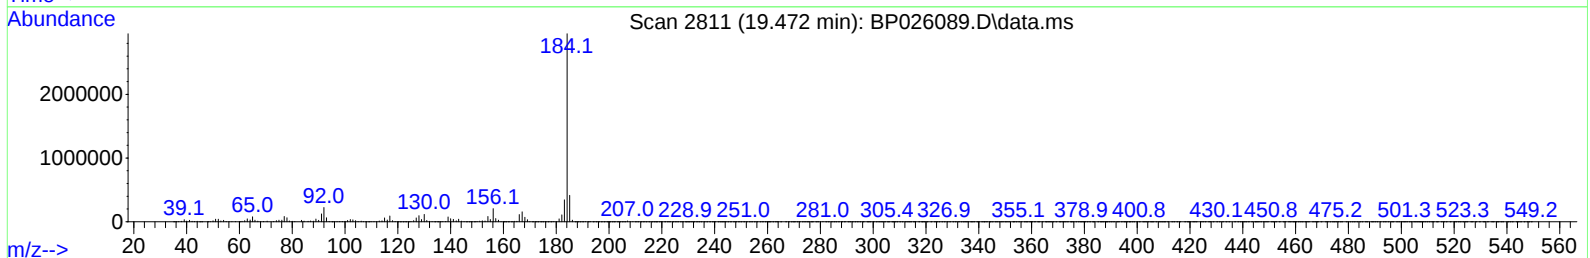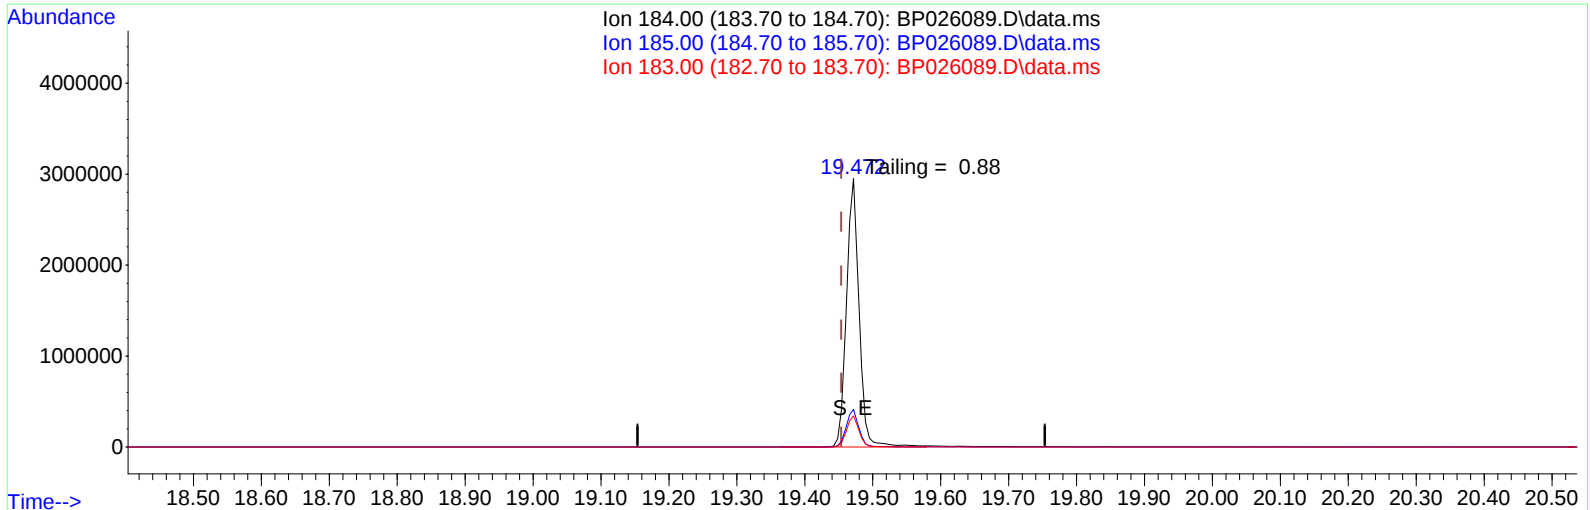

TIC: BP026089.D\data.ms

(77) Benzidine

19.472min (+ 0.018) 657528.85 ng

response 3788584

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.00
183.00	11.50	11.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2025	BNA_P	<u>BP026089.D</u>
Compound Name	Response	Retention Time
DDT	1683922	20.783
DDD	39274	20.319
DDE	2890	19.784
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
42164	1726086	2.44

Instrument :
BNA_P
ClientSampleId :
DFTPP