


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111225\
Data File : BP026107.D
Acq On : 12 Nov 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 30 11:51:34 2025

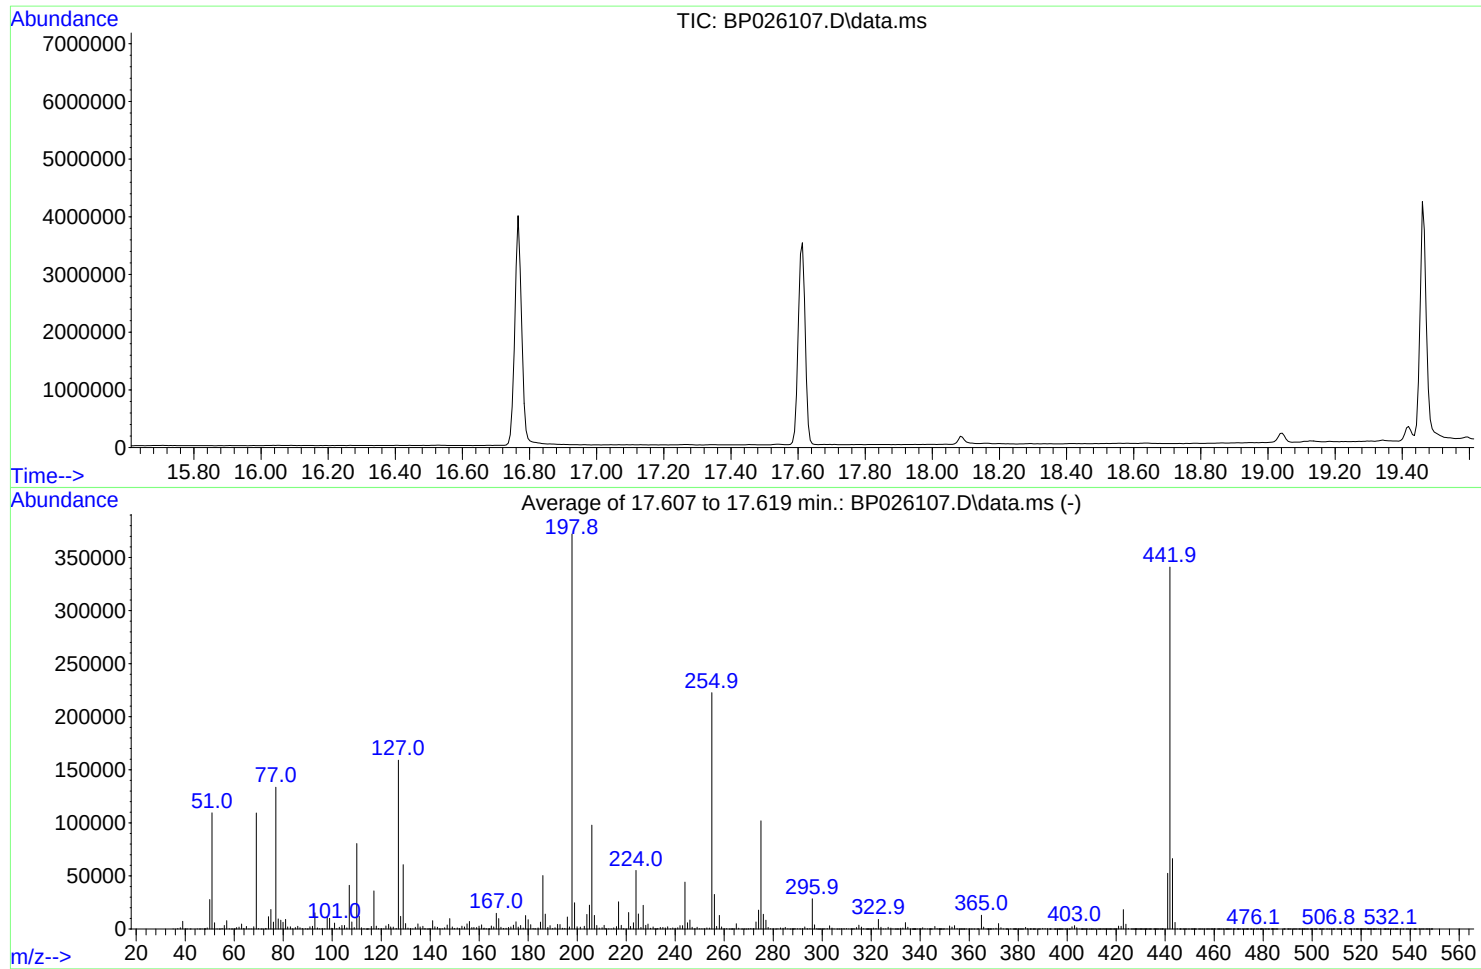

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	2105	PASS
69	69	100	100	100.0	109280	PASS
70	69	0.00	2	0.5	513	PASS
197	198	0.00	2	0.5	2025	PASS
198	198	100	100	100.0	372030	PASS
199	198	5	9	6.6	24715	PASS
365	198	1	100	3.5	12941	PASS
441	443	0.01	150	79.1	52451	PASS
442	442	100	100	100.0	341001	PASS
443	442	15	24	19.5	66336	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/12/2025	BNA_P	<u>BP026107.D</u>
Compound Name	Response	Retention Time
DDT	1708279	20.766
DDD	86648	20.307
DDE	3248	19.778
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
89896	1798175	5.00

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111225\
Data File : BP026107.D
Acq On : 12 Nov 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 12 11:18:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

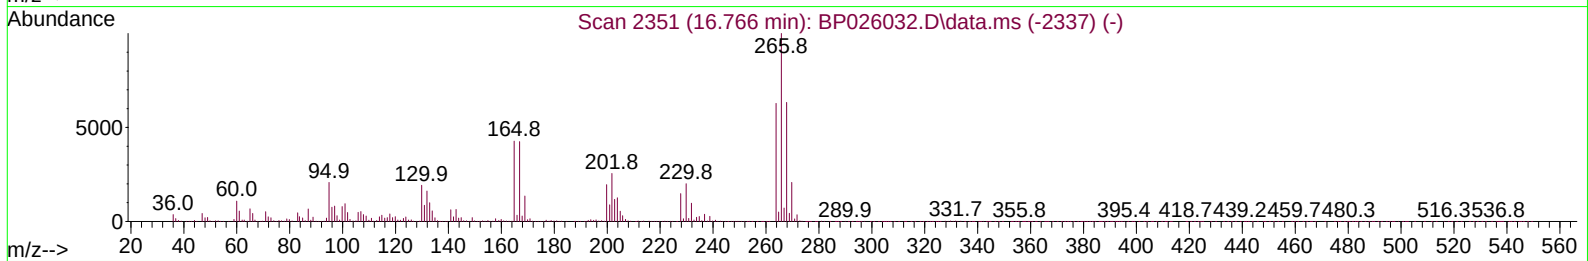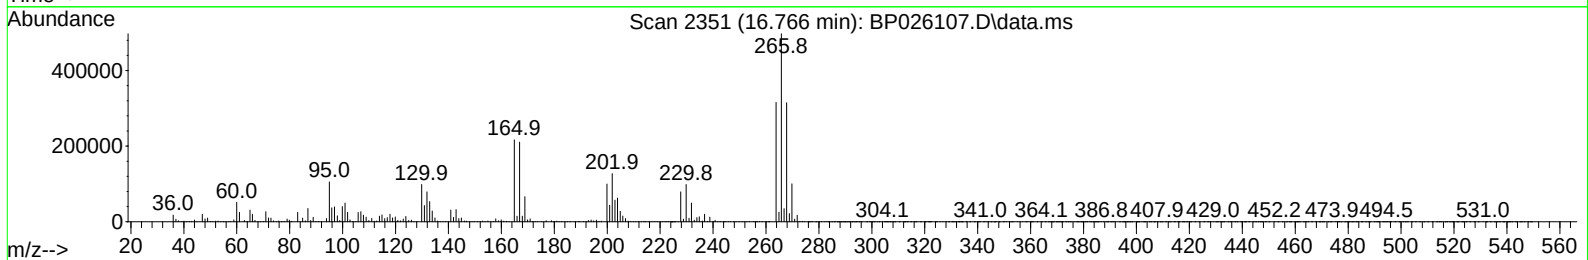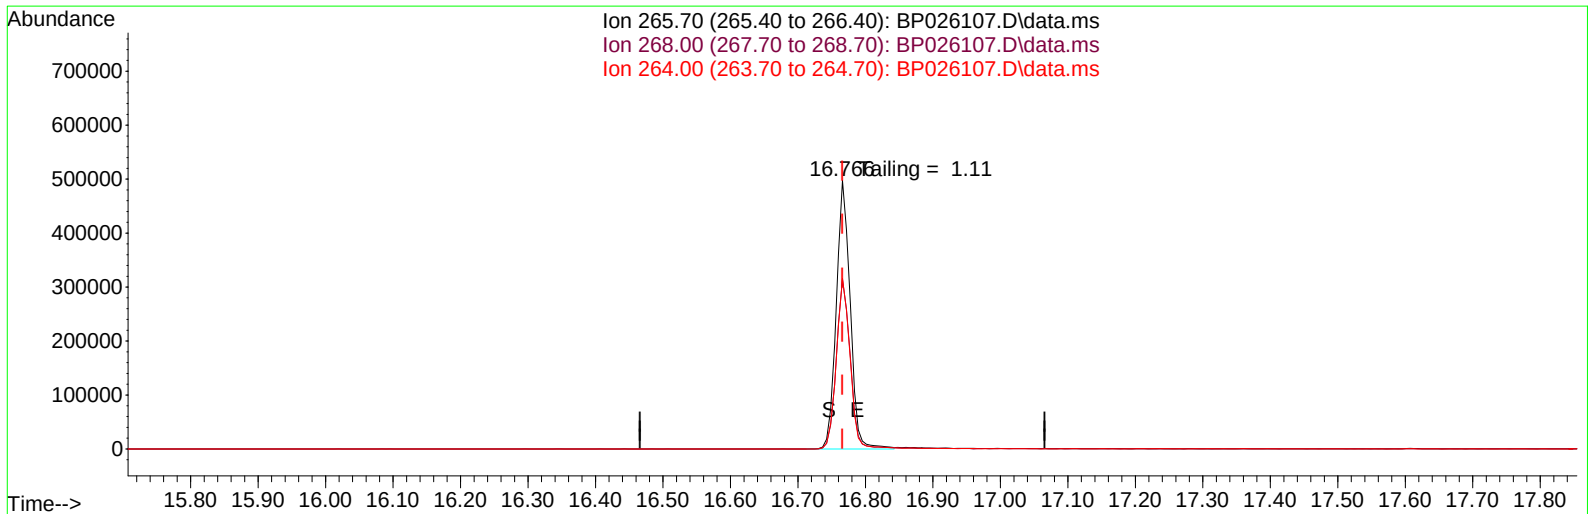

TIC: BP026107.D\data.ms

(70) Pentachlorophenol (C)

16.766min (+ 0.000) 116733.38 ng




response 714908

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.29
264.00	62.80	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111225\
Data File : BP026107.D
Acq On : 12 Nov 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 12 11:18:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

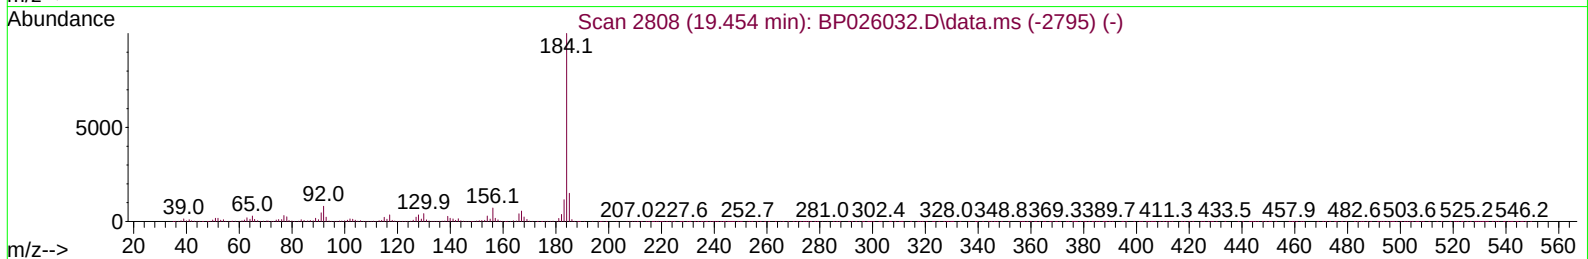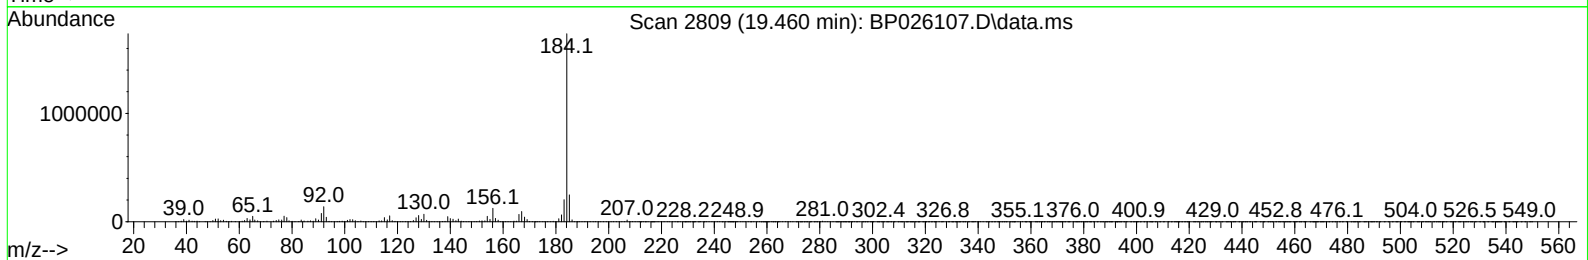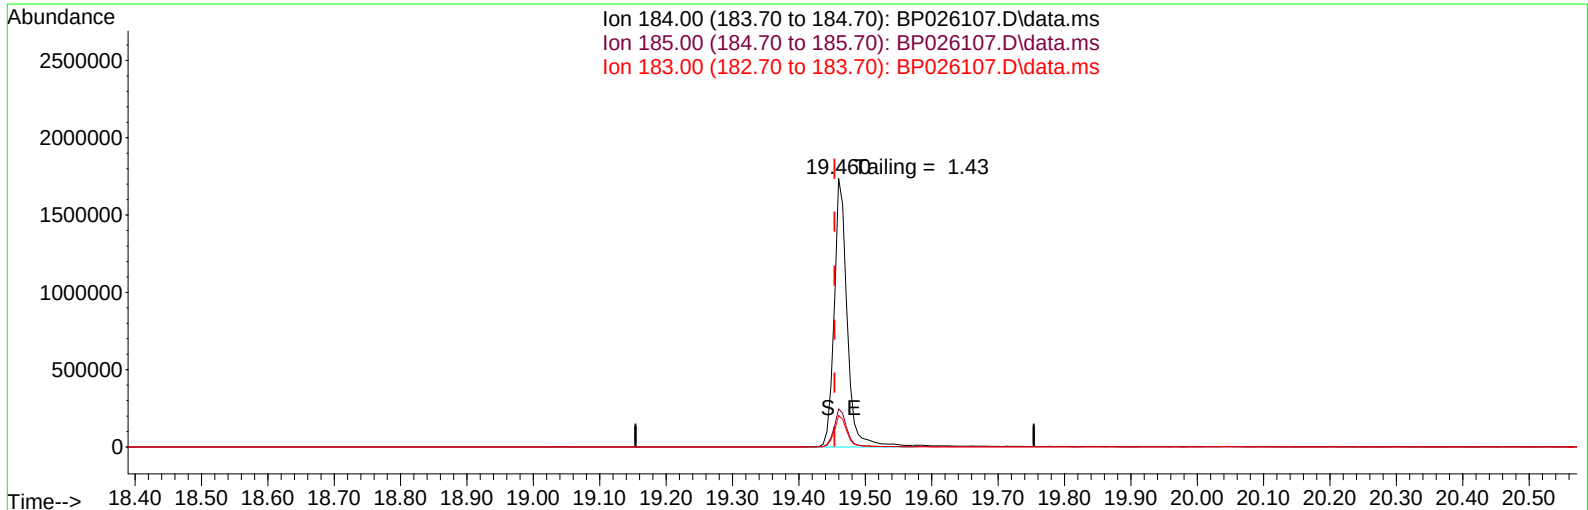

TIC: BP026107.D\data.ms

(77) Benzidine

19.460min (+ 0.006) 27750.80 ng

response 2359699

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.25
183.00	11.50	11.71
0.00	0.00	0.00