
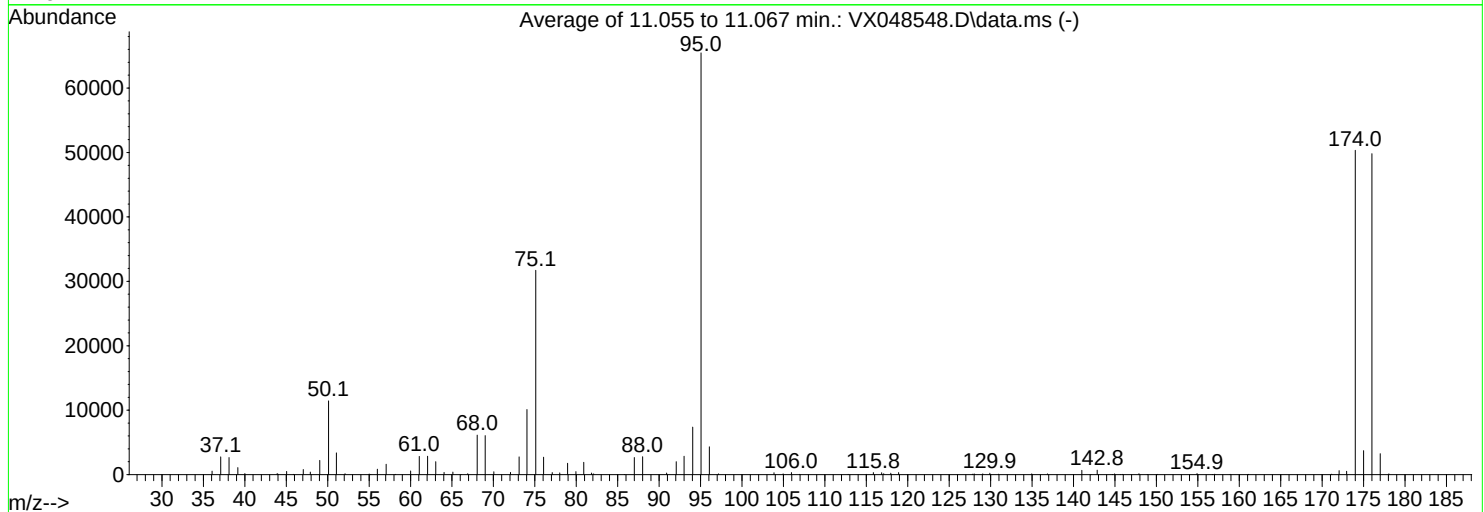


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111125\
Data File : VX048548.D
Acq On : 11 Nov 2025 08:09
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
Title : SW846 8260
Last Update : Sat Nov 08 05:08:11 2025

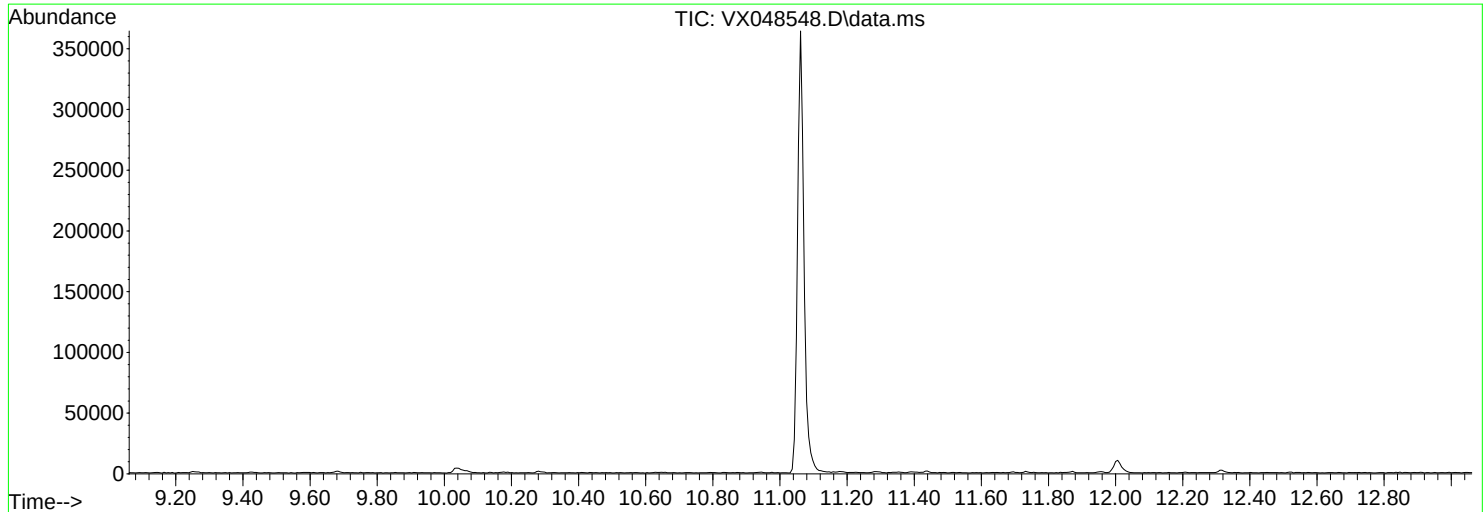

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1628

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	11450	PASS
75	95	30	60	48.4	31709	PASS
95	95	100	100	100.0	65464	PASS
96	95	5	9	6.6	4312	PASS
173	174	0.00	2	1.0	519	PASS
174	95	50	100	76.9	50333	PASS
175	174	5	9	7.4	3739	PASS
176	174	95	101	99.0	49821	PASS
177	176	5	9	6.5	3263	PASS