

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID:	Q3574	OrderDate:	11/7/2025 10:02:13 AM
Client:	Pacific Commercial Services Inc.	Project:	Kilo Pier
Contact:	Wendi Zheng	Location:	--Select--,J22,VOA Lab

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q3574-01	304641-01 Liquid	Water	Gasoline Range Organics	8015D	11/04/25		11/10/25	11/07/25



QC SUMMARY



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

WATER GASOLINE RANGE ORGANICS SURROGATE RECOVERY

Lab Name: Alliance

Client: Pacific Commercial Services Inc.

Lab Code: ACE

SDG No.: Q3574

CLIENT ID	S1 AAA-TFT	S2	S3	S4	TOT OUT
VB1110W1	98				0
BS1110W1	107				0
BS1110W2	103				0
304641-01 Liquid	77				0

QC LIMITS

AAA-TFT

For Water : 50-150

For Soil : 50-150

Column to be used to flag recovery values

* Values outside of contract required QC limits

D Surrogate Diluted Out

WATER GASOLINE RANGE ORGANICS LABORATORY CONTROL SPIKE/LABORATORY CONTROL SPIKE DUPLICATION

Lab Name: Alliance

Client: Pacific Commercial Services Inc.

Lab Code: ACE

SDG No: Q3574

Client Sample ID : BSF1110W1

Datafile: FB032336.D

COMPOUND	SPIKE ADDED ug/L	CONCENTRATION ug/L	LCS/LCSD CONCENTRATION ug/L	% REC	QC LIMITS (%)
GRO	180	0	206	114	50-150

WATER GASOLINE RANGE ORGANICS LABORATORY CONTROL SPIKE/LABORATORY CONTROL SPIKE DUPLICATION

Lab Name: Alliance

Client: Pacific Commercial Services Inc.

Lab Code: ACE

SDG No: Q3574

Client Sample ID : BSF1110W2

Datafile: FB032337.D

COMPOUND	SPIKE ADDED ug/L	CONCENTRATION ug/L	LCS/LCSD CONCENTRATION ug/L	% REC	QC LIMITS (%)
GRO	180	0	198	110	50-150

LCS/LCSD % Recovery RPD : 3.57

METHOD BLANK SUMMARY

CLIENT SAMPLE NO.

VBF1110W1

Lab Name: Alliance

Contract: PACI01

Lab Code: ACE

SDG NO.: Q3574

Lab File ID: FB032335.D

Lab Sample ID: VBF1110W1

Date Analyzed: 11/10/25

Time Analyzed: 9:13

GC Column: RTX-502.2 ID: 0.53 (mm)

Heated Purge: (Y/N) N

Instrument ID: FB

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

CLIENT SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
BSF1110W1	BSF1110W1	FB032336.D	11/10/25
BSF1110W2	BSF1110W2	FB032337.D	11/10/25
304641-01 Liquid	Q3574-01	FB032338.D	11/10/25

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	Pacific Commercial Services Inc.	Date Collected:	11/04/25
Project:	Kilo Pier	Date Received:	11/07/25
Client Sample ID:	304641-01 Liquid	SDG No.:	Q3574
Lab Sample ID:	Q3574-01	Matrix:	Water
Analytical Method:	8015D GRO	% Solid:	0
Sample Wt/Vol:	5 mL	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOD	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS										
GRO	GRO	6520000		10000	63200	90000	450000	ug/L	11/10/25 11:04	FB111025
SURROGATES										
98-08-8	Alpha,Alpha,Alpha-Trifluor	15.5			50 - 150		77%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032338.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 11:04
Operator : YP/AJ
Sample : Q3574-01 10000X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
304641-01 Liquid

Integration File: Calibration.e
Quant Time: Nov 11 03:38:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	314108	15.486 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032338.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 11:04
Operator : YP/AJ
Sample : Q3574-01 10000X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
304641-01 Liquid

Integration File: Calibration.e
Quant Time: Nov 11 03:38:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

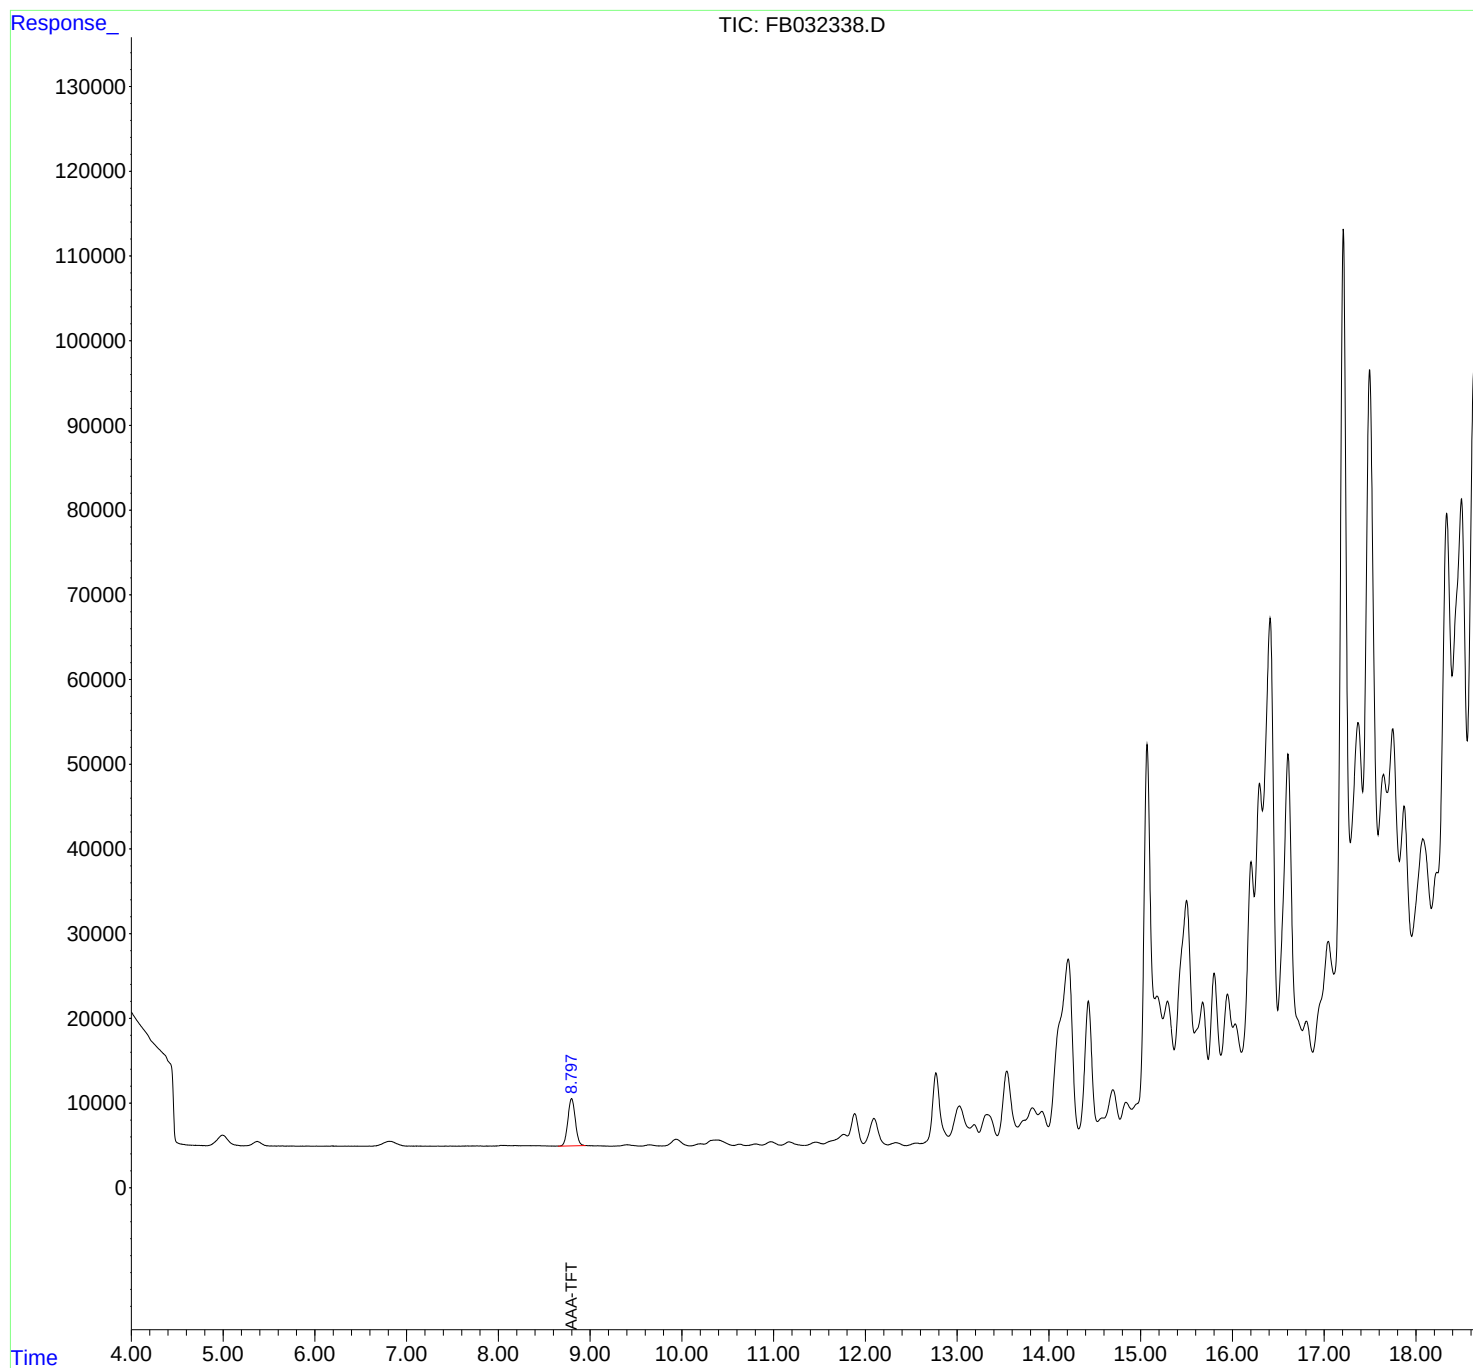

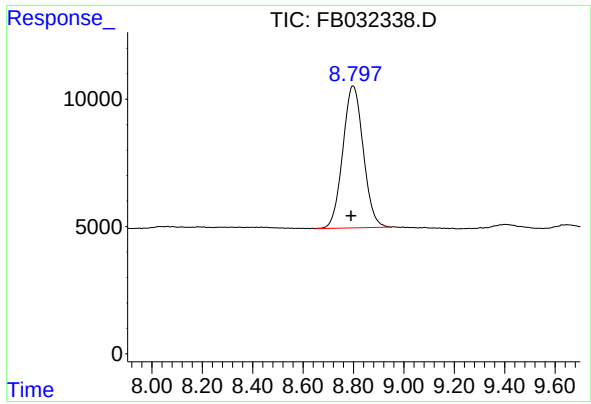

#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.008 min
Response: 314108
Conc: 15.49 ng/ml

Instrument :
FID_B
ClientSampleId :
304641-01 Liquid

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
 Data File : FB032338.D
 Signal(s) : FID2B.CH
 Acq On : 10 Nov 2025 11:04
 Sample : Q3574-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File: SAMPLE.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.641	4.604	4.664	BV	5	49	0.00%	0.000%
2	4.673	4.664	4.690	PV	9	71	0.00%	0.000%
3	4.701	4.690	4.777	PV	13	388	0.01%	0.002%
4	4.796	4.777	4.816	PV	11	110	0.00%	0.001%
5	5.238	5.224	5.254	VV	30	462	0.01%	0.002%
6	5.524	5.510	5.553	VV	15	309	0.01%	0.001%
7	5.563	5.553	5.584	VV	20	200	0.01%	0.001%
8	5.606	5.584	5.623	VV	28	307	0.01%	0.001%
9	5.650	5.623	5.675	VV	42	537	0.02%	0.003%
10	5.703	5.675	5.742	PV	19	448	0.01%	0.002%
11	5.772	5.742	5.809	VV	13	368	0.01%	0.002%
12	5.908	5.809	5.986	VV	24	1289	0.04%	0.006%
13	6.015	5.986	6.039	VV	31	374	0.01%	0.002%
14	6.063	6.039	6.100	PV	15	325	0.01%	0.002%
15	6.188	6.100	6.220	VV	44	1444	0.04%	0.007%
16	6.229	6.220	6.249	VV	31	251	0.01%	0.001%
17	6.281	6.249	6.313	VV	17	367	0.01%	0.002%
18	6.330	6.313	6.342	VV	22	223	0.01%	0.001%
19	6.366	6.342	6.417	VV	25	647	0.02%	0.003%
20	6.462	6.417	6.495	VV	29	587	0.02%	0.003%
21	6.538	6.495	6.569	VV	16	357	0.01%	0.002%
22	7.036	7.007	7.085	VV	24	986	0.03%	0.005%
23	7.098	7.085	7.109	VV	21	269	0.01%	0.001%
24	7.122	7.109	7.225	VV	25	1124	0.03%	0.005%
25	7.246	7.225	7.330	VV	18	746	0.02%	0.004%
26	7.343	7.330	7.395	VV	21	520	0.02%	0.003%
27	7.432	7.395	7.453	VV	22	570	0.02%	0.003%
28	7.479	7.453	7.551	VV	28	926	0.03%	0.004%
29	7.569	7.551	7.591	VV	14	297	0.01%	0.001%
30	7.668	7.591	7.754	VV	36	2458	0.07%	0.012%
31	7.771	7.754	7.843	VV	39	1334	0.04%	0.006%

					rteres			
32	7.871	7.843	7.898	VV	33	549	0.02%	0.003%
33	8.033	7.898	8.054	VV	89	4131	0.13%	0.020%
34	8.062	8.054	8.104	VV	101	2572	0.08%	0.012%
35	8.118	8.104	8.148	VV	78	1806	0.05%	0.009%
36	8.184	8.148	8.247	VV	81	3995	0.12%	0.019%
37	8.270	8.247	8.334	VV	68	3292	0.10%	0.016%
38	8.347	8.334	8.386	VV	70	1904	0.06%	0.009%
39	8.401	8.386	8.412	VV	67	967	0.03%	0.005%
40	8.436	8.412	8.649	VV	67	4932	0.15%	0.024%
41	8.799	8.649	9.057	VV	5619	324865	9.85%	1.567%
42	9.083	9.057	9.219	VV	58	2645	0.08%	0.013%
43	9.402	9.219	9.557	PV	170	13011	0.39%	0.063%
44	9.649	9.557	9.753	VV	153	9286	0.28%	0.045%
45	9.767	9.753	9.784	VV	28	372	0.01%	0.002%
46	9.939	9.784	10.082	VV	796	59840	1.81%	0.289%
47	10.203	10.082	10.240	VV	276	15169	0.46%	0.073%
48	10.383	10.240	10.574	VV	713	89020	2.70%	0.429%
49	10.629	10.574	10.700	VV	203	9986	0.30%	0.048%
50	10.804	10.700	10.871	VV	227	14591	0.44%	0.070%
51	10.972	10.871	11.082	VV	495	35613	1.08%	0.172%
52	11.168	11.082	11.333	VV	475	35043	1.06%	0.169%
53	11.462	11.333	11.541	VV	429	33290	1.01%	0.161%
54	11.766	11.541	11.806	VV	1346	125753	3.81%	0.606%
55	11.884	11.806	11.980	VV	3797	212781	6.45%	1.026%
56	12.094	11.980	12.245	VV	3228	216298	6.56%	1.043%
57	12.334	12.245	12.445	VV	375	24110	0.73%	0.116%
58	12.559	12.445	12.600	PV	186	10452	0.32%	0.050%
59	12.770	12.600	12.905	VV	8258	472880	14.34%	2.280%
60	13.025	12.905	13.137	VV	4077	331944	10.06%	1.601%
61	13.185	13.137	13.239	VV	1709	83150	2.52%	0.401%
62	13.328	13.239	13.438	VV	2741	210958	6.40%	1.017%
63	13.542	13.438	13.660	VV	7643	466148	14.13%	2.248%
64	13.822	13.660	13.882	VV	3010	270115	8.19%	1.303%
65	13.923	13.882	13.994	VV	2481	125015	3.79%	0.603%
66	14.210	13.994	14.326	VV	20168	1982325	60.10%	9.560%
67	14.431	14.326	14.534	PV	14823	749161	22.71%	3.613%
68	14.698	14.534	14.776	VV	3675	220283	6.68%	1.062%
69	14.842	14.776	14.903	PV	1797	85364	2.59%	0.412%
70	15.071	14.903	15.243	VV	43326	2947242	89.35%	14.213%
71	15.293	15.243	15.365	VV	12397	760651	23.06%	3.668%
72	15.501	15.365	15.591	VV	23676	2047883	62.08%	9.876%
73	15.676	15.591	15.737	VV	11159	744048	22.56%	3.588%
74	15.802	15.737	15.875	VV	14195	748172	22.68%	3.608%
75	15.948	15.875	16.100	VV	11296	1002803	30.40%	4.836%
76	16.205	16.100	16.238	VV	26133	1289008	39.08%	6.216%
77	16.298	16.238	16.328	VV	35025	1625694	49.29%	7.840%
78	16.410	16.328	16.454	VBA	54249	3298544	100.00%	15.907%

Sum of corrected areas: 20736002

rteres

FB102725.M Tue Nov 11 04:04:37 2025



CALIBRATION SUMMARY

GASOLINE RANGE ORGANICS INITIAL CALIBRATION SUMMARY

Lab Name: Alliance

Contract: PACI01

ProjectID: Kilo Pier

Lab Code: ACE

SDG No.: Q3574

Calibration Sequence : FB102725			Test : Gasoline Range Organics	
Concentration	(PPB)	Area Count	Reference Factor	File ID
45		1379940	30665	FB032267.D
90		2618714	29097	FB032268.D
180		5448966	30272	FB032269.D
450		14683527	32630	FB032270.D
900		30564498	33961	FB032271.D
AVG RF : 31325			% RSD : 6.215	AVG RT : 8.7908

GASOLINE RANGE ORGANICS CONTINUING CALIBRATION SUMMARY

20 PPB GRO STD

Lab Name: Alliane

Contract: PACI01

ProjectID: Kilo Pier

Lab Code: ACE

SDG No.: Q3574

DataFile: FB032334.D

Analyst Name: YP/AJ

Analyst Date: 11-10-2025

Conc. (PPB)	Area Count	RF	Average RF	%D
180	6453043	35850	31325	14.445

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
 Data File : FB032334.D
 Signal(s) : FID2B.CH
 Acq On : 10 Nov 2025 8:19
 Operator : YP/AJ
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Nov 11 03:37:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Quant Title :
 QLast Update : Tue Oct 28 04:57:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	396943	19.570 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	872120	31.835 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	1012376	32.859 ng/ml
3) t n-Heptane	7.755	318523	10.871 ng/ml
4) t Benzene	7.893	403482	11.655 ng/ml
6) t Toluene	10.624	1220755	34.117 ng/ml
7) t Ethylbenzene	13.060	381921	12.009 ng/ml
8) t m-Xylene	13.192	846555	25.420 ng/ml
9) t O-Xylene	13.920	738228	22.989 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	659083	23.819 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032334.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 8:19
Operator : YP/AJ
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Nov 11 03:37:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

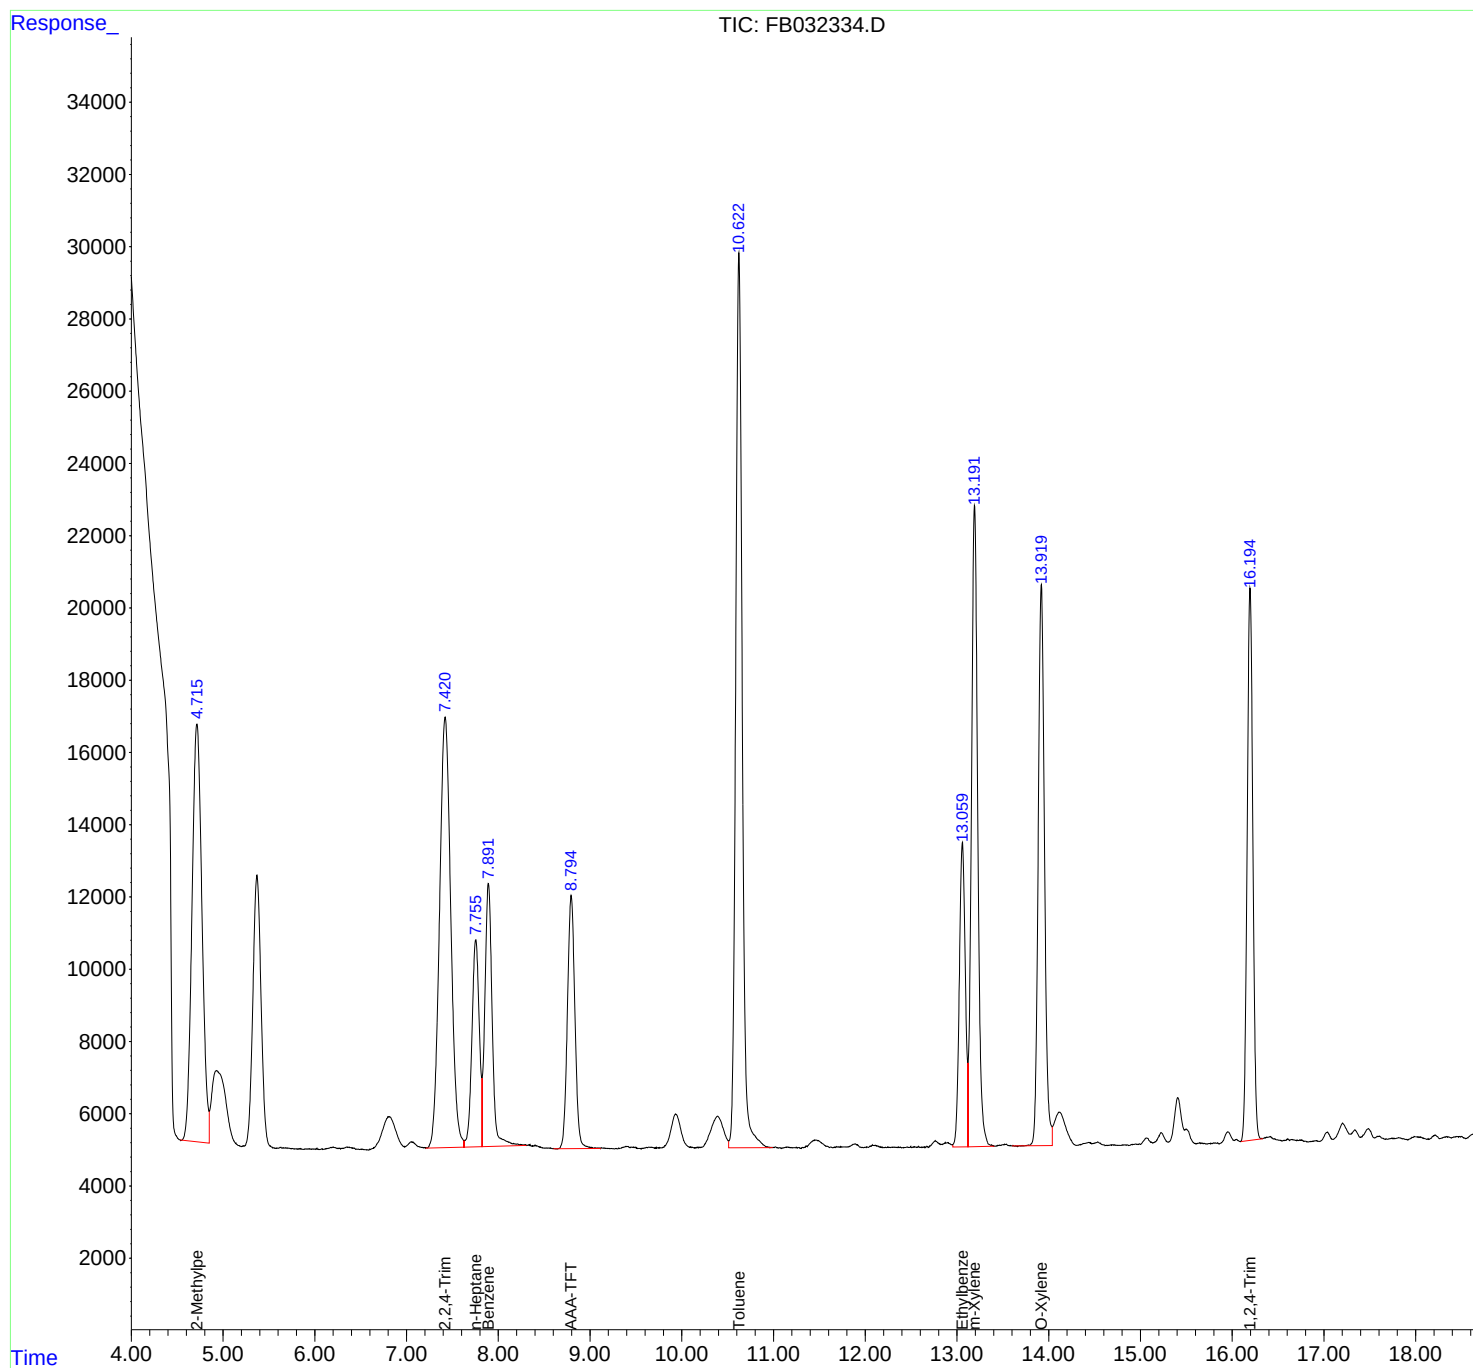

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032334.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 8:19
Sample : 20 PPB GR0 STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.716	4.532	4.850	BV	11562	872120	71.44%	12.732%
2	7.421	7.209	7.626	PV	11914	1012376	82.93%	14.779%
3	7.755	7.626	7.823	VV	5730	318523	26.09%	4.650%
4	7.893	7.823	8.309	VB	7274	403482	33.05%	5.890%
5	8.795	8.604	9.116	BB	7004	396943	32.52%	5.795%
6	10.624	10.512	10.992	VV	24770	1220755	100.00%	17.821%
7	13.060	12.954	13.120	VV	8428	381921	31.29%	5.576%
8	13.192	13.120	13.408	VV	17749	846555	69.35%	12.358%
9	13.920	13.600	14.039	BV	15530	738228	60.47%	10.777%
10	16.195	16.096	16.336	PV	15287	659083	53.99%	9.622%

Sum of corrected areas: 6849985

FB102725.M Tue Nov 11 03:59:46 2025

GASOLINE RANGE ORGANICS CONTINUING CALIBRATION SUMMARY

20 PPB GRO STD

Lab Name: Alliane

Contract: PACI01

ProjectID: Kilo Pier

Lab Code: ACE

SDG No.: Q3574

DataFile: FB032340.D

Analyst Name: YP/AJ

Analyst Date: 11-10-2025

Conc. (PPB)	Area Count	RF	Average RF	%D
180	6340513	35225	31325	12.45

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
 Data File : FB032340.D
 Signal(s) : FID2B.CH
 Acq On : 10 Nov 2025 12:45
 Operator : YP/AJ
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Nov 11 03:38:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Quant Title :
 QLast Update : Tue Oct 28 04:57:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	423154	20.863 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	887653	32.402 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	1046423	33.964 ng/ml
3) t n-Heptane	7.760	320012	10.922 ng/ml
4) t Benzene	7.899	402456	11.626 ng/ml
6) t Toluene	10.629	1208203	33.767 ng/ml
7) t Ethylbenzene	13.064	359481	11.303 ng/ml
8) t m-Xylene	13.197	763175	22.916 ng/ml
9) t O-Xylene	13.925	738090	22.985 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	615020	22.227 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032340.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 12:45
Operator : YP/AJ
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Nov 11 03:38:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

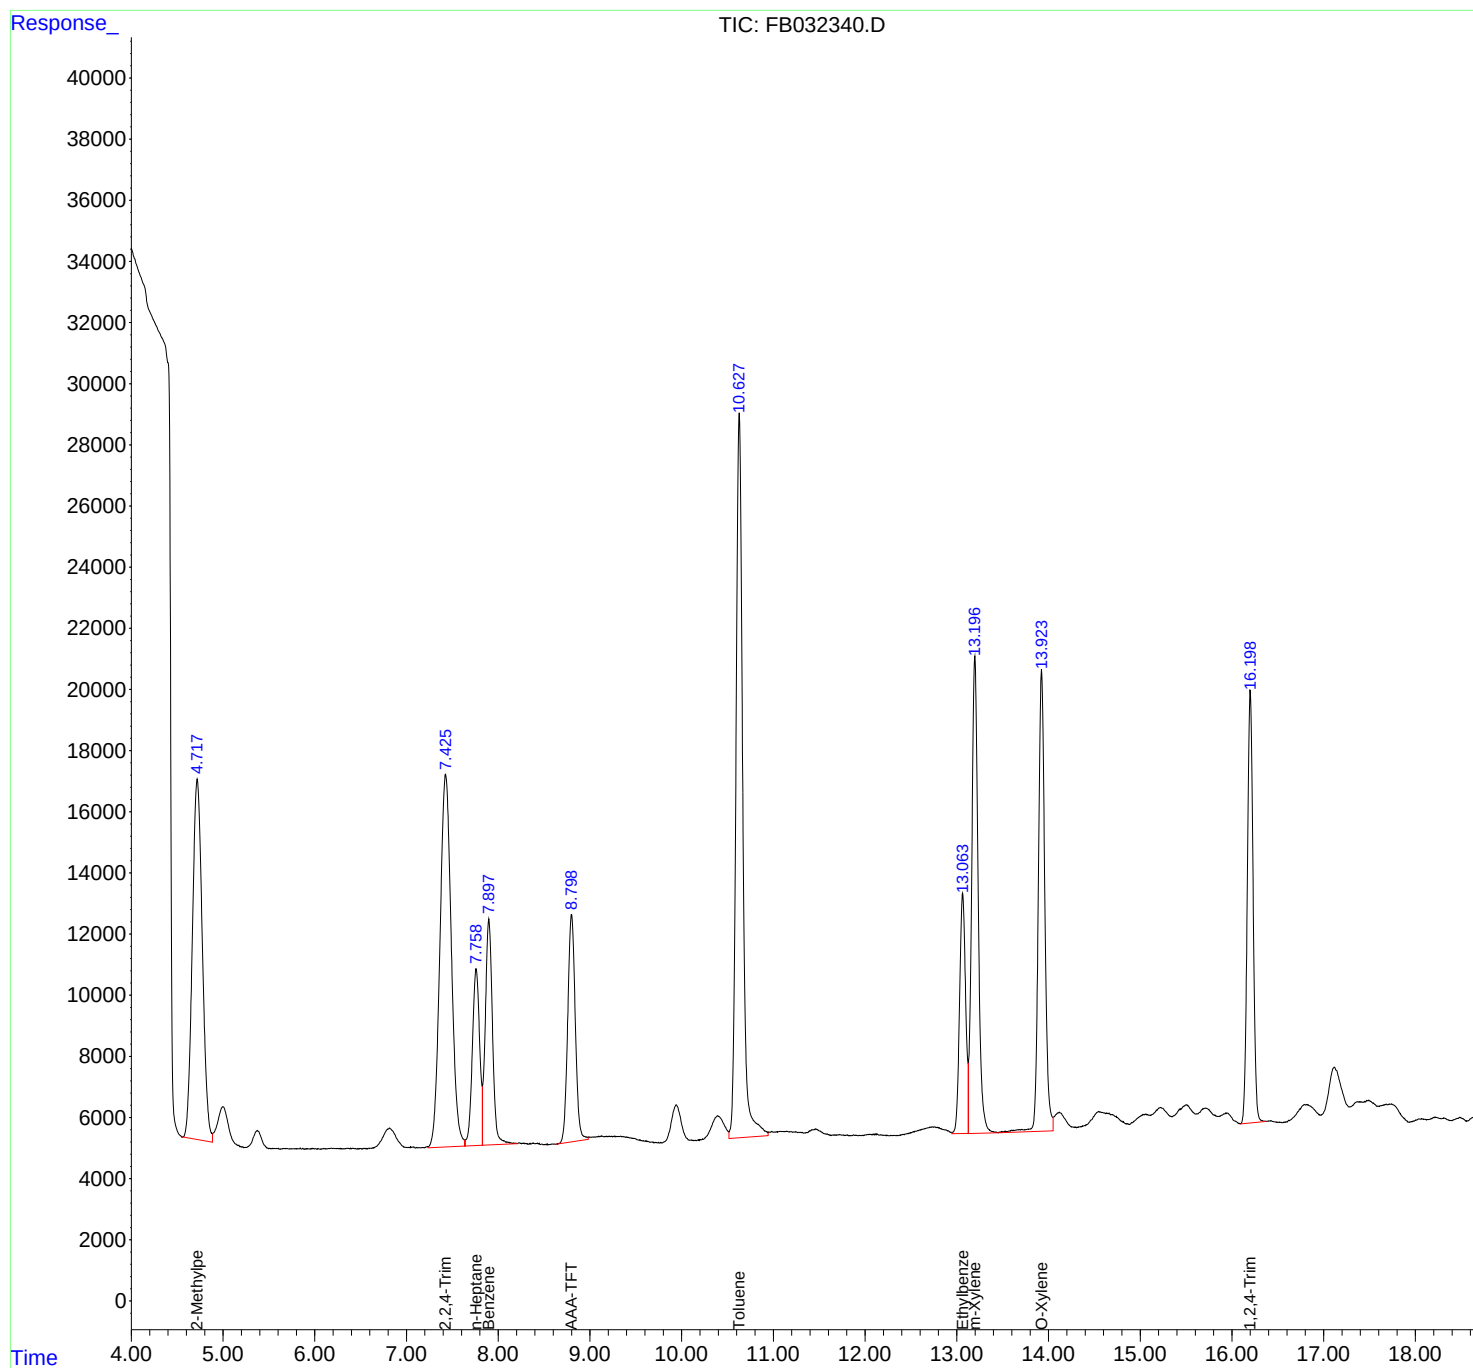

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032340.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 12:45
Sample : 20 PPB GR0 STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.718	4.548	4.885	BV	11785	887653	73.47%	13.124%
2	7.426	7.237	7.638	VV	12194	1046423	86.61%	15.471%
3	7.760	7.638	7.828	VV	5785	320012	26.49%	4.731%
4	7.899	7.828	8.211	VV	7389	402456	33.31%	5.950%
5	8.800	8.627	8.982	PV	7435	423154	35.02%	6.256%
6	10.629	10.515	10.943	VV	23700	1208203	100.00%	17.863%
7	13.064	12.946	13.125	VV	7865	359481	29.75%	5.315%
8	13.197	13.125	13.452	VV	15589	763175	63.17%	11.283%
9	13.925	13.452	14.051	PV	15083	738090	61.09%	10.913%
10	16.200	16.090	16.375	PV	14162	615020	50.90%	9.093%

Sum of corrected areas: 6763667

FB102725.M Tue Nov 11 04:03:48 2025

Analytical Sequence

Client: Pacific Commercial Services Inc.

SDG No.: Q3574

Project: Kilo Pier

Instrument ID: FID_B

GC Column: RTX-502.2 ID: 0.53 (mm)

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

MEAN SUROGATE RT FROM INITIAL CALIBRATION 8.7908					
CLIENT SAMPLE NO.	LAB SAMPLE ID	DATE AND TIME ANALYZED	DATAFILE	RT	#
20 PPB GRO STD	20 PPB GRO STD	10 Nov 2025 8:19	FB032334.D	8.795	
VBF1110W1	VBF1110W1	10 Nov 2025 9:13	FB032335.D	8.798	
BSF1110W1	BSF1110W1	10 Nov 2025 9:41	FB032336.D	8.799	
BSF1110W2	BSF1110W2	10 Nov 2025 10:09	FB032337.D	8.799	
304641-01 Liquid	Q3574-01	10 Nov 2025 11:04	FB032338.D	8.799	
20 PPB GRO STD	20 PPB GRO STD	10 Nov 2025 12:45	FB032340.D	8.800	



QC SAMPLE DATA

Report of Analysis

Client:	Pacific Commercial Services Inc.	Date Collected:	
Project:	Kilo Pier	Date Received:	
Client Sample ID:	VBF1110W1	SDG No.:	Q3574
Lab Sample ID:	VBF1110W1	Matrix:	Water
Analytical Method:	8015D GRO	% Solid:	0
Sample Wt/Vol:	5 mL	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOD	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS										
GRO	GRO	9.00	U	1	6.00	9.00	45.0	ug/L	11/10/25 9:13	FB111025
SURROGATES										
98-08-8	Alpha,Alpha,Alpha-Trifluor	19.5			50 - 150		98%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032335.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 9:13
Operator : YP/AJ
Sample : VBF1110W1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1110W1

Integration File: Calibration.e
Quant Time: Nov 11 03:37:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	395890	19.519 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032335.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 9:13
Operator : YP/AJ
Sample : VBF1110W1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1110W1

Integration File: Calibration.e
Quant Time: Nov 11 03:37:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

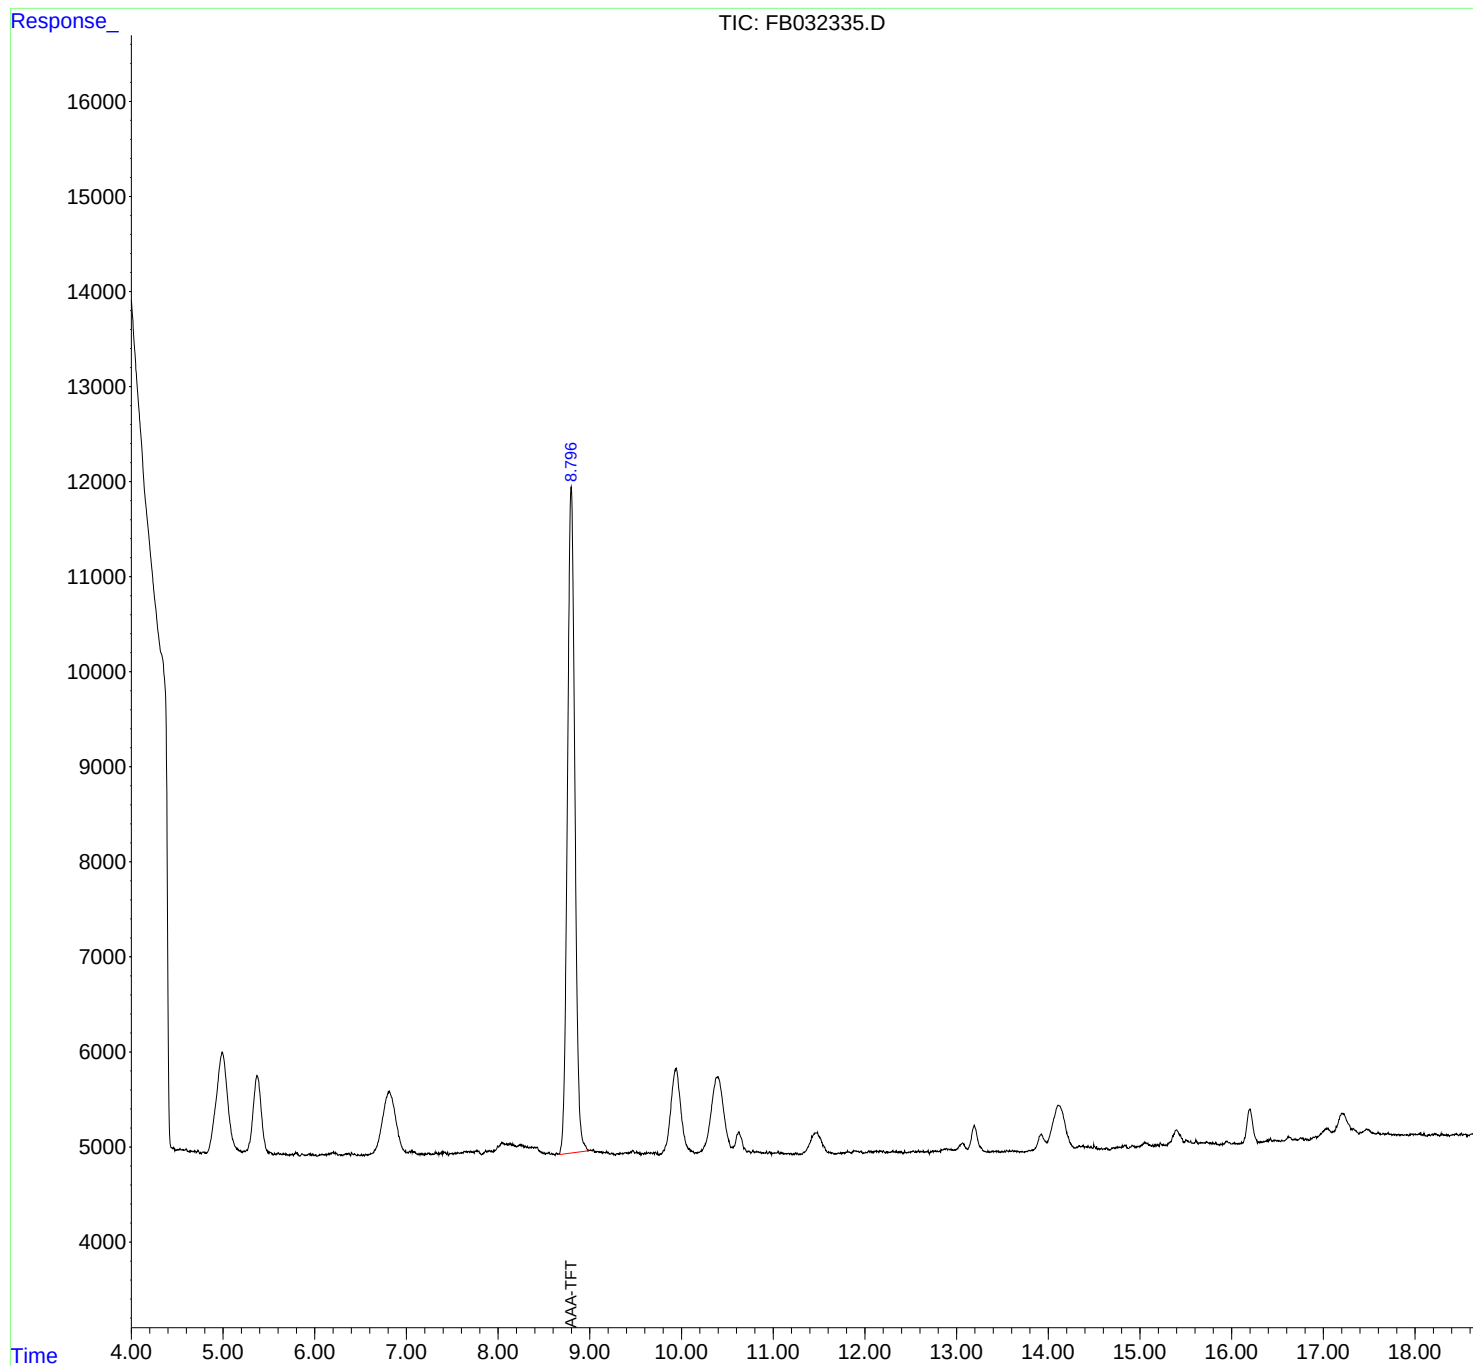

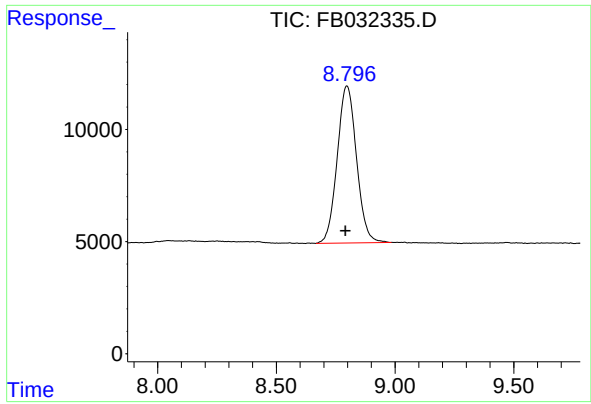

#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.007 min
Response: 395890
Conc: 19.52 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1110W1

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032335.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 9:13
Sample : VBF1110W1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	8.798	8.667	8.985	PV	7005	395890	100.00%	100.000%
Sum of corrected areas:						395890		

FB102725.M Tue Nov 11 04:00:21 2025

Report of Analysis

Client:	Pacific Commercial Services Inc.	Date Collected:	
Project:	Kilo Pier	Date Received:	
Client Sample ID:	BSF1110W1	SDG No.:	Q3574
Lab Sample ID:	BSF1110W1	Matrix:	Water
Analytical Method:	8015D GRO	% Solid:	0
Sample Wt/Vol:	5 mL	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOD	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS										
GRO	GRO	206		1	6.00	9.00	45.0	ug/L	11/10/25 9:41	FB111025
SURROGATES										
98-08-8	Alpha,Alpha,Alpha-Trifluor	21.5			50 - 150		107%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
 Data File : FB032336.D
 Signal(s) : FID2B.CH
 Acq On : 10 Nov 2025 9:41
 Operator : YP/AJ
 Sample : BSF1110W1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1110W1

Integration File: Calibration.e
 Quant Time: Nov 11 03:37:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Quant Title :
 QLast Update : Tue Oct 28 04:57:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	435739	21.483 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	905106	33.039 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	1078762	35.014 ng/ml
3) t n-Heptane	7.759	331738	11.322 ng/ml
4) t Benzene	7.897	410791	11.866 ng/ml
6) t Toluene	10.628	1215990	33.984 ng/ml
7) t Ethylbenzene	13.063	368685	11.592 ng/ml
8) t m-Xylene	13.196	770906	23.148 ng/ml
9) t O-Xylene	13.924	743187	23.144 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	630071	22.771 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032336.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 9:41
Operator : YP/AJ
Sample : BSF1110W1
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1110W1

Integration File: Calibration.e
Quant Time: Nov 11 03:37:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

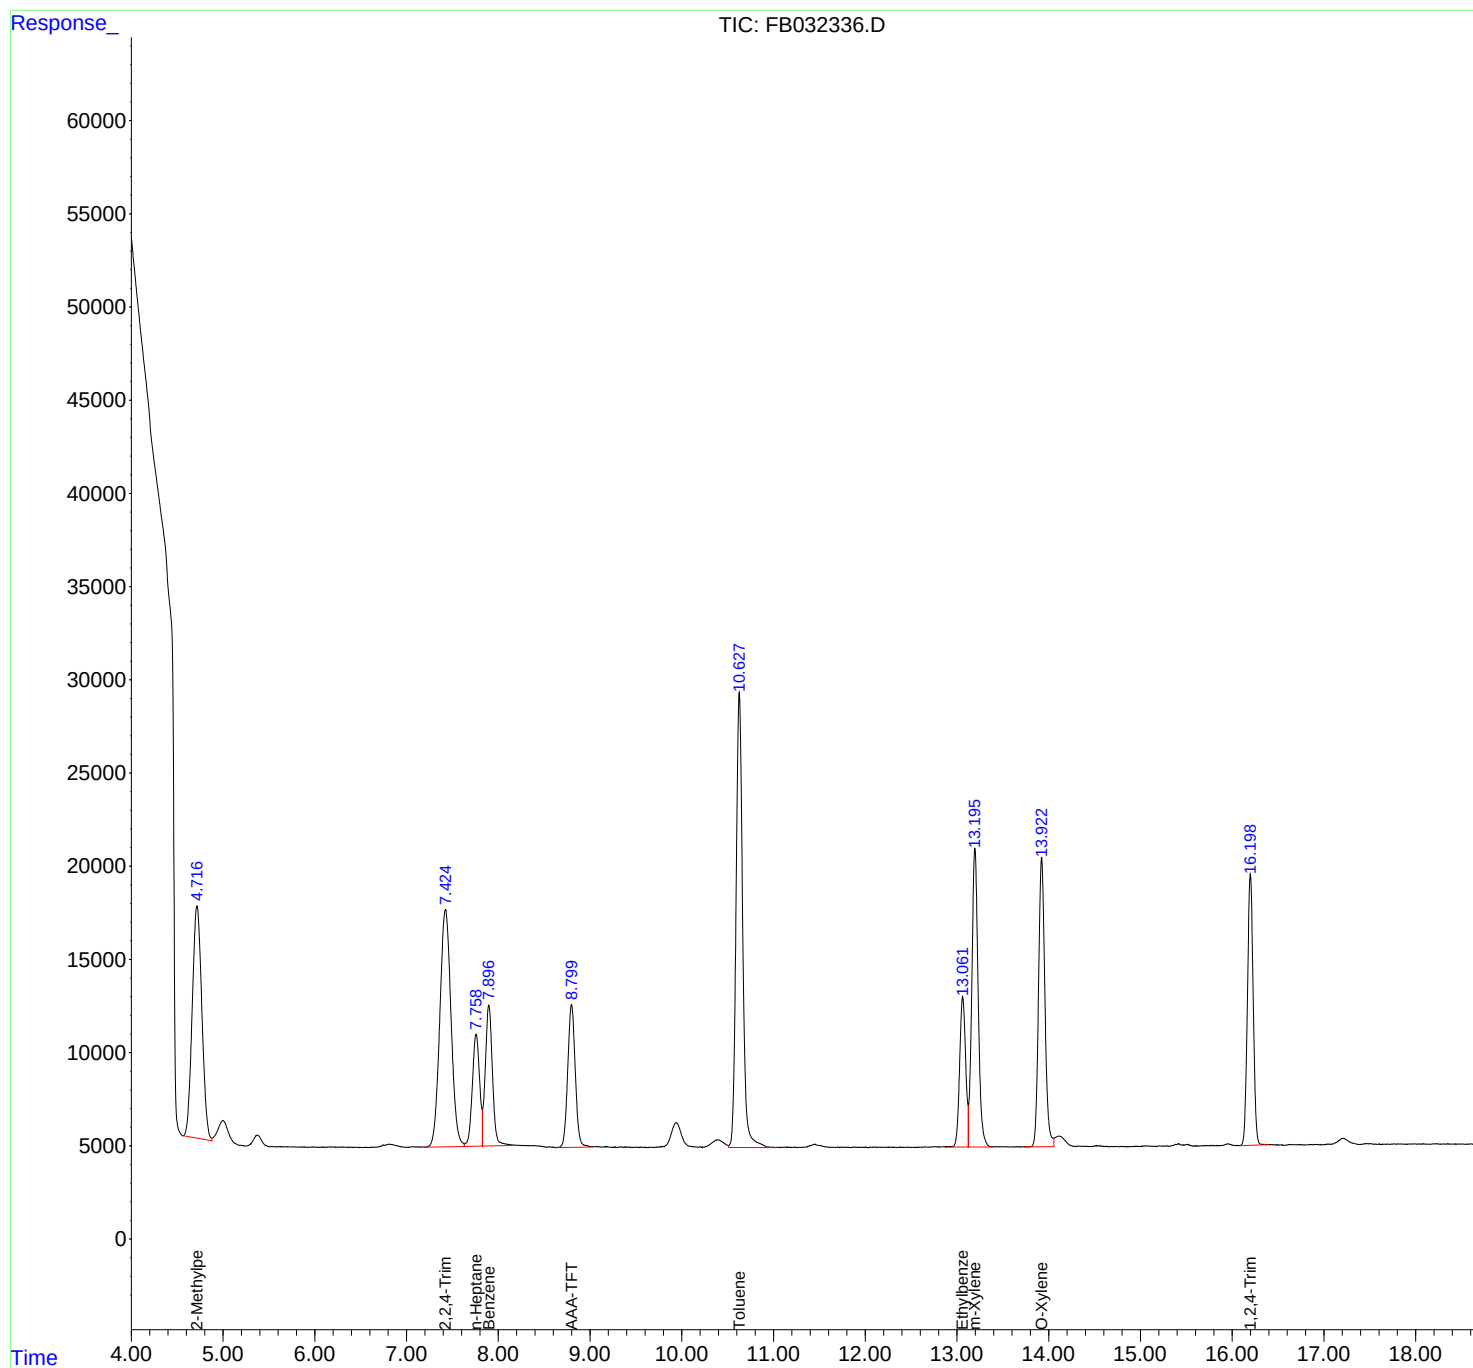

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032336.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 9:41
Sample : BSF1110W1
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.717	4.559	4.880	BV	12463	905106	74.43%	13.135%
2	7.425	7.193	7.630	PV	12731	1078762	88.71%	15.655%
3	7.759	7.630	7.827	VV	6013	331738	27.28%	4.814%
4	7.897	7.827	8.203	VV	7555	410791	33.78%	5.961%
5	8.799	8.631	9.032	BV	7652	435739	35.83%	6.323%
6	10.628	10.510	11.039	VV	24385	1215990	100.00%	17.646%
7	13.063	12.876	13.124	PV	8076	368685	30.32%	5.350%
8	13.196	13.124	13.388	VB	16015	770906	63.40%	11.187%
9	13.924	13.736	14.056	BV	15525	743187	61.12%	10.785%
10	16.199	16.082	16.401	BBA	14554	630071	51.82%	9.143%

Sum of corrected areas: 6890975

FB102725.M Tue Nov 11 04:01:26 2025

Report of Analysis

Client:	Pacific Commercial Services Inc.	Date Collected:	
Project:	Kilo Pier	Date Received:	
Client Sample ID:	BSF1110W2	SDG No.:	Q3574
Lab Sample ID:	BSF1110W2	Matrix:	Water
Analytical Method:	8015D GRO	% Solid:	0
Sample Wt/Vol:	5 mL	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOD	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS										
GRO	GRO	198		1	6.00	9.00	45.0	ug/L	11/10/25 10:09	FB111025
SURROGATES										
98-08-8	Alpha,Alpha,Alpha-Trifluor	20.7			50 - 150		103%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
 Data File : FB032337.D
 Signal(s) : FID2B.CH
 Acq On : 10 Nov 2025 10:09
 Operator : YP/AJ
 Sample : BSF1110W2
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1110W2

Integration File: Calibration.e
 Quant Time: Nov 11 03:38:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Quant Title :
 QLast Update : Tue Oct 28 04:57:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	419413	20.678 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	873029	31.868 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	1043588	33.872 ng/ml
3) t n-Heptane	7.759	318597	10.873 ng/ml
4) t Benzene	7.898	392442	11.336 ng/ml
6) t Toluene	10.627	1171046	32.728 ng/ml
7) t Ethylbenzene	13.063	353639	11.119 ng/ml
8) t m-Xylene	13.196	741293	22.259 ng/ml
9) t O-Xylene	13.923	714436	22.248 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	607974	21.972 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032337.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 10:09
Operator : YP/AJ
Sample : BSF1110W2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1110W2

Integration File: Calibration.e
Quant Time: Nov 11 03:38:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

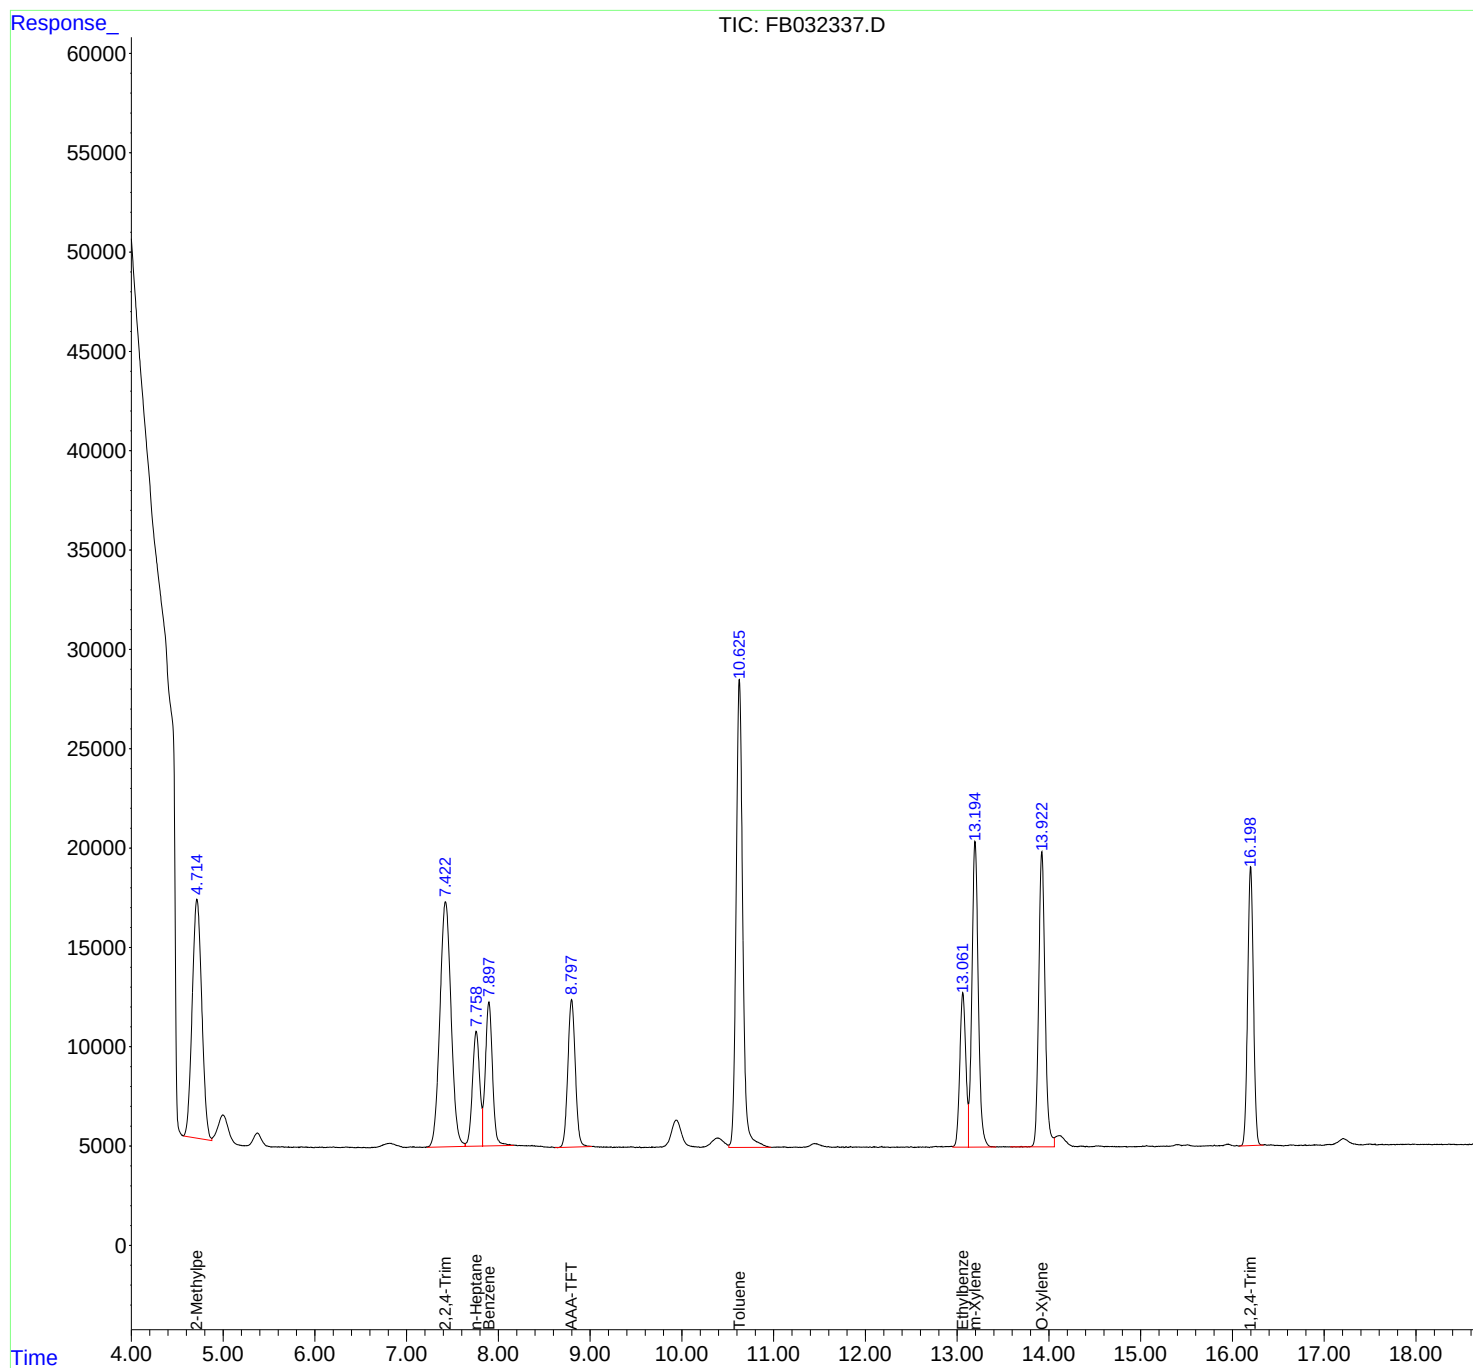

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032337.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 10:09
Sample : BSF1110W2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.716	4.566	4.877	PV	12028	873029	74.55%	13.157%
2	7.424	7.228	7.639	VV	12337	1043588	89.12%	15.727%
3	7.759	7.639	7.827	VV	5792	318597	27.21%	4.801%
4	7.898	7.827	8.169	VV	7245	392442	33.51%	5.914%
5	8.799	8.618	9.021	BV	7426	419413	35.82%	6.321%
6	10.627	10.512	10.972	VV	23555	1171046	100.00%	17.648%
7	13.063	12.953	13.124	VV	7775	353639	30.20%	5.330%
8	13.196	13.124	13.424	VB	15382	741293	63.30%	11.172%
9	13.923	13.577	14.059	BV	14853	714436	61.01%	10.767%
10	16.199	16.074	16.336	PV	14035	607974	51.92%	9.162%

Sum of corrected areas: 6635456

FB102725.M Tue Nov 11 04:02:31 2025

Manual Integration Report

Sample ID	ClientId ID	File ID	Sequence ID	Parameter	Supervised By	Supervised On	Reason
.BLK		FB032339.D	fb111025	AAA-TFT	yogesh	11/11/2025 8:40:23 AM	Peak Integrated by Software incorrectly

Instrument ID: FID_B

Daily Analysis Runlog For Sequence/QC Batch ID # FB102725

Review By	yogesh	Review On	10/29/2025 7:48:30 AM		
Supervise By	mohammad	Supervise On	10/29/2025 7:50:23 AM		
SubDirectory	FB102725	HP Acquire Method	FID_B	HP Processing Method	fb102725.m
STD. NAME		STD REF.#			
Tune/Reschk Initial Calibration Stds		PP24717,PP25006,PP25007,PP25008,PP25009,PP25010			
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard		PP24718,PP25011			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	5 GRO STD	FB032267.D	27 Oct 2025 9:43 am	YP/AJ	Ok
2	10 GRO STD	FB032268.D	27 Oct 2025 10:11 am	YP/AJ	Ok
3	20 GRO STD	FB032269.D	27 Oct 2025 10:38 am	YP/AJ	Ok
4	50 GRO STD	FB032270.D	27 Oct 2025 11:06 am	YP/AJ	Ok
5	100 GRO STD	FB032271.D	27 Oct 2025 11:34 am	YP/AJ	Ok
6	FB1027GROICV	FB032272.D	27 Oct 2025 12:20 pm	YP/AJ	Ok

M : Manual Integration

Instrument ID: FID_B

Daily Analysis Runlog For Sequence/QC Batch ID # FB111025

Review By	Amit	Review On	11/11/2025 7:21:59 AM
Supervise By	yogesh	Supervise On	11/11/2025 8:40:34 AM
SubDirectory	FB111025	HP Acquire Method	FID_B
		HP Processing Method	fb102725
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24717,PP25006,PP25007,PP25008,PP25009,PP25010		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP25050,PP25051		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	20 PPB GRO STD	FB032334.D	10 Nov 2025 8:19	YP/AJ	Ok
2	VBF1110W1	FB032335.D	10 Nov 2025 9:13	YP/AJ	Ok
3	BSF1110W1	FB032336.D	10 Nov 2025 9:41	YP/AJ	Ok
4	BSF1110W2	FB032337.D	10 Nov 2025 10:09 am	YP/AJ	Ok
5	Q3574-01	FB032338.D	10 Nov 2025 11:04	YP/AJ	Ok
6	I.BLK	FB032339.D	10 Nov 2025 12:18	YP/AJ	Ok,M
7	20 PPB GRO STD	FB032340.D	10 Nov 2025 12:45 pm	YP/AJ	Ok

M : Manual Integration

Instrument ID: FID_B

Daily Analysis Runlog For Sequence/QC Batch ID # FB102725

Review By	yogesh	Review On	10/29/2025 7:48:30 AM
Supervise By	mohammad	Supervise On	10/29/2025 7:50:23 AM
SubDirectory	FB102725	HP Acquire Method	FID_B
		HP Processing Method	fb102725.m

STD. NAME	STD REF.#
Tune/Reschk Initial Calibration Stds	PP24717,PP25006,PP25007,PP25008,PP25009,PP25010
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24718,PP25011

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	5 GRO STD		FB032267.D	27 Oct 2025 9:43 am		YP/AJ	Ok
2	10 GRO STD		FB032268.D	27 Oct 2025 10:11 am		YP/AJ	Ok
3	20 GRO STD		FB032269.D	27 Oct 2025 10:38 am		YP/AJ	Ok
4	50 GRO STD		FB032270.D	27 Oct 2025 11:06 am		YP/AJ	Ok
5	100 GRO STD		FB032271.D	27 Oct 2025 11:34 am		YP/AJ	Ok
6	FB1027GROICV		FB032272.D	27 Oct 2025 12:20 pm		YP/AJ	Ok

M : Manual Integration

Instrument ID: FID_B

Daily Analysis Runlog For Sequence/QC Batch ID # FB111025

Review By	Amit	Review On	11/11/2025 7:21:59 AM
Supervise By	yogesh	Supervise On	11/11/2025 8:40:34 AM
SubDirectory	FB111025	HP Acquire Method	FID_B
		HP Processing Method	fb102725

STD. NAME	STD REF.#
Tune/Reschk Initial Calibration Stds	PP24717,PP25006,PP25007,PP25008,PP25009,PP25010
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP25050,PP25051

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	20 PPB GRO STD		FB032334.D	10 Nov 2025 8:19		YP/AJ	Ok
2	VBF1110W1		FB032335.D	10 Nov 2025 9:13		YP/AJ	Ok
3	BSF1110W1		FB032336.D	10 Nov 2025 9:41		YP/AJ	Ok
4	BSF1110W2		FB032337.D	10 Nov 2025 10:09 am		YP/AJ	Ok
5	Q3574-01		FB032338.D	10 Nov 2025 11:04		YP/AJ	Ok
6	I.BLK		FB032339.D	10 Nov 2025 12:18		YP/AJ	Ok,M
7	20 PPB GRO STD		FB032340.D	10 Nov 2025 12:45 pm		YP/AJ	Ok

M : Manual Integration



SHIPPING DOCUMENTS



284 Sheffield Street, Mountainside, NJ 07092
(908) 789-8900 Fax: (908) 788-9222
www.chemtech.net

CHAIN OF CUSTODY RECORD

Alliance Project Number:

Q3574

COC Number:

CLIENT INFORMATION

PROJECT INFORMATION

BILLING INFORMATION

COMPANY: Pacific Commercial Services, Inc.
ADDRESS: 91-254 Olai Street
CITY Kapolei STATE: HI ZIP: 96707
ATTENTION: Wendi Zheng
PHONE: 808-545-4599 FAX:

PROJECT NAME: Kilo Pier
PROJECT #: 304641-01 LOCATION: JBPHH
PROJECT MANAGER: Wendi Zheng, Daniel Barragan
E-MAIL: Wendi.Zheng@pcshi.com
PHONE: 808-729-0889 FAX:

BILL TO: Pacific Commercial Services PO#
ADDRESS: PO Box 235117
CITY: Honolulu STATE: HI ZIP: 96823
ATTENTION: PHONE:

DATA TURNAROUND INFORMATION

DATA DELIVERABLE INFORMATION

ANALYSIS

FAX: _____ DAYS*
HARD COPY: _____ DAYS*
EDD _____ DAYS*
* TO BE APPROVED BY ALLIANCE
STANDARD TURNAROUND TIME IS 10 BUSINESS DAYS

☐ RESEULTS ONLY ☐ USEPA CLP
☐ RESULTS + QC ☐ New York State ASP "B"
☐ New Jersey REDUCED ☐ New York State ASP "A"
☐ New Jersey CLP ☐ Other _____
☐ EDD Format _____

TPH GC	GRO	VOC	PCB	Priority metals	TCLP metals	pH	Flash point	PAH
1	2	3	4	5	6	7	8	9

PRESERVATIVES

COMMENTS

<-- Specify Preservatives
A-HCl B-HNO3
C-H2SO4 D-NaOH
E-ICE F-Other

CHEMTECH SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# of Bottles										
			COMP	GRAB	DATE	TIME		1	2	3	4	5	6	7	8	9	
1.	304641-01-Wash water	liquid		X	11/4/25	8:45	9	X	X	X	X	X	X	X	X	X	
2.	304614-01-Fuel			X	11/4/25	8:45	1								X		
3.																	
4.																	
5.																	
6.																	
7.																	
8.																	
9.																	
10.																	

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE PROSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER 1. Anrit Krishna	DATE/TIME 11/4/25	RECEIVED BY 	Conditions of bottles or coolers at receipt: ☐ Compliant ☐ Non Compliant ☐ Cooler Temp 2.3°C MeOH extraction requires an additional 4oz. Jar for percent solid Comments: 13.7 + 0.2 = 13.9 (FEDER)	☐ Ice in Cooler?: YES
RELINQUISHED BY 2.	DATE/TIME 11/6/25 10:35	RECEIVED BY 2.		
RELINQUISHED BY 3.	DATE/TIME 11/7/25 9:40	RECEIVED FOR LAB BY 3.	SHIPPED VIA: CLIENT: ☐ Hand Delivered ☐ Overnight ALLIANCE: ☐ Picked Up ☐ Overnight	Shipment Complete ☐ YES ☐ NO

WHITE - ALLIANCE COPY FOR RETURN TO CLIENT YELLOW - ALLIANCE COPY PINK - SAMPLER COPY

Laboratory Certification

Certified By	License No.
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255425
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	TX-C25-00189
Virginia	460312

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q3574	PACI01	Order Date : 11/7/2025 10:02:13 AM	Project Mgr : Deepak
Client Name : Pacific Commercial Service		Project Name : Kilo Pier	Report Type : Level 2
Client Contact : Wendi Zheng		Receive DateTime : 11/7/2025 9:40:00 AM	EDD Type : EXCEL NOCLEANUP
Invoice Name : Pacific Commercial Service		Purchase Order :	Hard Copy Date :
Invoice Contact : Wendi Zheng			Date Signoff : 11/7/2025 11:34:12 AM

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q3574-01	304641-01 Liquid	Water	11/04/2025	08:45					
					Gasoline Range Organics		8015D		10 Bus. Days

Relinquished By : afDate / Time : 11/7/25 11:45Received By : SeemyDate / Time : 11/07/25 11:45

Storage Area : VOA Refridgerator Room


LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q3574	PACI01	Order Date : 11/7/2025 10:02:13 AM	Project Mgr : Deepak
Client Name : Pacific Commercial Service		Project Name : Kilo Pier	Report Type : Level 2
Client Contact : Wendi Zheng		Receive DateTime : 11/7/2025 9:40:00 AM	EDD Type : EXCEL NOCLEANUP
Invoice Name : Pacific Commercial Service		Purchase Order :	Hard Copy Date :
Invoice Contact : Wendi Zheng			Date Signoff : 11/7/2025 11:34:12 AM

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q3574-01	304641-01 Liquid	Water	11/04/2025	08:45	VOC-TCLVOA-10		8260-Low		10 Bus. Days

Relinquished By : 

Date / Time : 11/7/25 11:45

Received By : 

Date / Time : 11/7/25 11:45 Pg # 4

Storage Area : VOA Refridgerator Room