
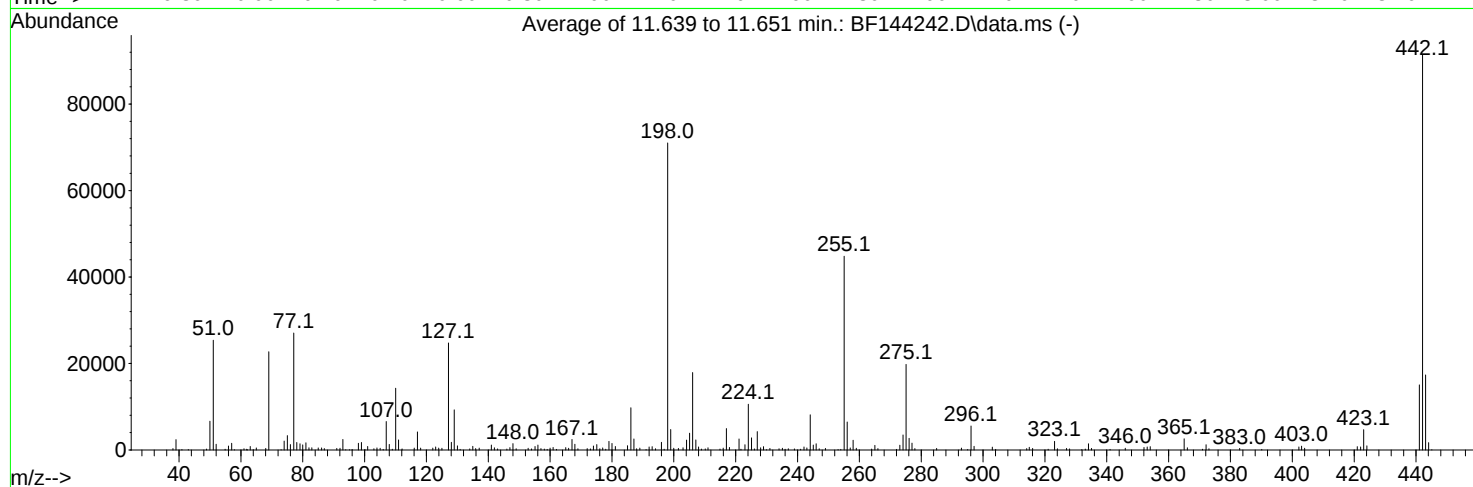


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111325\
Data File : BF144242.D
Acq On : 13 Nov 2025 14:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

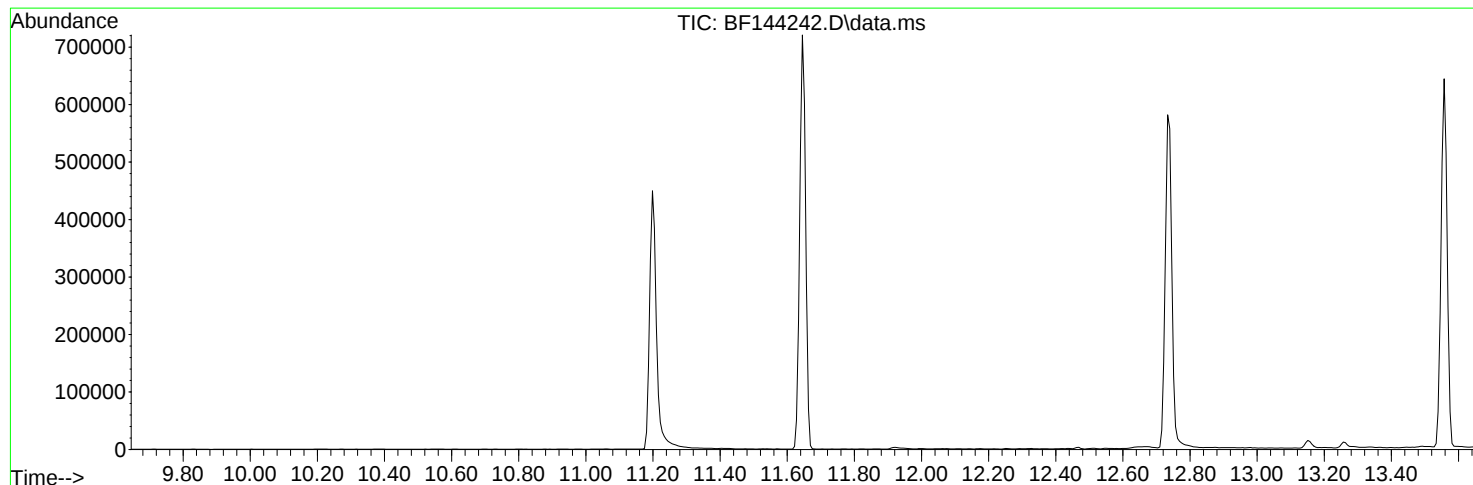




AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1600

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.5	342	PASS
69	69	100	100	100.0	22725	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.2	165	PASS
198	198	100	100	100.0	71013	PASS
199	198	5	9	6.7	4738	PASS
365	198	1	100	3.6	2591	PASS
441	443	0.01	150	86.9	15065	PASS
442	442	100	100	100.0	91344	PASS
443	442	15	24	19.0	17330	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111325\
Data File : BF144242.D
Acq On : 13 Nov 2025 14:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 13 15:07:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

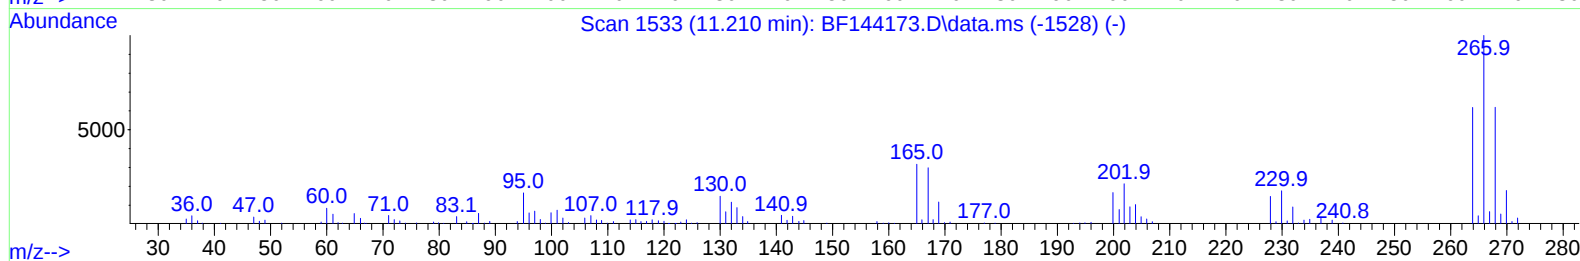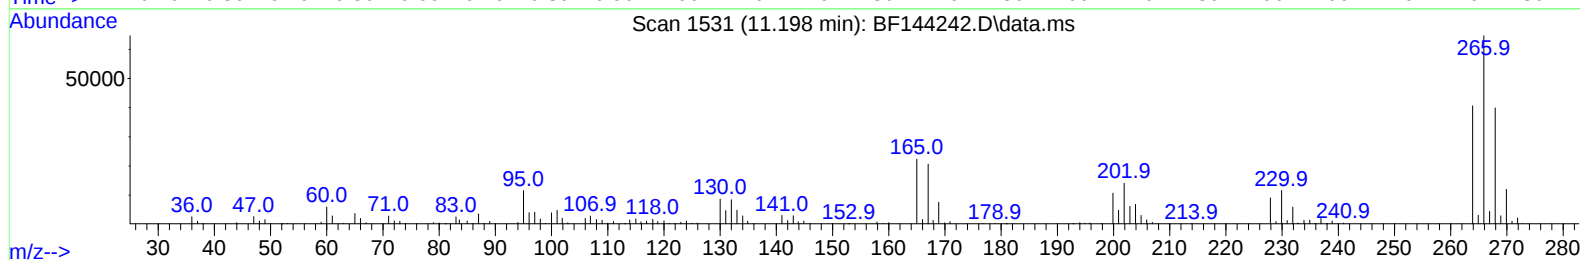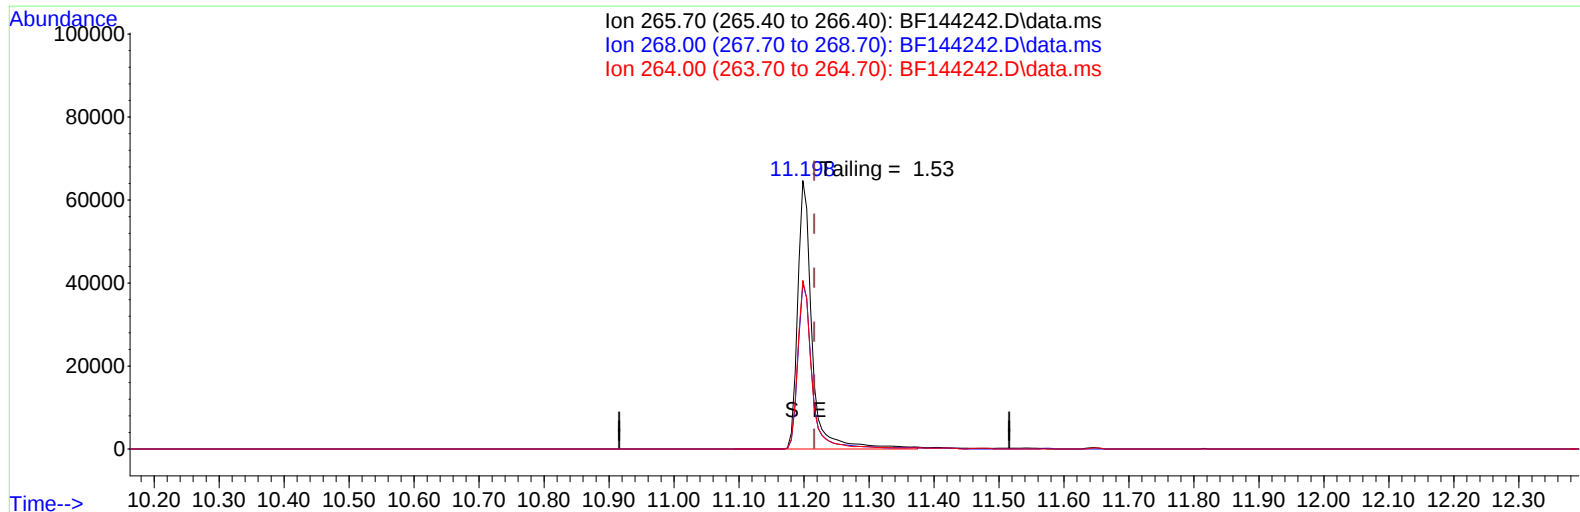

TIC: BF144242.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.017) 60191.23 ng




response 99588

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	61.71
264.00	61.80	62.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111325\
Data File : BF144242.D
Acq On : 13 Nov 2025 14:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 13 15:07:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

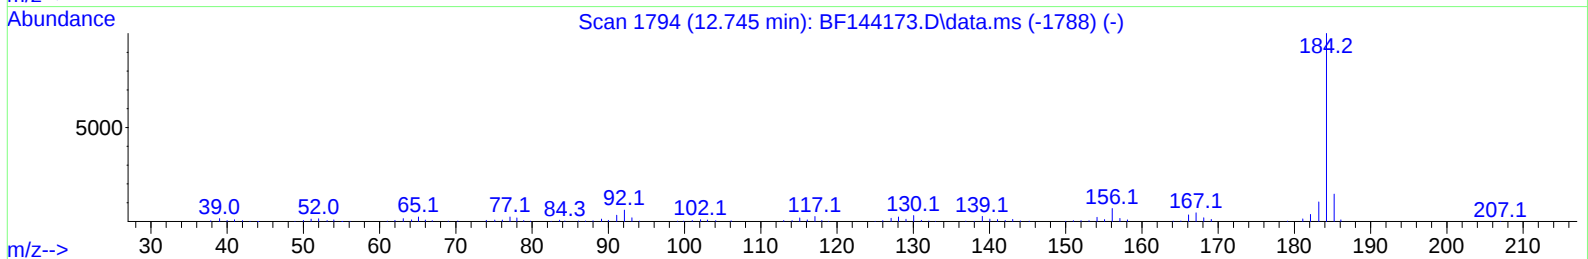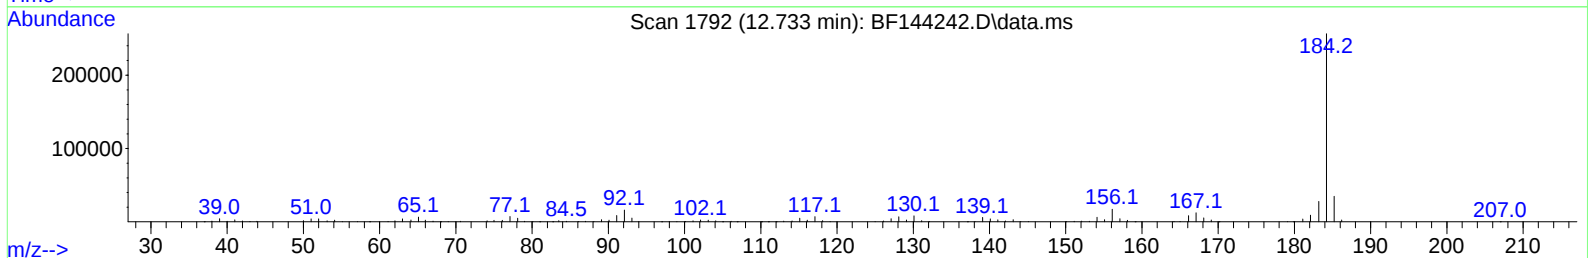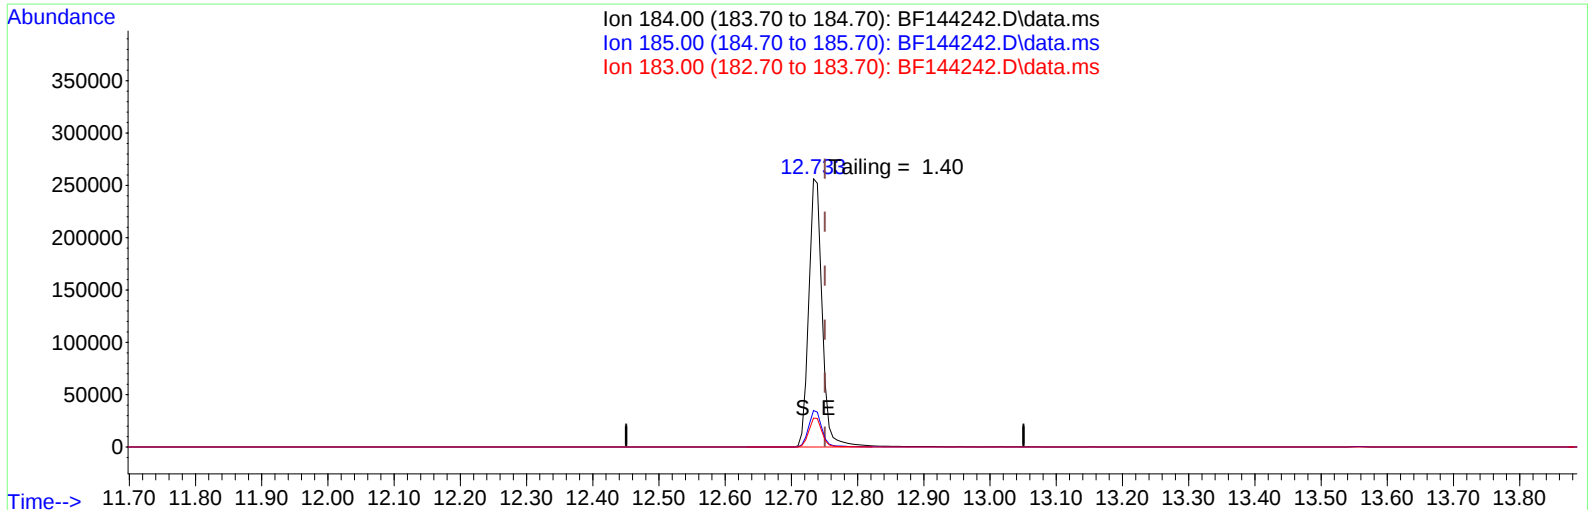

TIC: BF144242.D\data.ms

(77) Benzidine

12.733min (-0.017) 0.00 ng

response 363312

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.60
183.00	10.40	10.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/13/2025	BNA_F	<u>BF144242.D</u>
Compound Name	Response	Retention Time
DDT	171177	13.557
DDD	4877	13.257
DDE	191	12.928
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5068	176245	2.88

Instrument :
BNA_F
ClientSampleId :
DFTPP