


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111225\
Data File : BN038182.D
Acq On : 12 Nov 2025 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 29 13:09:46 2025

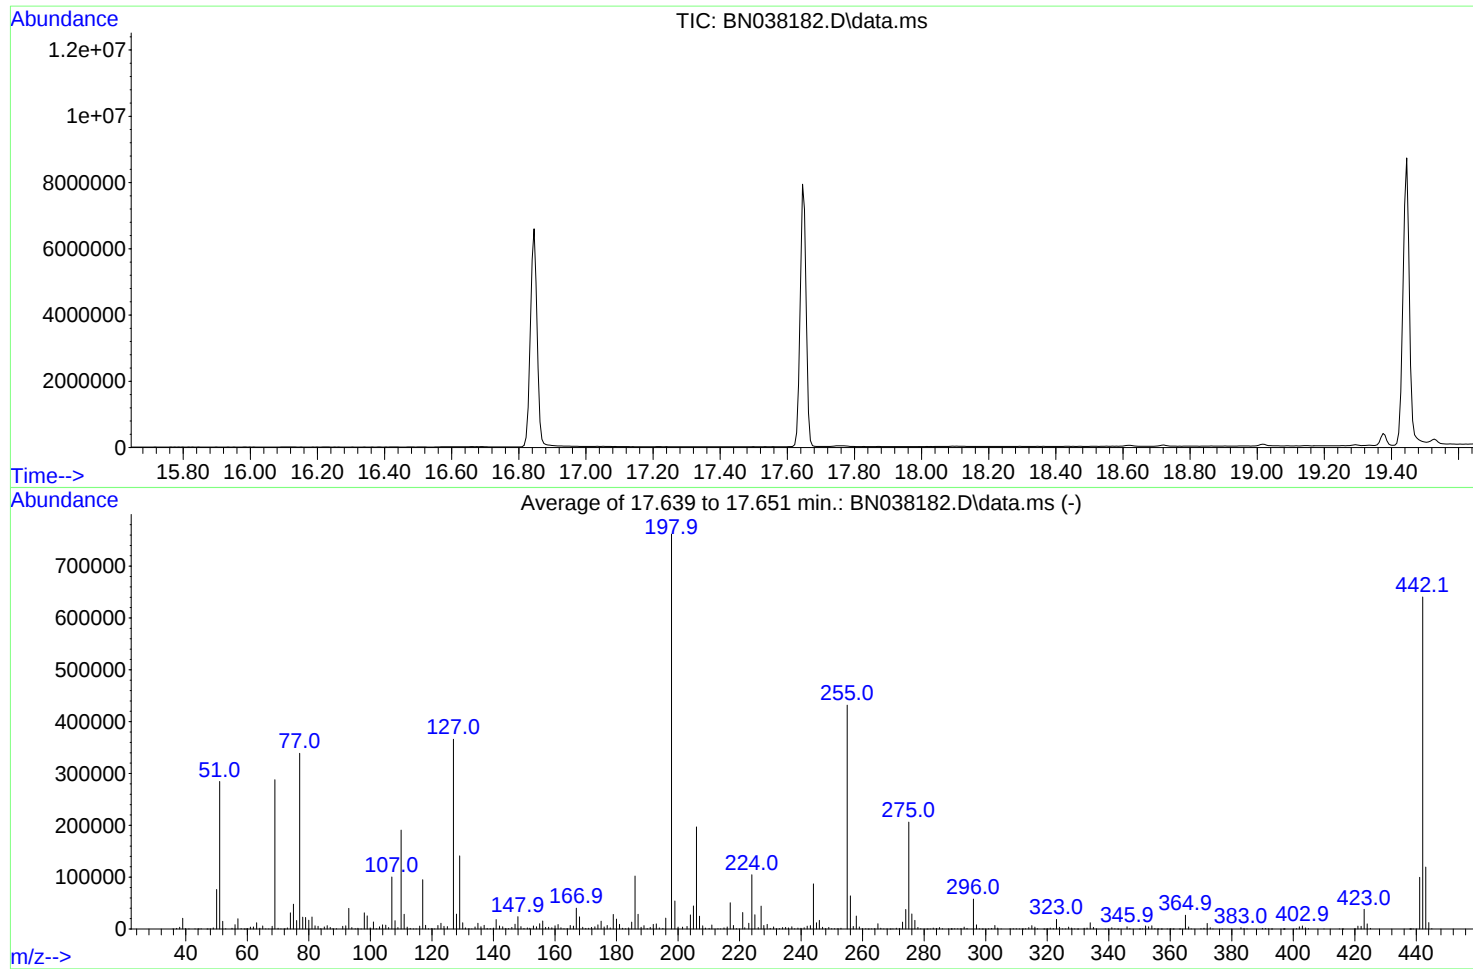

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	5354	PASS
69	69	100	100	100.0	287920	PASS
70	69	0.00	2	0.5	1437	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	761707	PASS
199	198	5	9	7.1	53917	PASS
365	198	1	100	3.5	26494	PASS
441	443	0.01	150	83.5	99787	PASS
442	442	100	100	100.0	640512	PASS
443	442	15	24	18.6	119448	PASS