

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111325\
 Data File : BF144244.D
 Acq On : 13 Nov 2025 15:25
 Operator : RC/JU
 Sample : PB170473BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB170473BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	489	496	509	rBV	14232	24684	1.27%	0.204%
2	5.492	556	561	588	rBV	1146669	1596327	82.21%	13.172%
3	6.498	726	732	751	rBV	1124184	1627688	83.83%	13.431%
4	6.863	789	794	805	rVB	268525	337739	17.39%	2.787%
5	7.428	884	890	908	rBV	774534	1037948	53.46%	8.565%
6	8.145	1007	1012	1020	rBV	341110	443322	22.83%	3.658%
7	9.222	1189	1195	1217	rBV	1483418	1941711	100.00%	16.022%
8	9.904	1306	1311	1324	rBV	412855	518090	26.68%	4.275%
9	10.698	1440	1446	1480	rBV	921549	1286795	66.27%	10.618%
10	11.392	1559	1564	1584	rVB	404734	535355	27.57%	4.418%
11	12.986	1829	1835	1840	rBV	1331973	1807471	93.09%	14.915%
12	13.892	1973	1989	2006	rBV5	11973	66320	3.42%	0.547%
13	14.045	2009	2015	2026	rVB	218786	307574	15.84%	2.538%
14	15.321	2227	2232	2246	rVB8	10189	32017	1.65%	0.264%
15	15.521	2260	2266	2280	rBV	214032	353610	18.21%	2.918%
16	16.486	2425	2430	2437	rVB3	12161	23475	1.21%	0.194%
17	17.192	2540	2550	2566	rVB2	36831	158141	8.14%	1.305%
18	17.798	2649	2653	2664	rVB6	7814	20527	1.06%	0.169%




Sum of corrected areas: 12118794

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111325\
Data File : BF144244.D
Acq On : 13 Nov 2025 15:25
Operator : RC/JU
Sample : PB170473BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

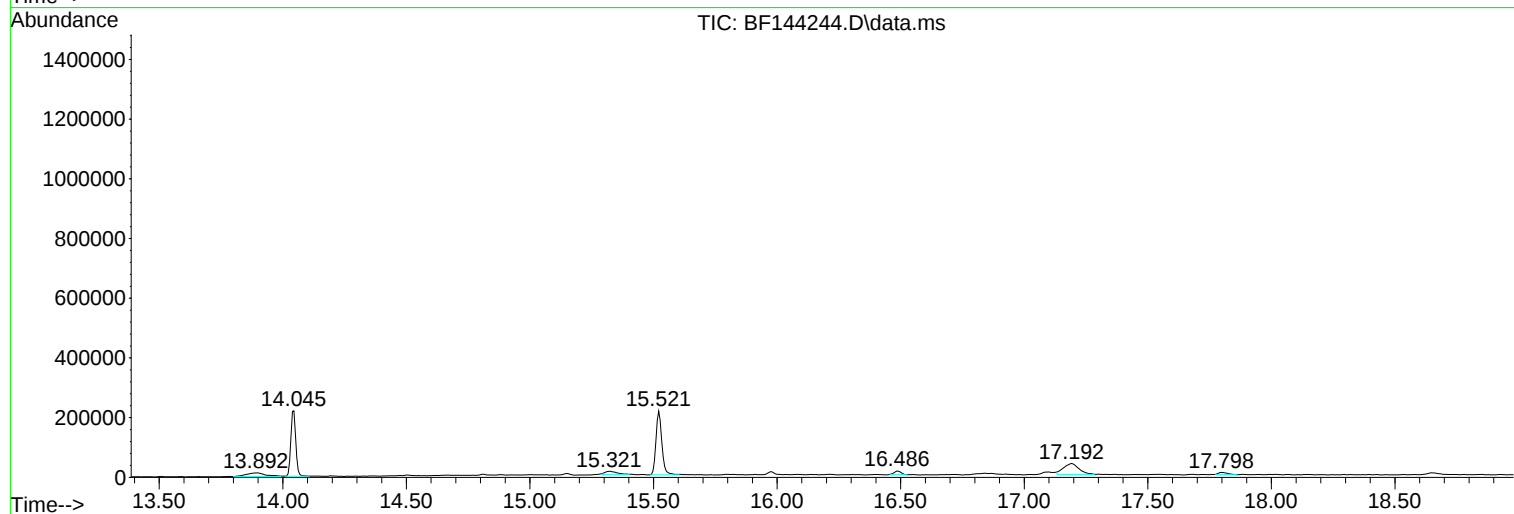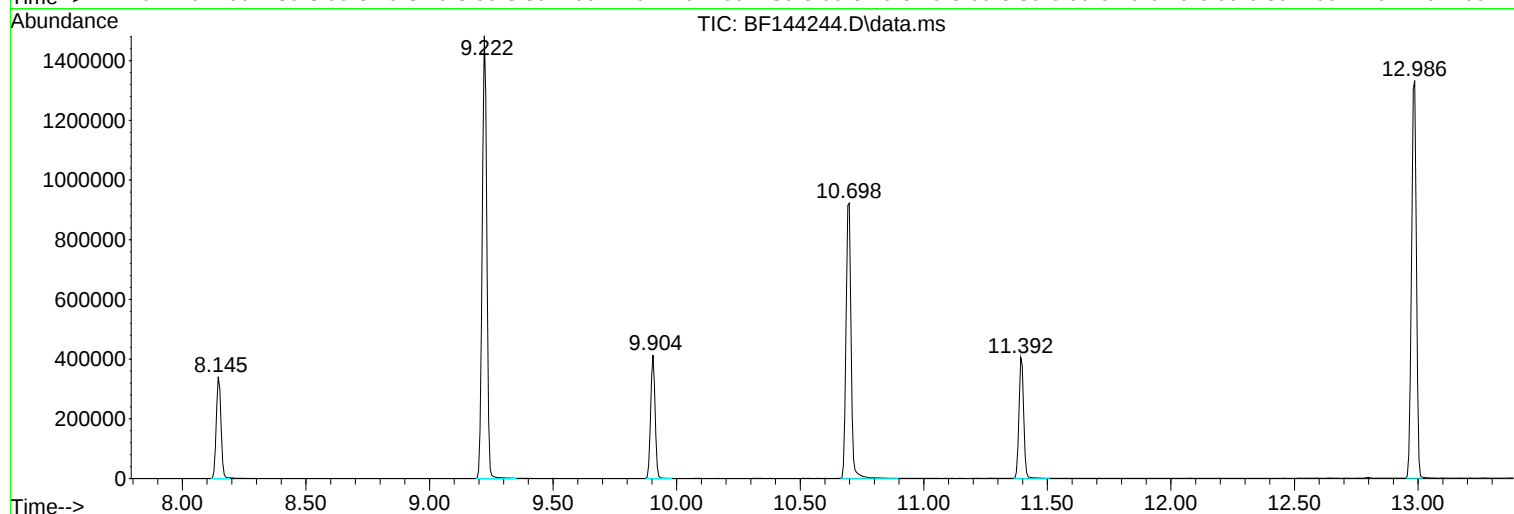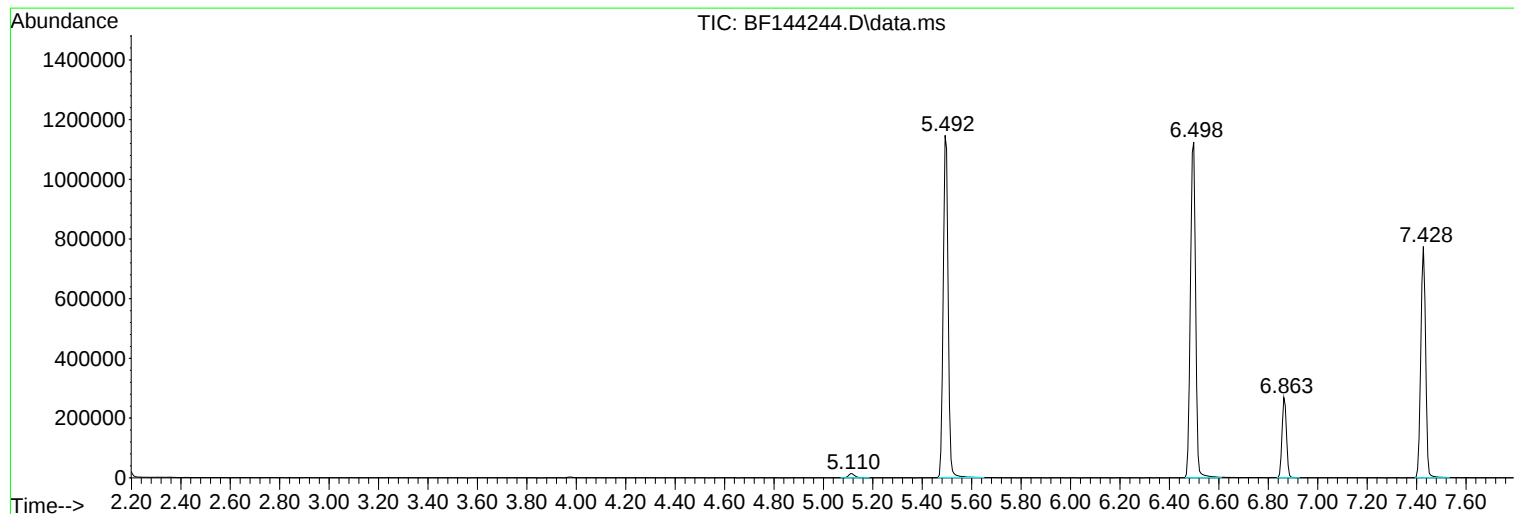

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111325\
Data File : BF144244.D
Acq On : 13 Nov 2025 15:25
Operator : RC/JU
Sample : PB170473BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111325\
Data File : BF144244.D
Acq On : 13 Nov 2025 15:25
Operator : RC/JU
Sample : PB170473BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------