
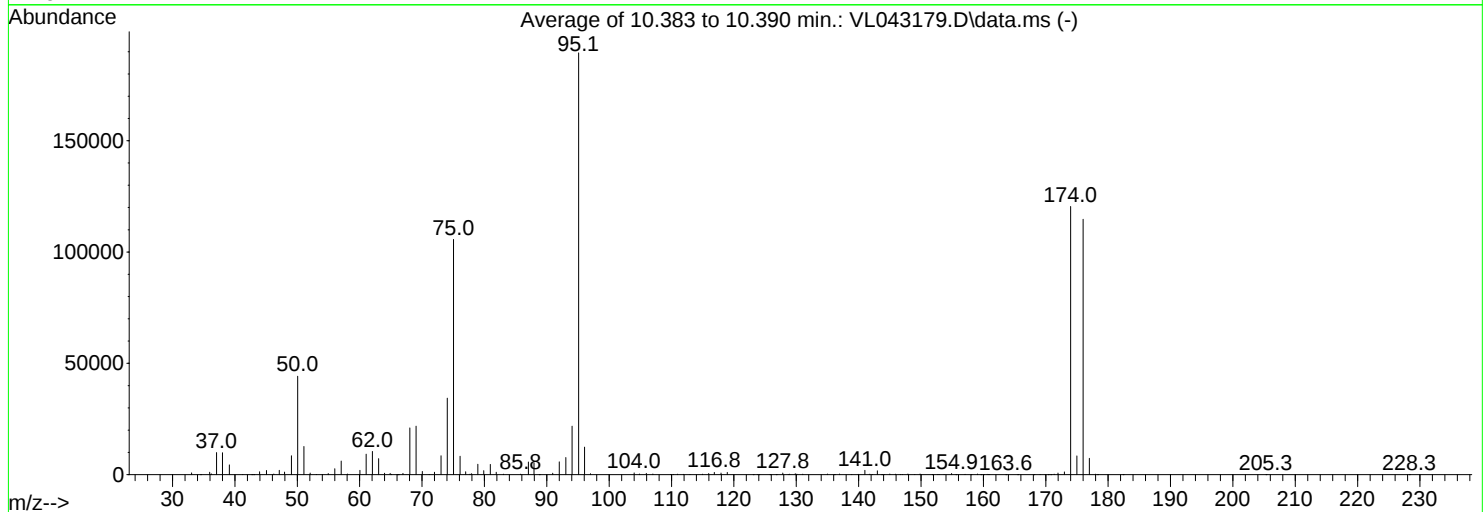


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL111125\
Data File : VL043179.D
Acq On : 11 Nov 2025 07:30
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL101425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Oct 15 02:12:58 2025

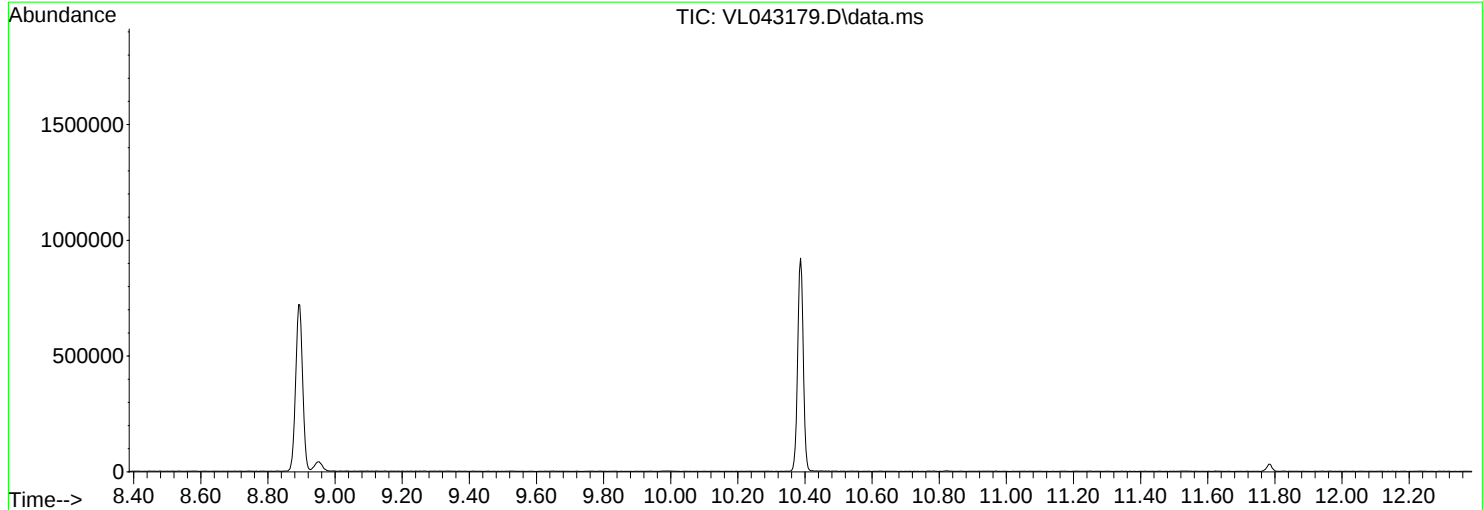

AutoFind: Scans 3181, 3182, 3183; Background Corrected with Scan 3168

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.3	44243	PASS
75	95	30	66	55.7	105627	PASS
95	95	100	100	100.0	189483	PASS
96	95	5	9	6.5	12377	PASS
173	174	0.00	2	1.0	1260	PASS
174	95	50	120	63.6	120448	PASS
175	174	4	9	7.0	8399	PASS
176	174	93	101	95.2	114699	PASS
177	176	5	9	6.4	7339	PASS

Average of 10.383 to 10.390 min.: VL043179.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.05	814	45.05	1844	56.00	2648	66.20	31
34.50	33	46.25	278	57.05	6120	66.95	59
35.95	1073	47.10	1977	58.05	261	68.05	2102
36.20	355	47.95	1147	60.05	1953	69.05	2181
37.05	9914	49.05	8494	61.05	9194	70.05	1417
38.00	9816	50.05	44243	62.05	10407	71.15	64
39.10	4381	51.05	12690	63.05	7207	72.00	1105
41.25	75	52.05	693	64.00	672	73.05	8513
42.70	31	53.05	104	64.90	562	74.05	34336
43.00	39	54.05	86	65.10	155	75.05	105627
43.95	1314	54.95	514	66.00	27	76.10	8302

Average of 10.383 to 10.390 min.: VL043179.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	1276	88.80	33	107.00	279	123.10	36
77.70	215	90.95	655	109.85	91	123.75	97
77.95	405	92.00	5746	110.30	99	124.00	29
78.95	4651	93.05	7735	110.95	225	125.80	18
79.90	1769	94.05	21797	111.90	139	126.80	34
80.95	4595	95.10	189483	112.95	92	127.85	747
81.90	1050	96.05	12377	114.95	191	128.70	52
83.05	250	97.00	416	115.95	490	128.95	213
85.80	244	104.00	813	116.85	1033	129.85	407
87.05	5701	104.85	261	117.95	733	130.10	205
87.95	5305	105.95	594	118.95	979	131.05	203

Average of 10.383 to 10.390 min.: VL043179.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
135.00	289	145.00	275	154.90	539	165.50	19
136.10	37	145.90	193	155.60	37	168.10	18
136.95	278	146.70	46	157.05	172	169.10	52
138.90	108	147.00	76	158.00	19	169.90	100
139.95	126	147.90	323	159.05	287	170.40	39
141.00	1919	149.00	42	159.60	26	170.80	26
141.80	218	149.85	323	160.00	24	171.35	211
142.20	69	151.80	22	160.60	125	171.95	737
143.00	1726	152.70	74	160.80	97	173.00	1260
143.70	28	152.90	79	161.00	60	174.00	120448
144.10	69	153.70	42	163.60	35	175.00	8399

Average of 10.383 to 10.390 min.: VL043179.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.00	114699						
177.00	7339						
178.00	205						
178.30	38						
182.40	28						
205.30	18						
228.30	26						