


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112625\
Data File : BF144357.D
Acq On : 26 Nov 2025 13:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

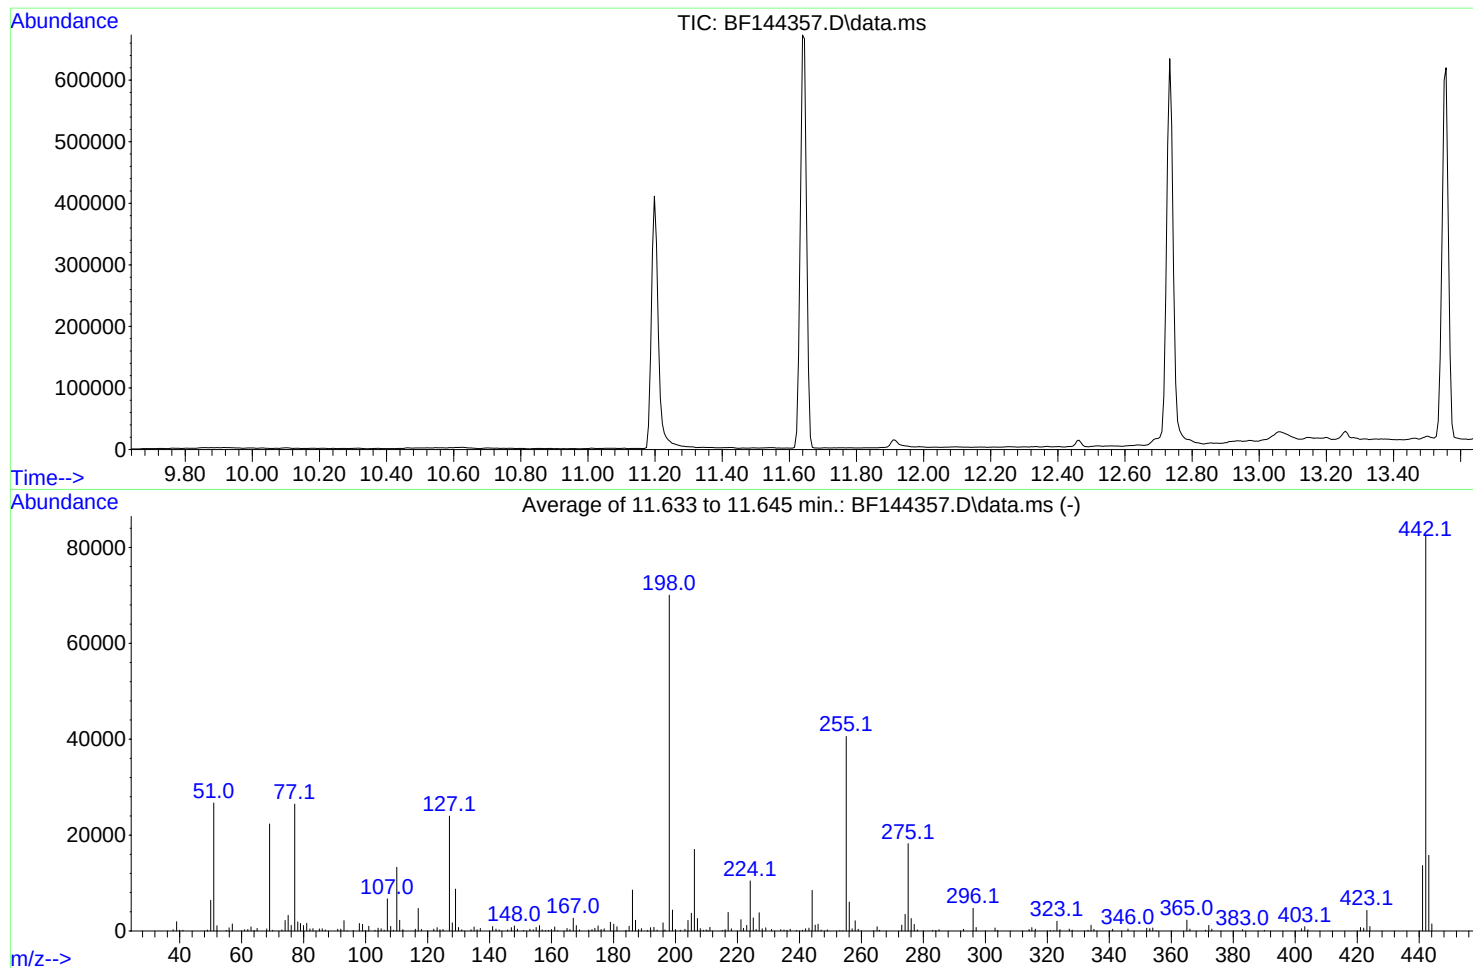

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	434	PASS
69	69	100	100	100.0	22312	PASS
70	69	0.00	2	0.8	175	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70035	PASS
199	198	5	9	6.2	4374	PASS
365	198	1	100	3.2	2260	PASS
441	443	0.01	150	86.5	13647	PASS
442	442	100	100	100.0	82341	PASS
443	442	15	24	19.2	15775	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/26/2025	BNA_F	<u>BF144357.D</u>
Compound Name	Response	Retention Time
DDT	170867	13.557
DDD	5037	13.257
DDE	501	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5538	176405	3.14

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112625\
Data File : BF144357.D
Acq On : 26 Nov 2025 13:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 26 13:20:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

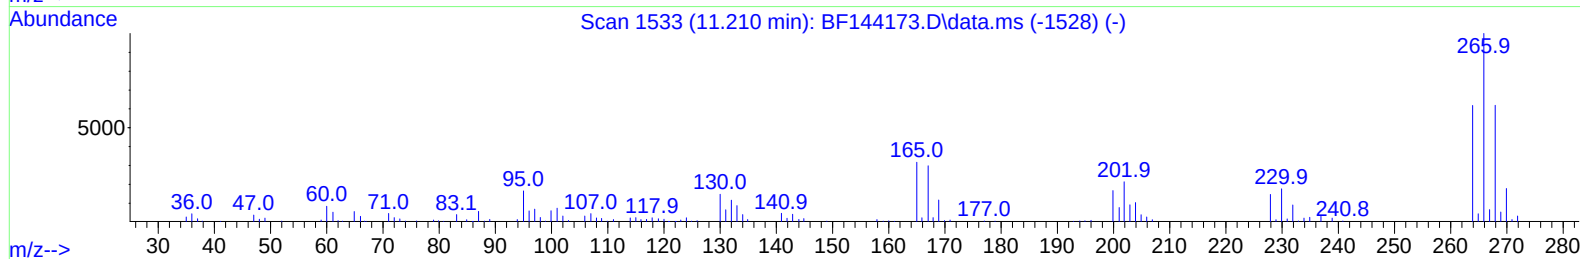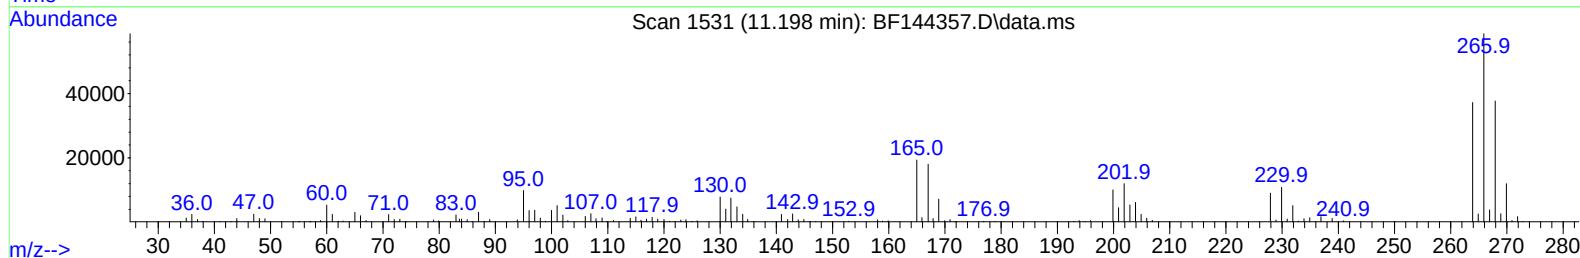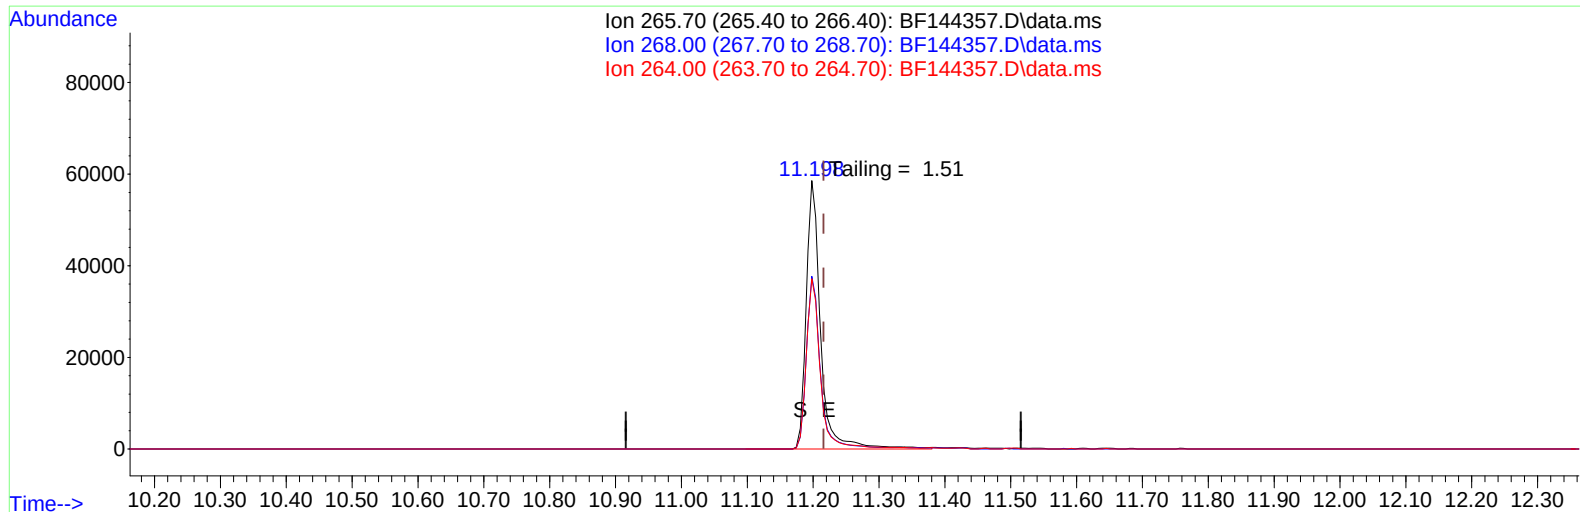

TIC: BF144357.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.018) 39088.69 ng




response 89255

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	64.33
264.00	61.80	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112625\
Data File : BF144357.D
Acq On : 26 Nov 2025 13:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 26 13:20:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

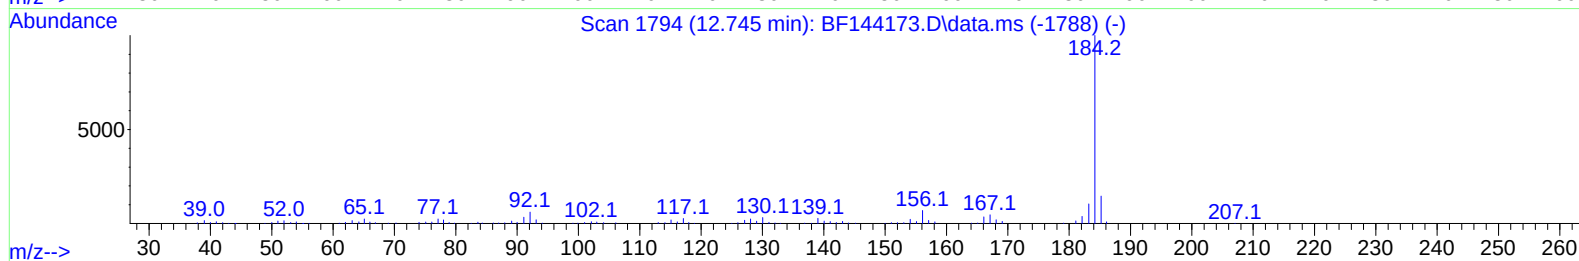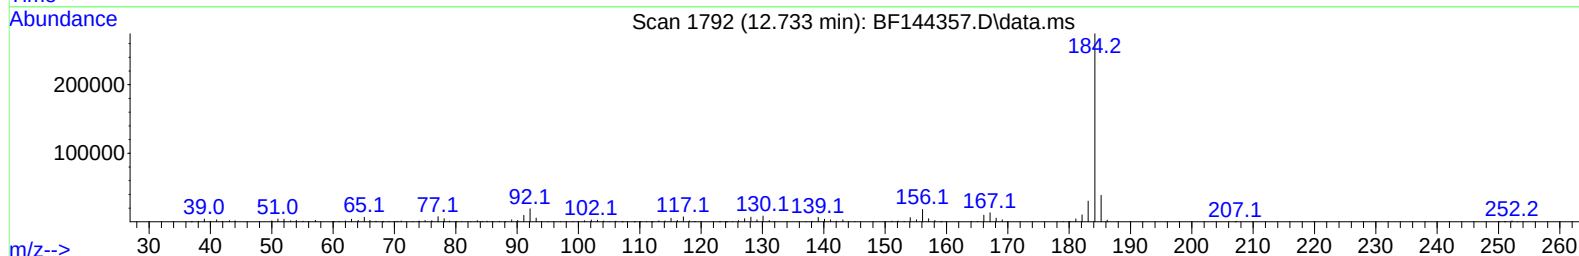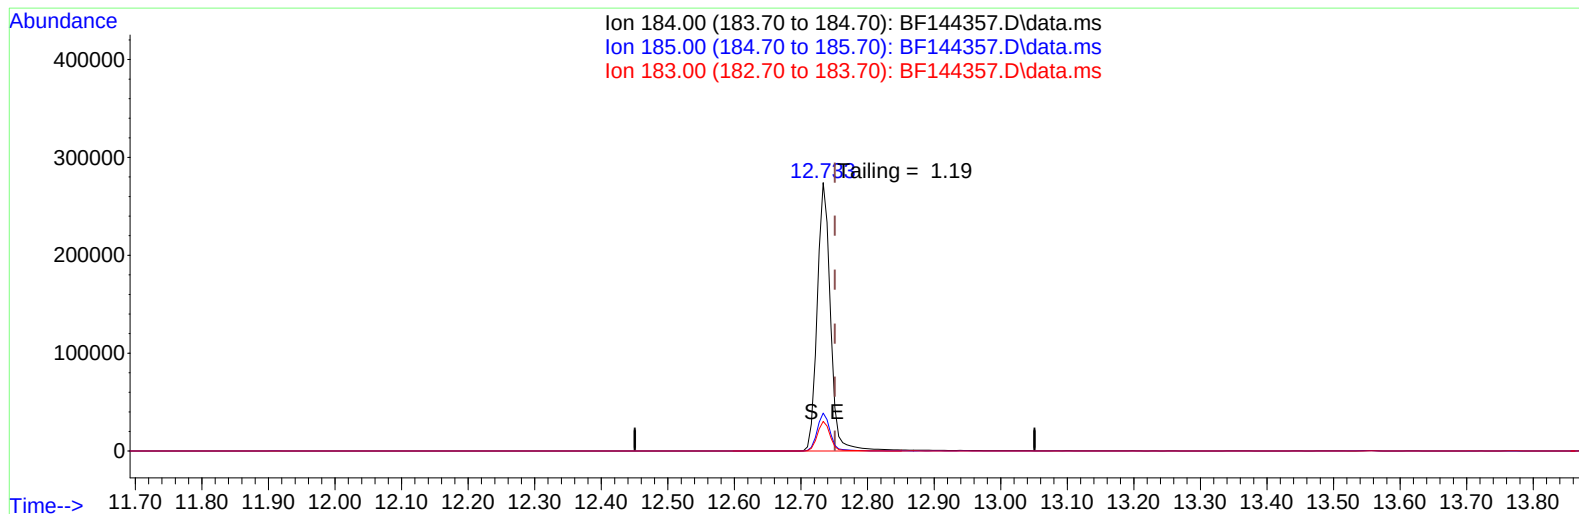

TIC: BF144357.D\data.ms

(77) Benzidine

12.733min (-0.018) 0.00 ng

response 380762

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.14
183.00	10.40	11.08
0.00	0.00	0.00