


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120125\
Data File : BP026196.D
Acq On : 01 Dec 2025 12:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 19 01:25:31 2025

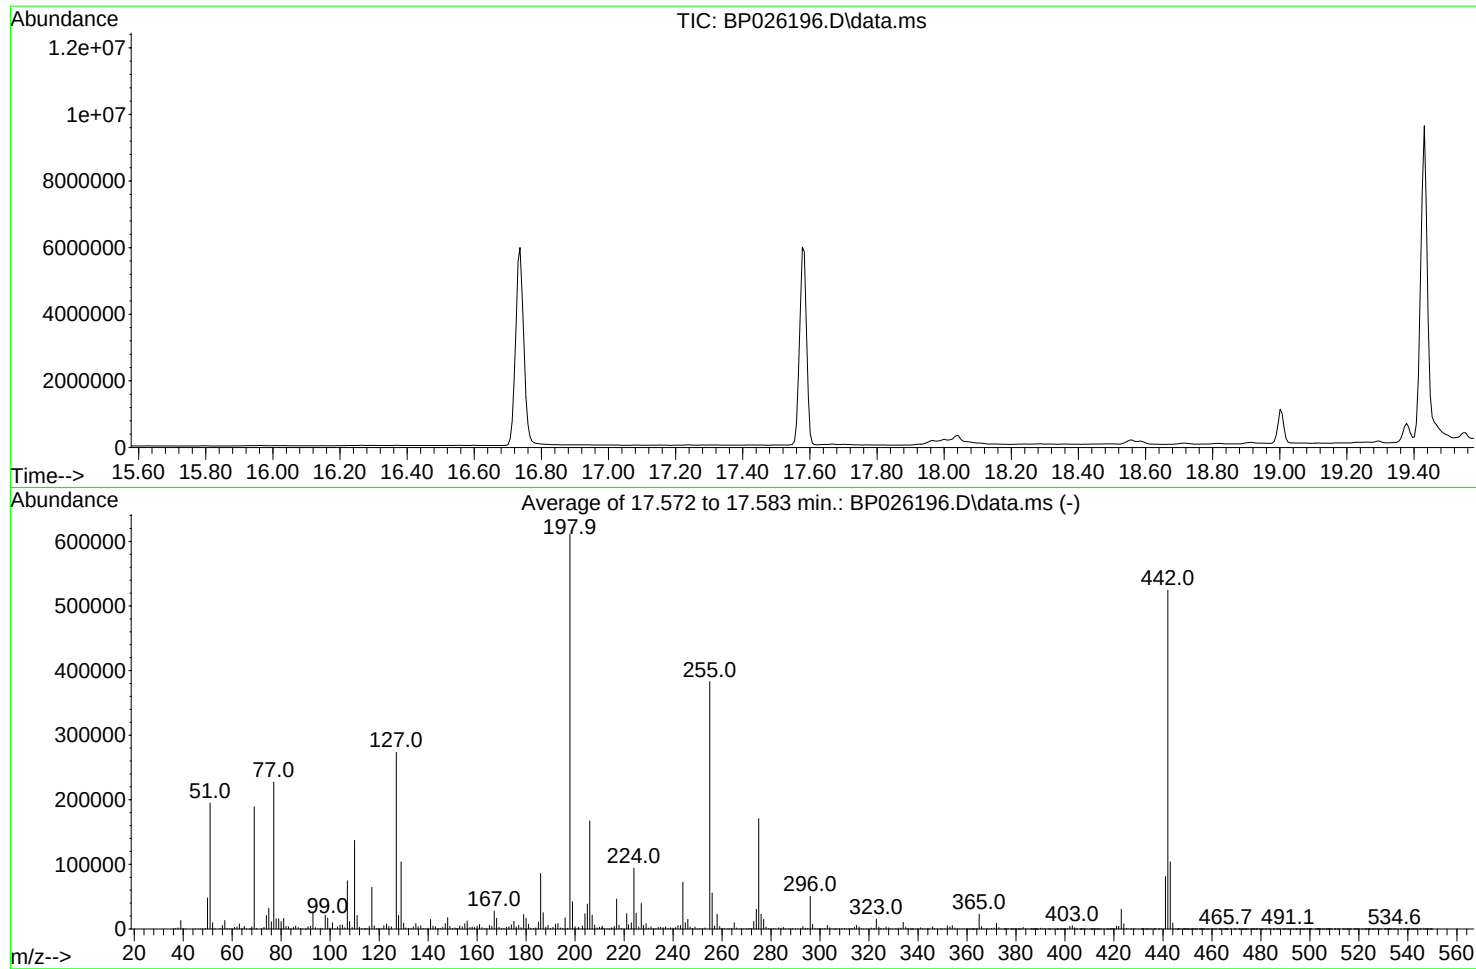




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2478

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	3456	PASS
69	69	100	100	100.0	189224	PASS
70	69	0.00	2	0.4	845	PASS
197	198	0.00	2	0.2	1172	PASS
198	198	100	100	100.0	611343	PASS
199	198	5	9	6.9	42128	PASS
365	198	1	100	3.7	22761	PASS
441	443	0.01	150	77.9	80939	PASS
442	442	100	100	100.0	524437	PASS
443	442	15	24	19.8	103887	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120125\
Data File : BP026196.D
Acq On : 01 Dec 2025 12:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 01 13:09:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

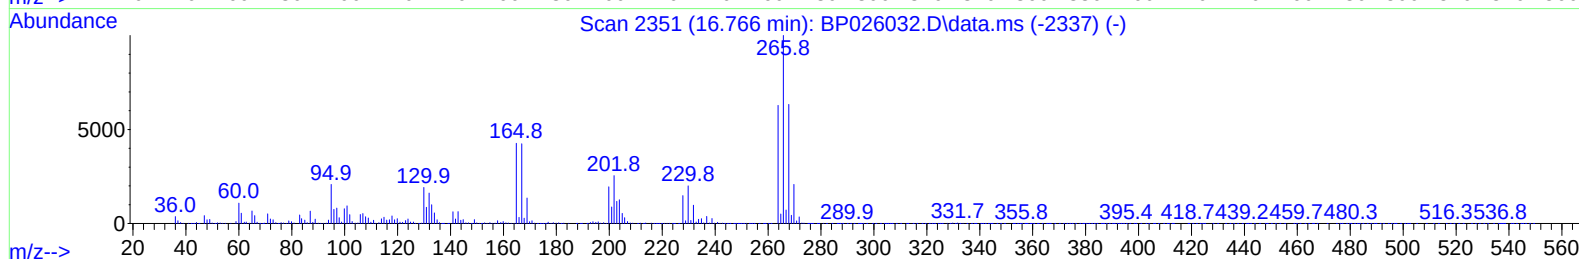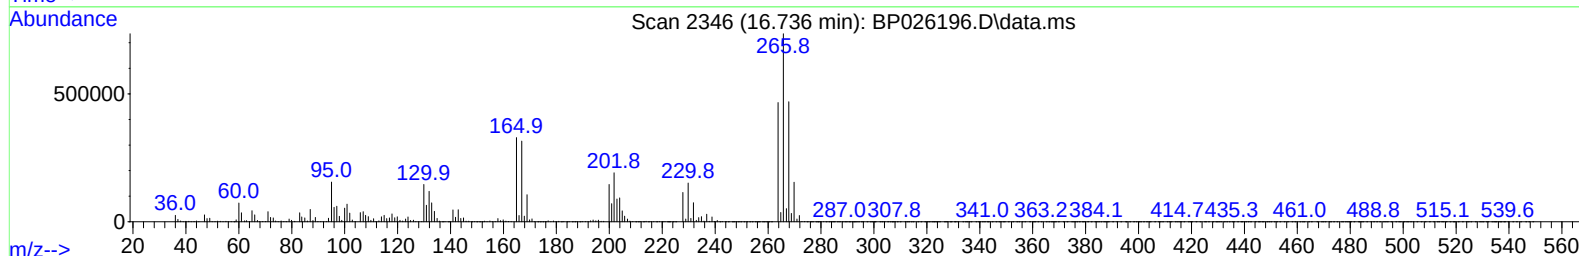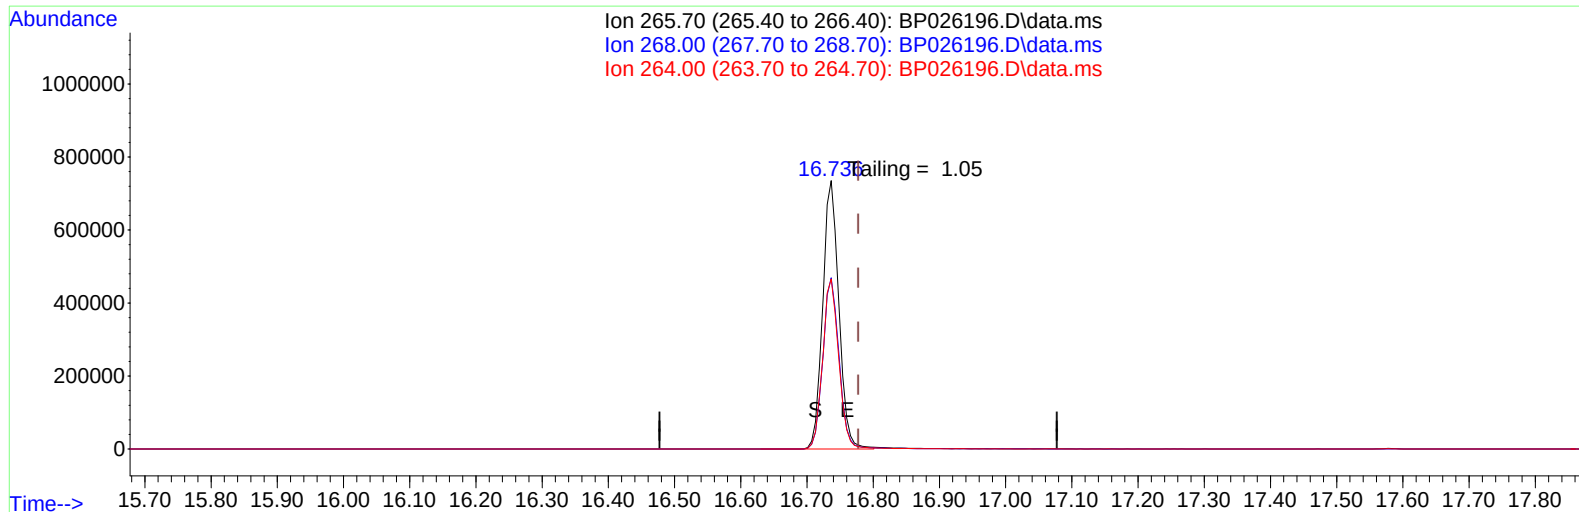

TIC: BP026196.D\data.ms

(70) Pentachlorophenol (C)

16.736min (-0.041) 24101.08 ng


response 1253121

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.81
264.00	62.70	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120125\
Data File : BP026196.D
Acq On : 01 Dec 2025 12:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 01 13:09:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

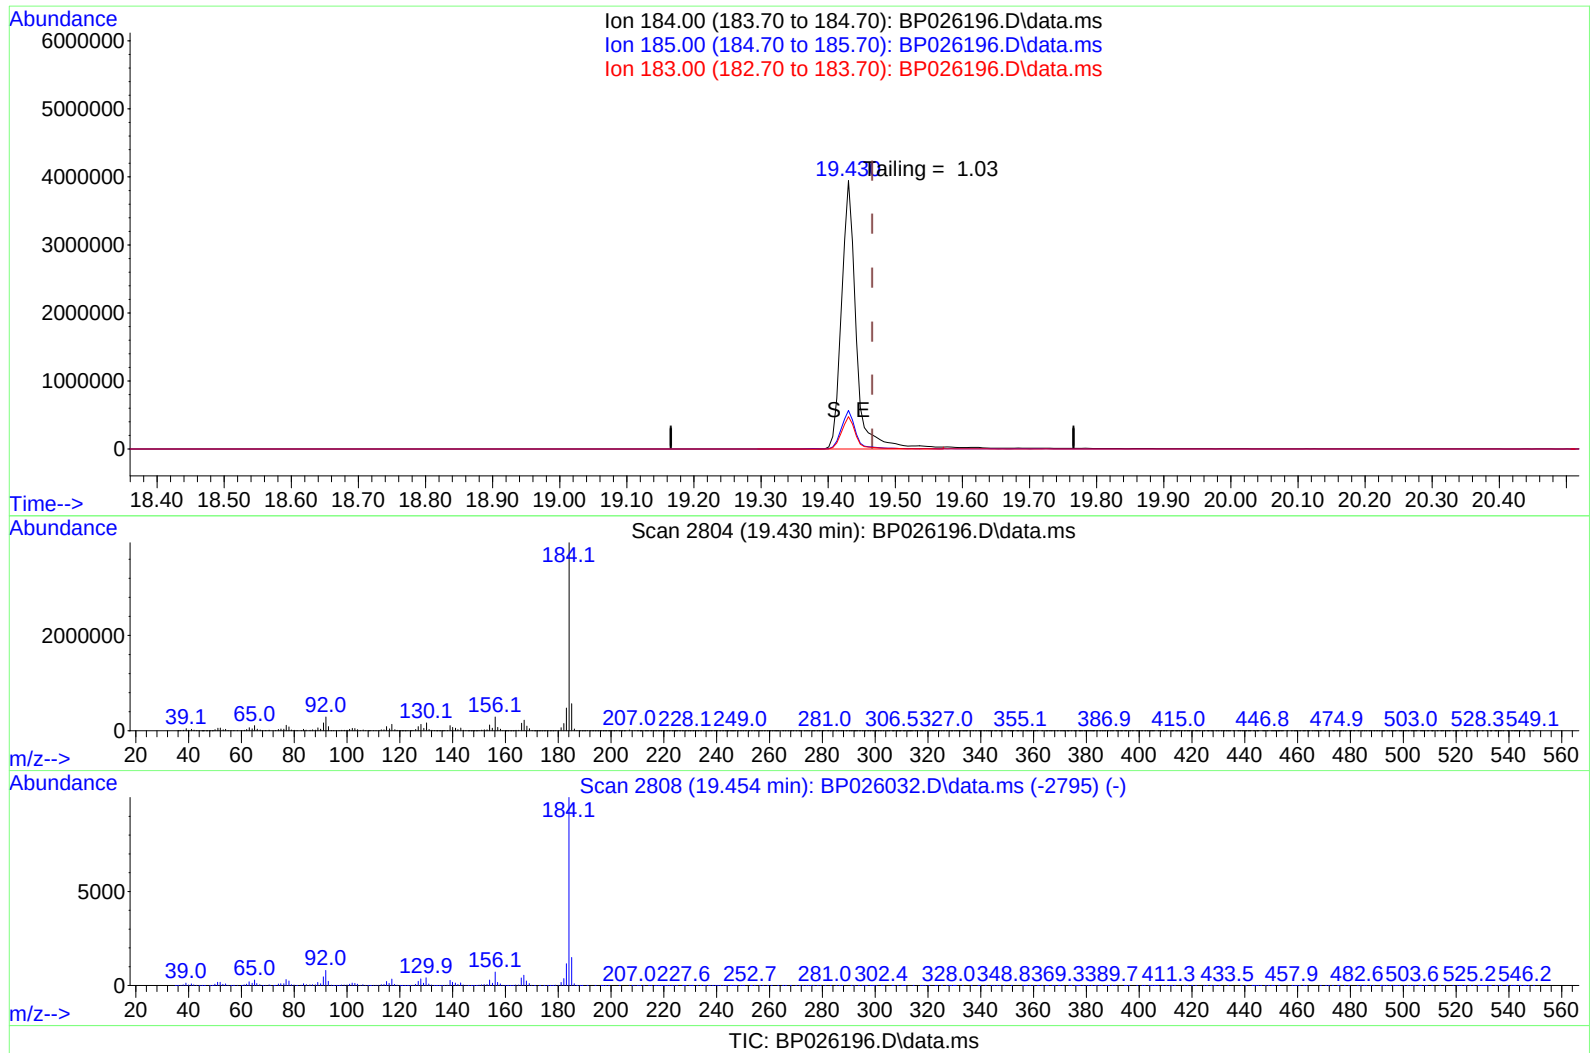

(77) Benzidine

19.430min (-0.035) 1977.46 ng

response 5896454

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.37
183.00	11.30	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2025	BNA_P	<u>BP026196.D</u>
Compound Name	Response	Retention Time
DDT	2964416	20.742
DDD	50794	20.271
DDE	6617	19.736
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
57411	3021827	1.90

Instrument :
BNA_P
ClientSampleId :
DFTPP