

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112625\
 Data File : BF144359.D
 Acq On : 26 Nov 2025 14:00
 Operator : RC/JU
 Sample : PB170735BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB170735BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.093	486	493	511	rBV	315959	508465	26.01%	3.934%
2	5.493	556	561	590	rBV	1115698	1556363	79.61%	12.042%
3	6.498	726	732	751	rBV	1095602	1570333	80.32%	12.151%
4	6.863	789	794	801	rBV	283681	367528	18.80%	2.844%
5	7.422	883	889	908	rBV	739135	1011102	51.72%	7.823%
6	8.140	1006	1011	1020	rBV	358323	479865	24.54%	3.713%
7	9.222	1188	1195	1200	rBV	1440340	1955055	100.00%	15.127%
8	9.898	1305	1310	1318	rBV	450737	579329	29.63%	4.483%
9	10.692	1440	1445	1467	rBV	949877	1274674	65.20%	9.863%
10	11.392	1559	1564	1571	rBV	471931	600241	30.70%	4.644%
11	12.980	1828	1834	1839	rBV	1476203	1930217	98.73%	14.935%
12	13.880	1971	1987	1999	rBV6	17962	94361	4.83%	0.730%
13	14.039	2009	2014	2021	rBV	289013	385924	19.74%	2.986%
14	15.521	2260	2266	2279	rVB	286158	461387	23.60%	3.570%
15	17.180	2541	2548	2564	rVB2	39181	149123	7.63%	1.154%




Sum of corrected areas: 12923967

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112625\
Data File : BF144359.D
Acq On : 26 Nov 2025 14:00
Operator : RC/JU
Sample : PB170735BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170735BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

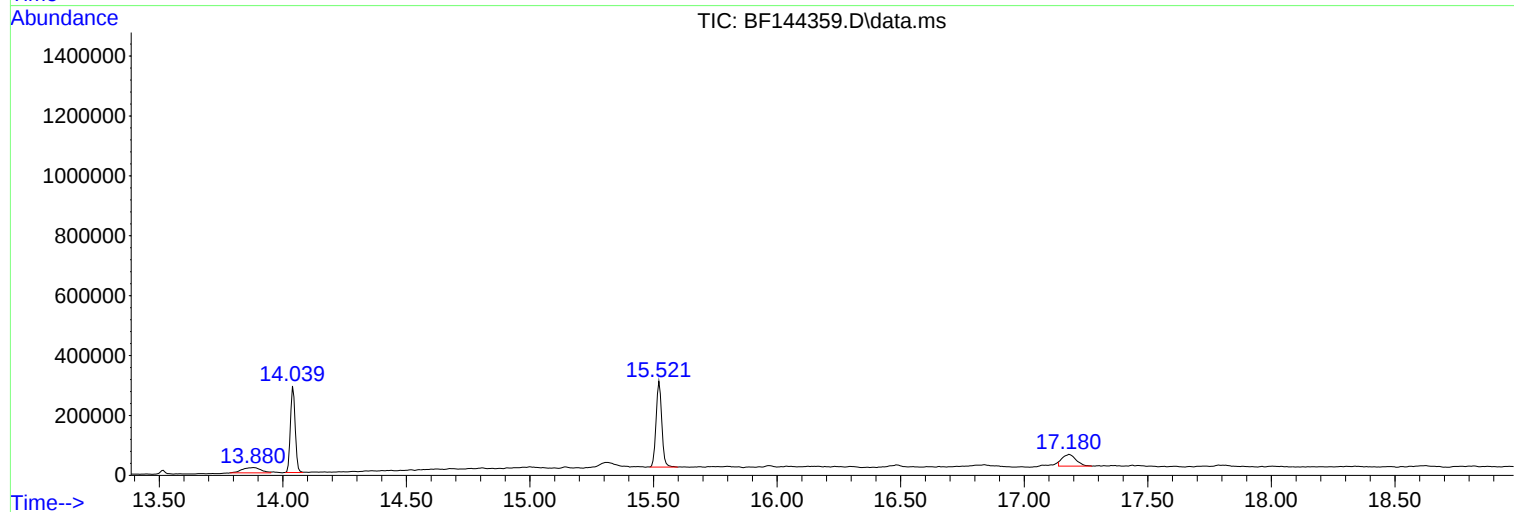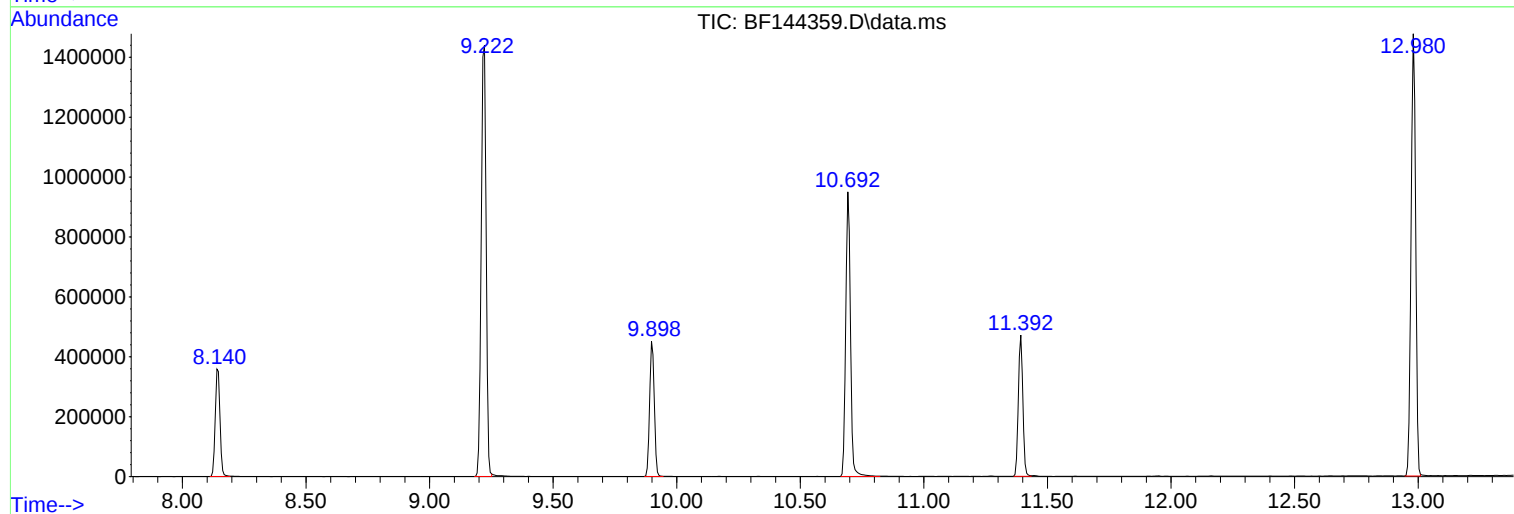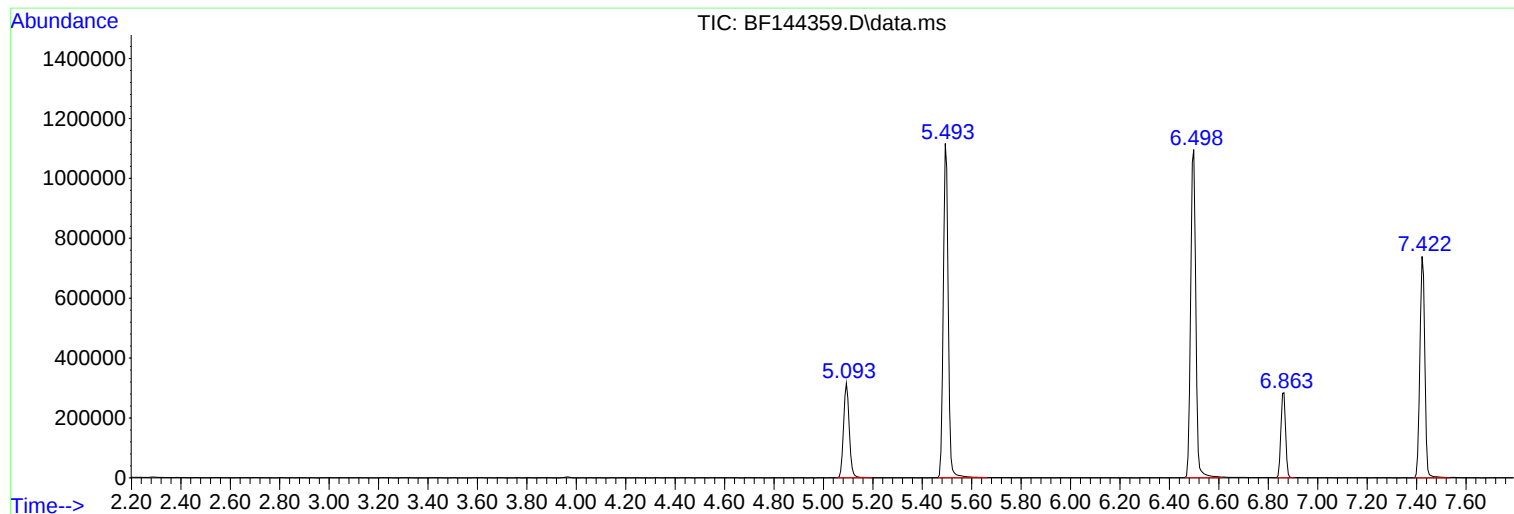

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112625\
Data File : BF144359.D
Acq On : 26 Nov 2025 14:00
Operator : RC/JU
Sample : PB170735BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170735BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112625\
Data File : BF144359.D
Acq On : 26 Nov 2025 14:00
Operator : RC/JU
Sample : PB170735BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170735BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------