
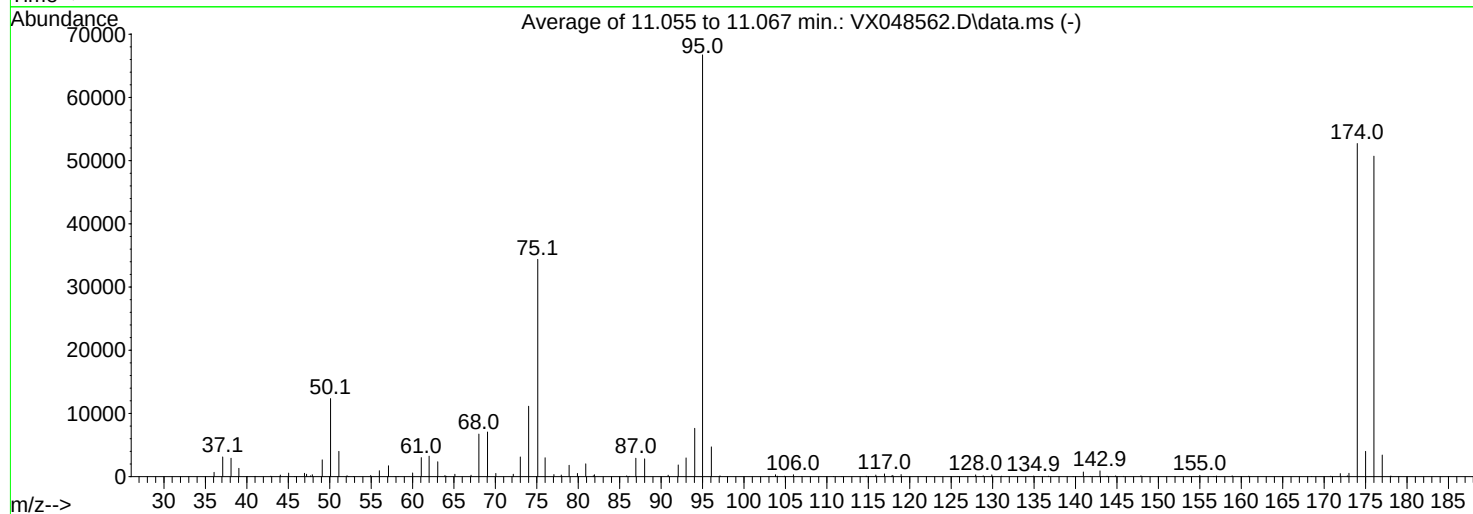


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111225\
Data File : VX048562.D
Acq On : 12 Nov 2025 08:08
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
Title : SW846 8260
Last Update : Sat Nov 08 05:08:11 2025

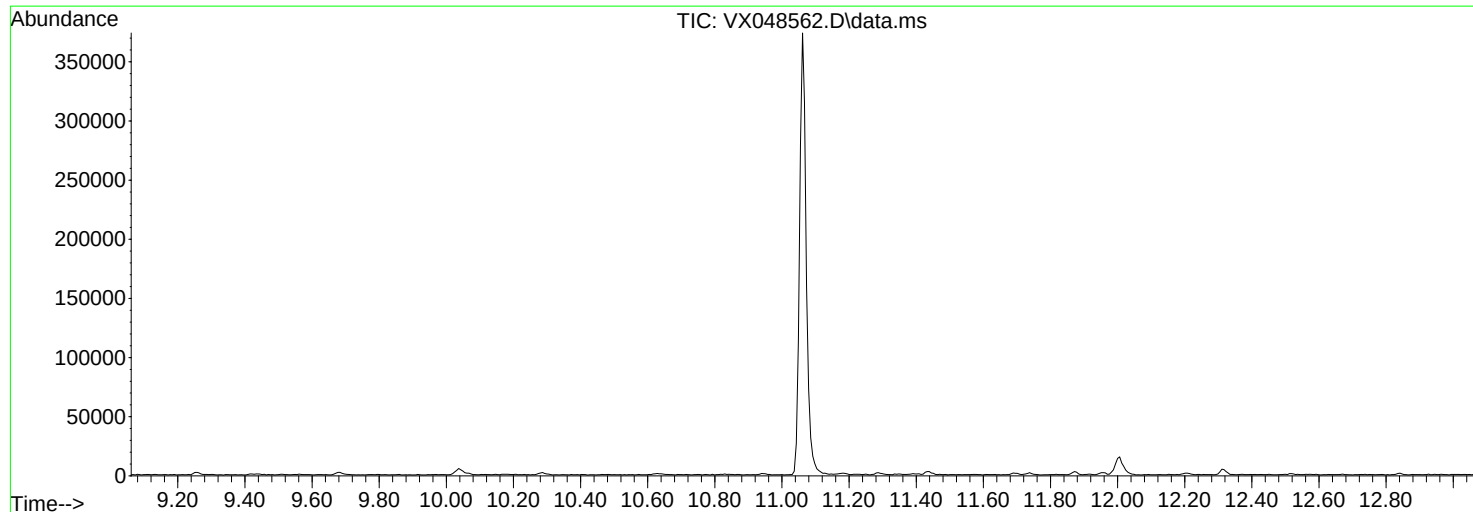

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	12354	PASS
75	95	30	60	51.5	34373	PASS
95	95	100	100	100.0	66749	PASS
96	95	5	9	7.1	4719	PASS
173	174	0.00	2	1.0	544	PASS
174	95	50	100	79.0	52731	PASS
175	174	5	9	7.6	3999	PASS
176	174	95	101	96.2	50712	PASS
177	176	5	9	6.7	3409	PASS