
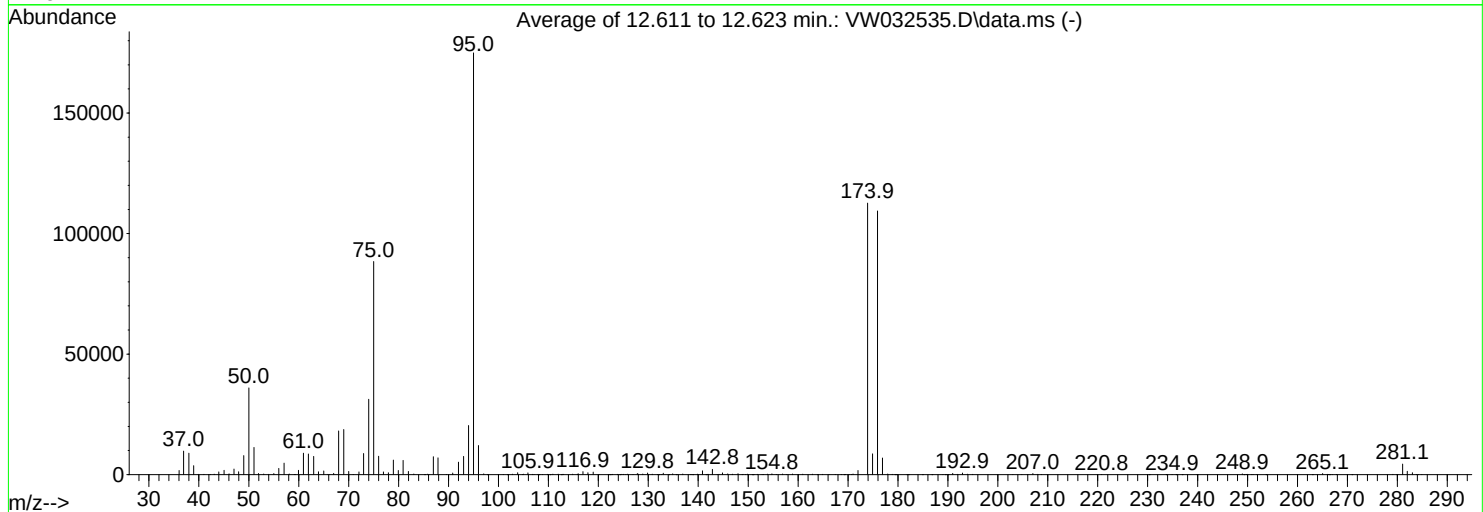


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112625\
Data File : VW032535.D
Acq On : 26 Nov 2025 11:05
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111025S.M
Title : SW846 8260
Last Update : Tue Nov 11 03:48:21 2025

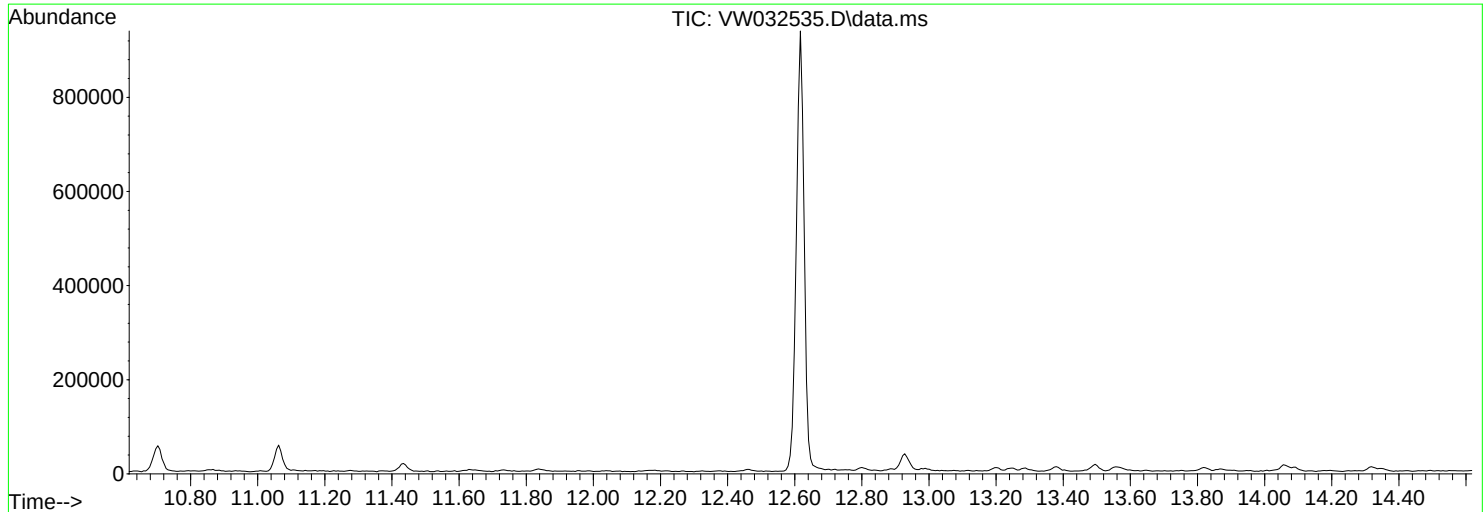

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	35963	PASS
75	95	30	60	50.5	88400	PASS
95	95	100	100	100.0	174976	PASS
96	95	5	9	6.9	12114	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	64.4	112659	PASS
175	174	5	9	7.7	8636	PASS
176	174	95	101	97.1	109392	PASS
177	176	5	9	6.3	6939	PASS