


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111225\
Data File : VY023751.D
Acq On : 12 Nov 2025 09:23
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110425S.M
Title : SW846 8260
Last Update : Wed Nov 05 04:41:50 2025

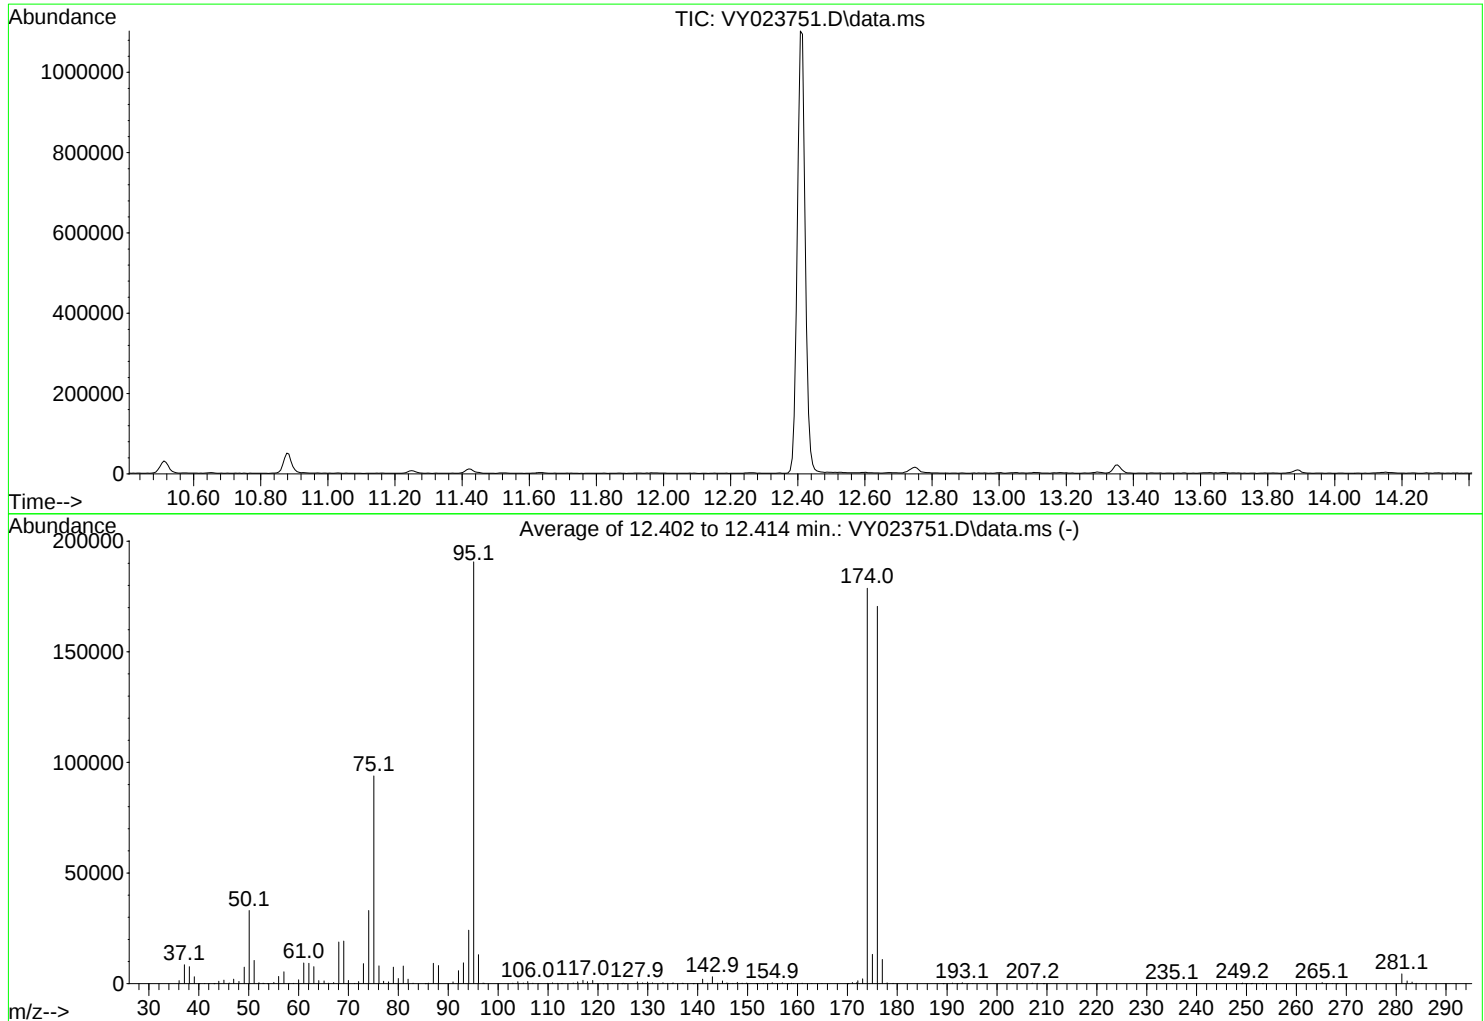

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	33064	PASS
75	95	30	60	49.2	93869	PASS
95	95	100	100	100.0	190677	PASS
96	95	5	9	6.9	13077	PASS
173	174	0.00	2	1.2	2214	PASS
174	95	50	100	93.7	178731	PASS
175	174	5	9	7.4	13246	PASS
176	174	95	101	95.4	170573	PASS
177	176	5	9	6.4	10938	PASS