

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111325\
 Data File : PS032398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2025 15:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 03:37:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.290	7.622	1763.7E6	2172.2E6	389.225	595.853 #
Target Compounds							
2) T	3,5-DICHL...	6.446	0.000	26004946	0	4.022	N.D. #
6) T	MCP	0.000	7.905	0	210.0E6	N.D.	15.786
7) T	MCPA	7.795	0.000	376323	0	<MDL	N.D. #
8) T	DICHLORPROP	8.199f	0.000	5589270	0	1.256	N.D. #
9) T	2,4-D	8.453f	0.000	95985840	0	21.274	N.D. #
10) T	Pentachlo...	8.715	9.363	7842965	3671529	<MDL	<MDL #
11) T	2,4,5-TP ...	9.284	9.778f	3985882	3817296	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.181	0	2154670	N.D.	<MDL
13) T	2,4-DB	10.177	0.000	2421944	0	<MDL	N.D. #
14) T	DINOSEB	11.343	11.119	12023290	4723041	<MDL	<MDL #
15) T	Picloram	11.135f	12.186f	622453	27698748	<MDL	<MDL #
16) T	DCPA	11.651	12.186f	10351829	27698748	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110325\
Data File : PS032398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2025 15:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 03:37:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

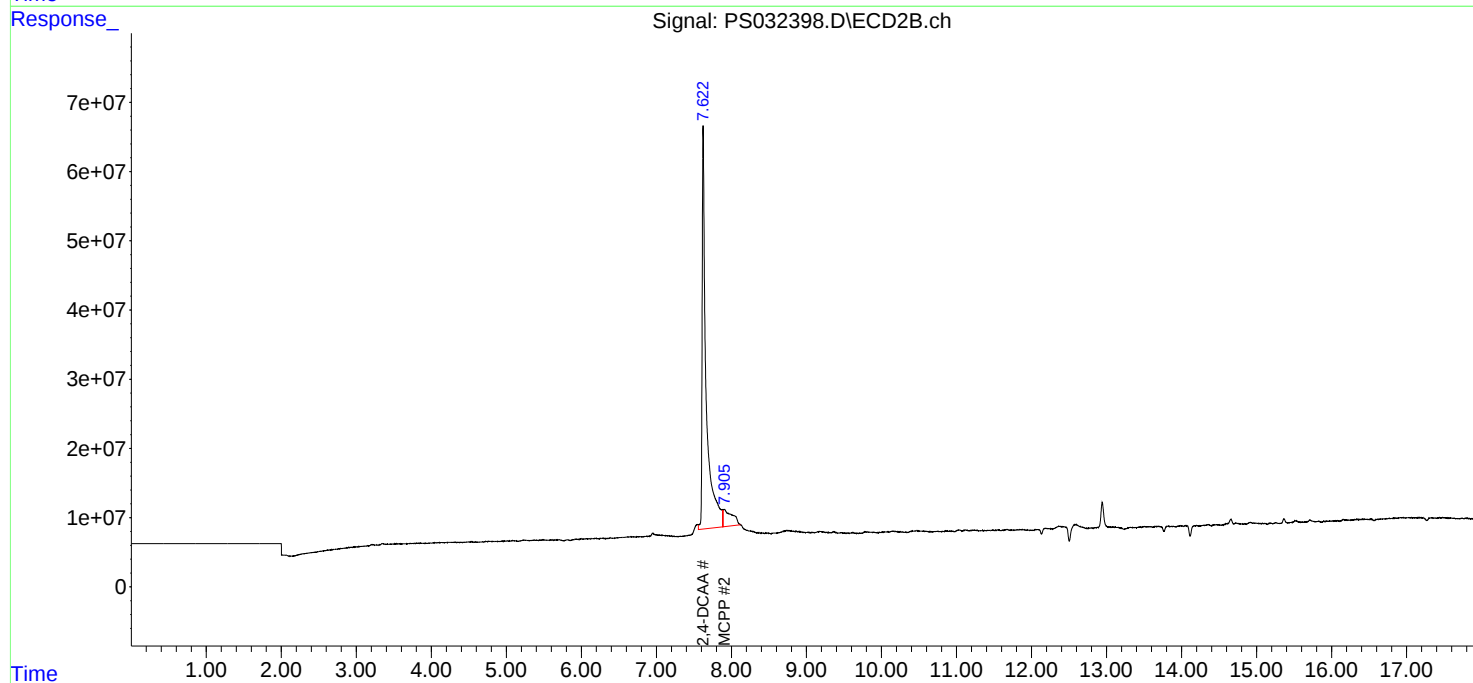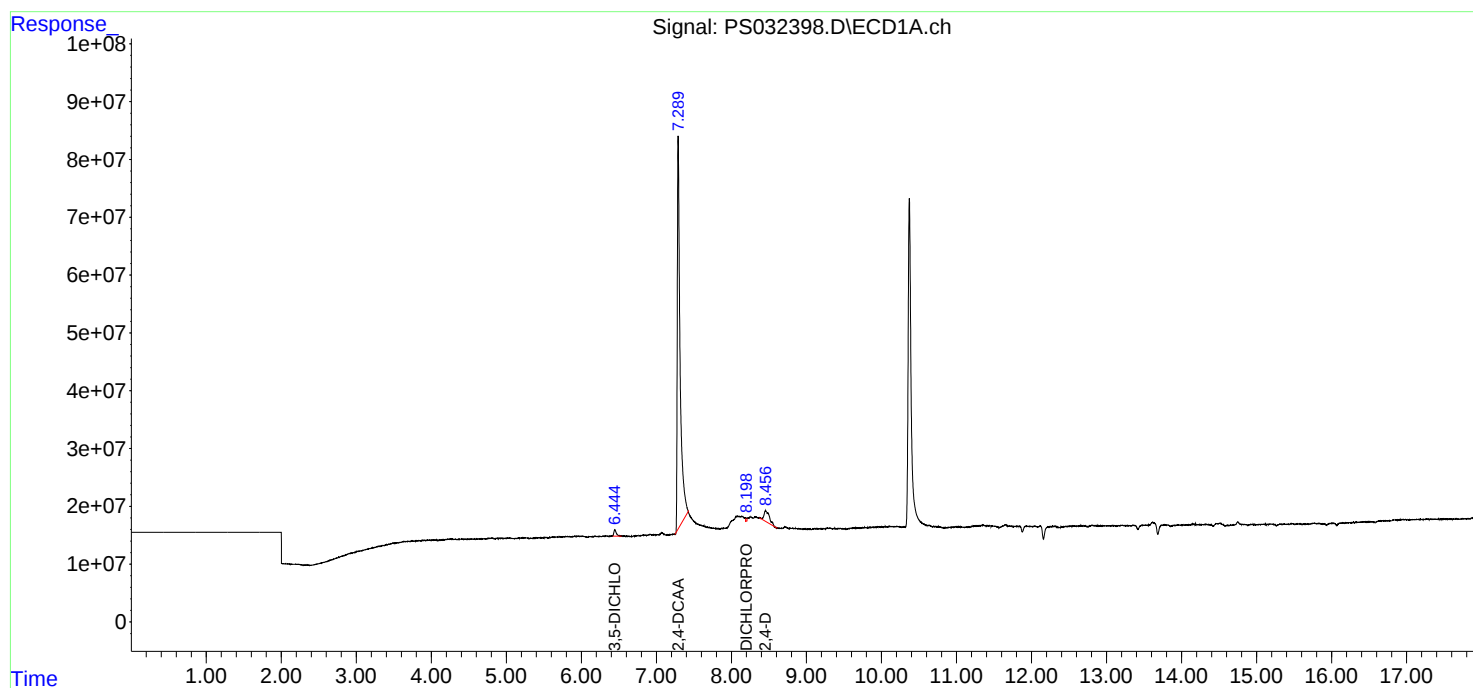


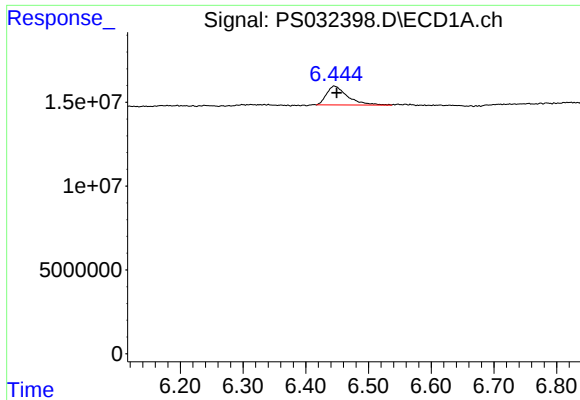

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.446 min
Delta R.T.: -0.003 min
Response: 26004946
Conc: 4.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

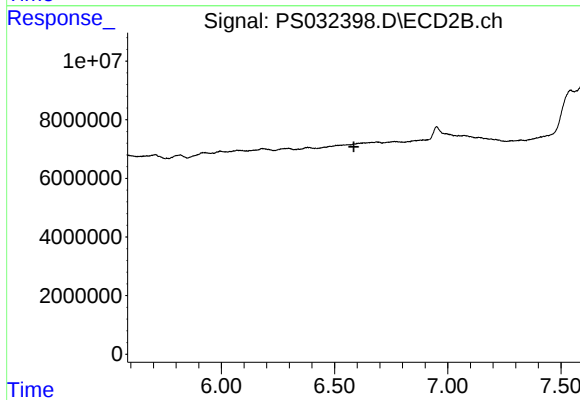


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

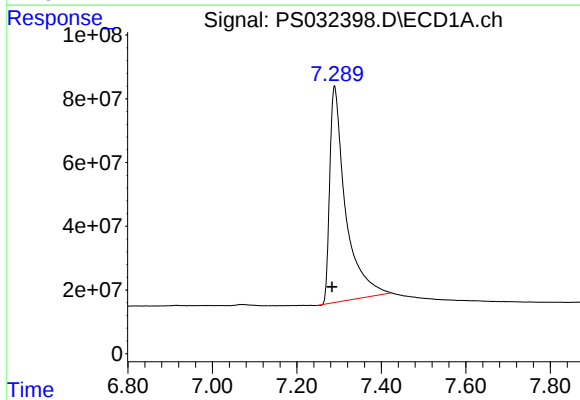


#4 2,4-DCAA

R.T.: 7.290 min
Delta R.T.: 0.006 min
Response: 1763683683
Conc: 389.22 ng/ml

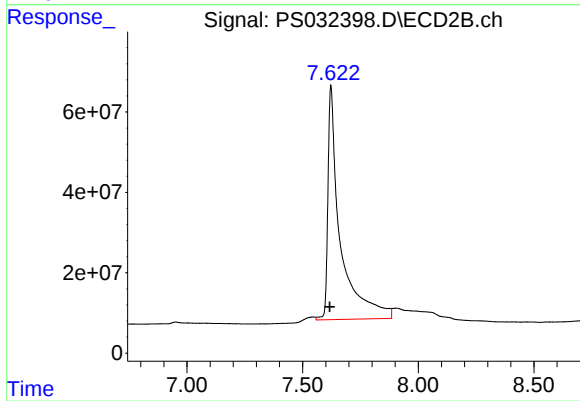

#4 2,4-DCAA


R.T.: 7.622 min
Delta R.T.: 0.005 min
Response: 2172178446
Conc: 595.85 ng/ml

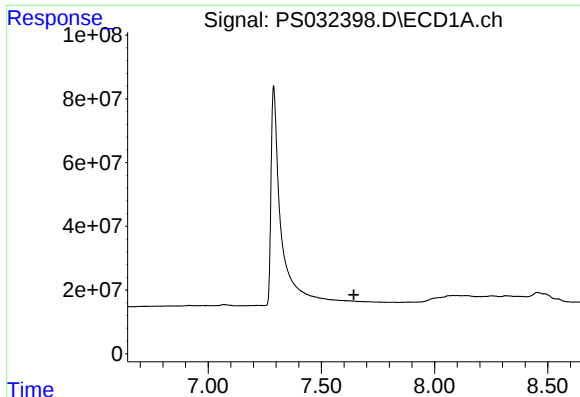

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.644 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

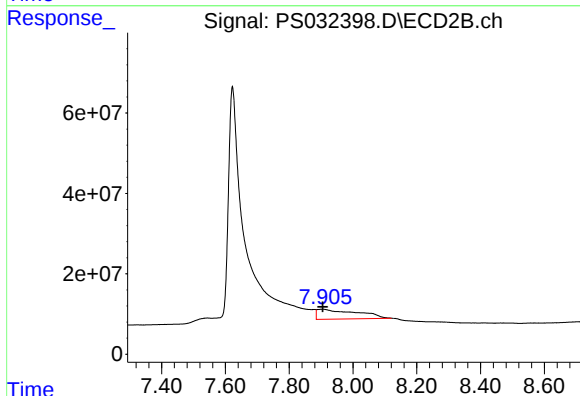


#6 MCP

R.T.: 7.905 min
Delta R.T.: 0.000 min
Response: 209970272
Conc: 15.79 ug/ml

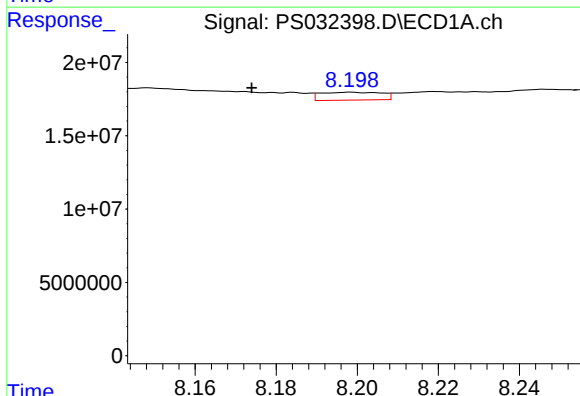


#8 DICHLORPROP

R.T.: 8.199 min
Delta R.T.: 0.025 min
Response: 5589270
Conc: 1.26 ng/ml

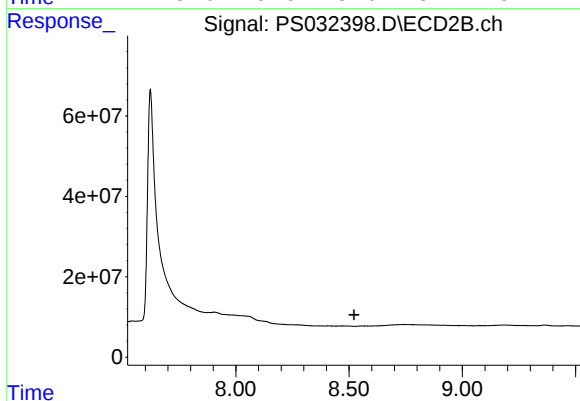

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.522 min
Response: 0
Conc: N.D.

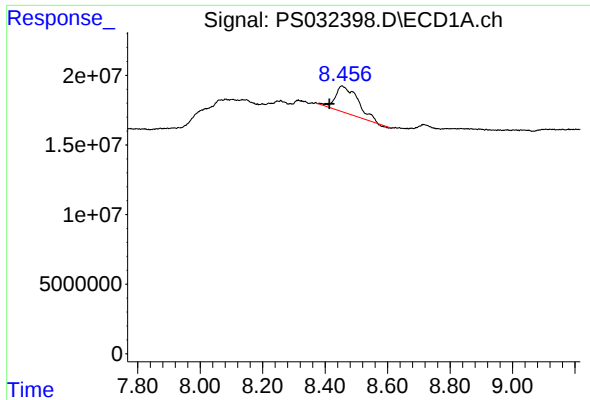

#9 2,4-D

R.T.: 8.453 min
Delta R.T.: 0.040 min
Response: 95985840
Conc: 21.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

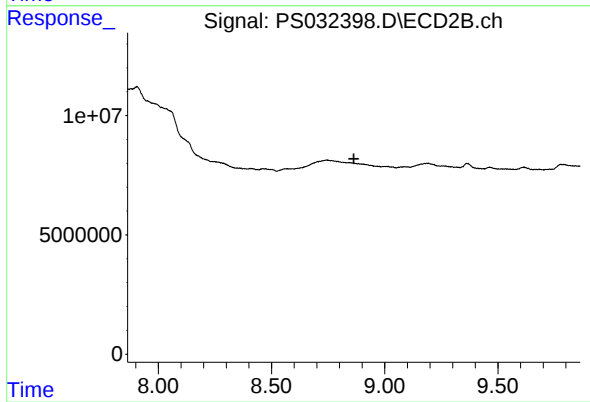

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.864 min
Response: 0
Conc: N.D.