

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111325\
 Data File : PS032412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2025 21:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 03:44:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.284	7.624	1772.7E6	1924.9E6	391.205	528.014 #
Target Compounds							
2) T	3,5-DICHL...	6.443	0.000	23256475	0	3.597	N.D. #
6) T	MCP	7.684f	7.911	1014274	28997180	<MDL	2.180 #
7) T	MCPA	7.794	8.101f	748561	3766668	<MDL	<MDL #
8) T	DICHLORPROP	8.167	0.000	743219	0	<MDL	N.D. #
10) T	Pentachlo...	8.712	9.368	6389662	5877294	<MDL	<MDL #
11) T	2,4,5-TP ...	9.277	0.000	6301703	0	<MDL	N.D. #
12) T	2,4,5-T	9.585	10.148	1729123	5984084	<MDL	<MDL #
13) T	2,4-DB	10.148	10.708f	2197006	3001771	<MDL	<MDL #
14) T	DINOSEB	11.347	11.058f	6448691	1990332	<MDL	<MDL #
15) T	Picloram	11.198	0.000	9015112	0	<MDL	N.D. #
16) T	DCPA	11.636	12.099f	3627948	19691932	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110325\
Data File : PS032412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2025 21:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 03:44:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

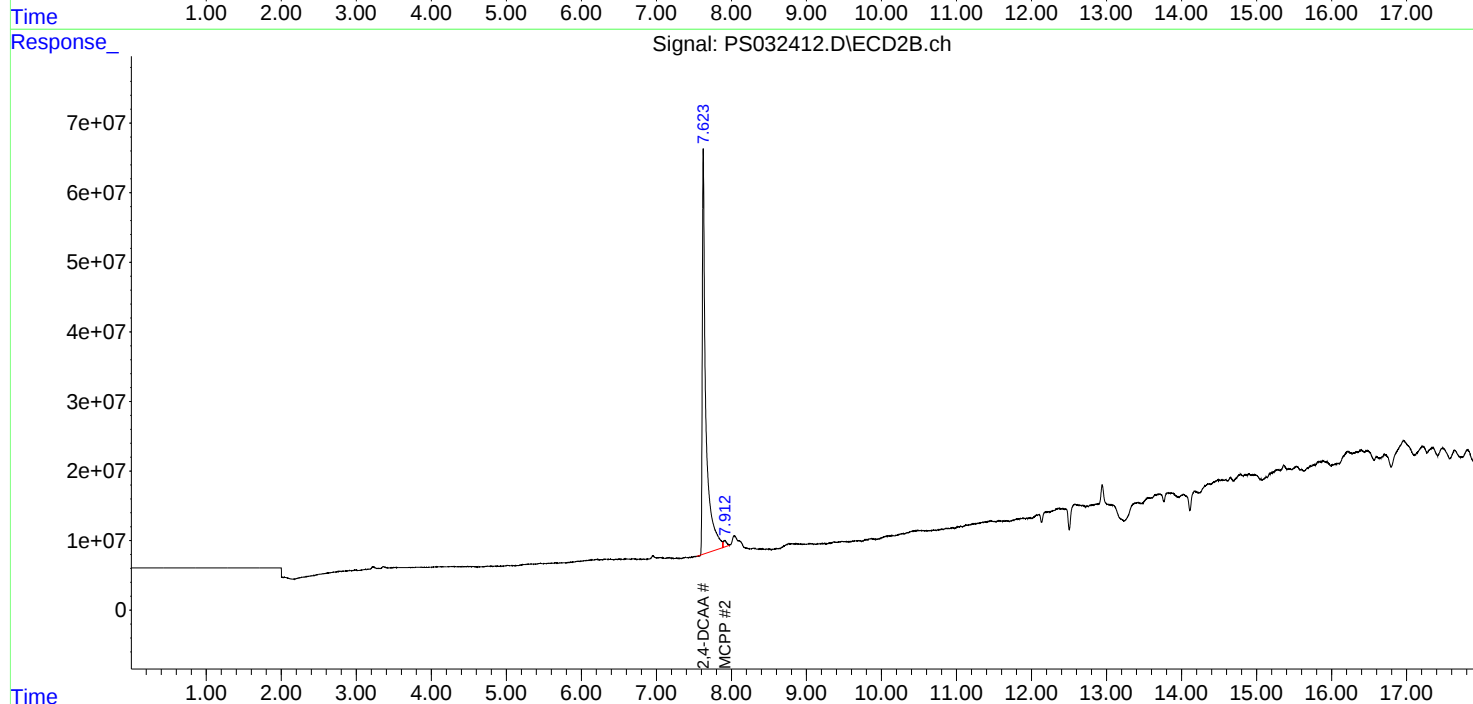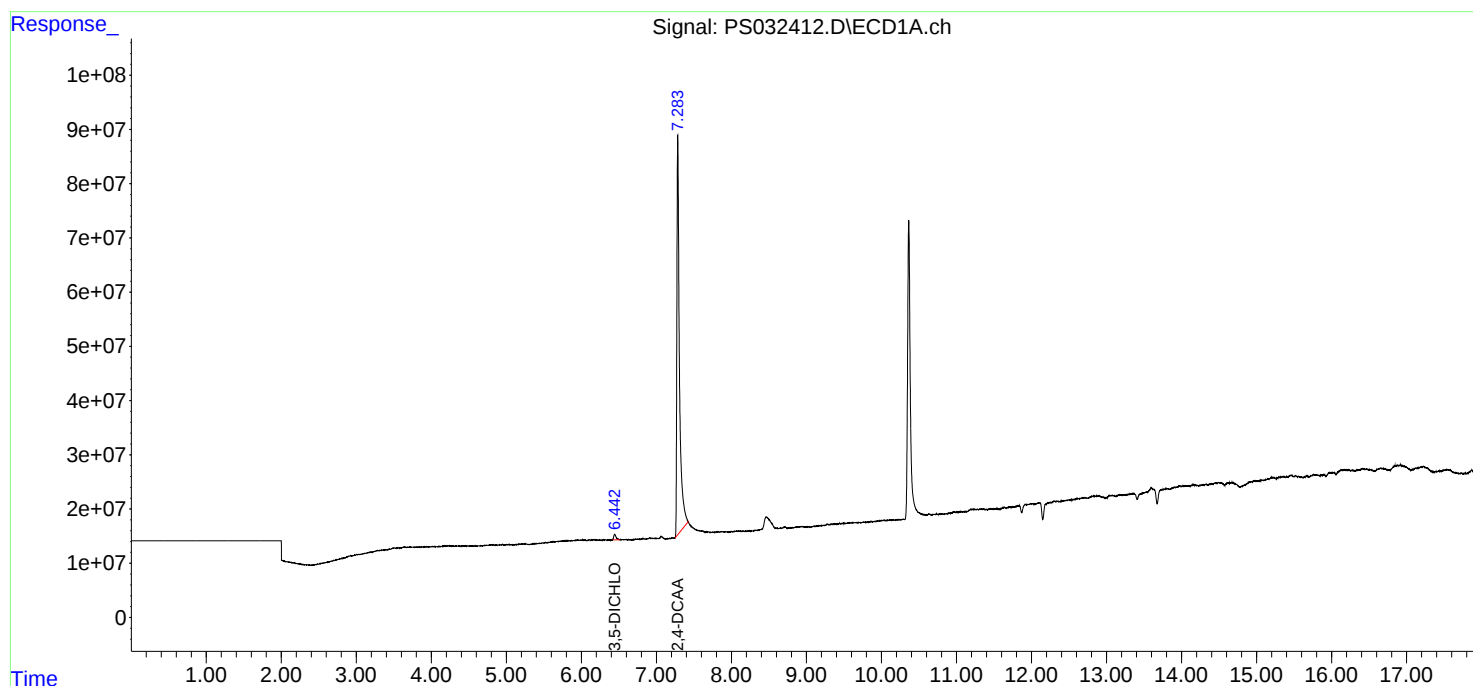


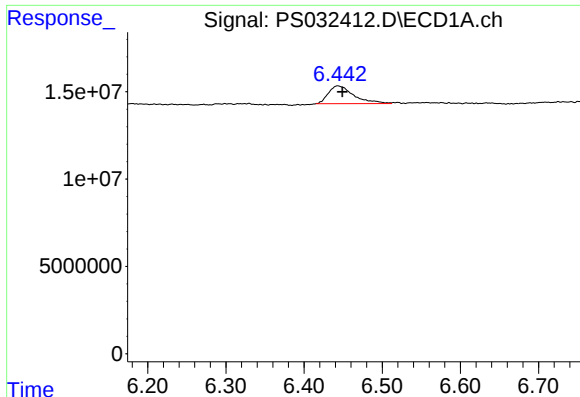

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.443 min
Delta R.T.: -0.006 min
Response: 23256475
Conc: 3.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

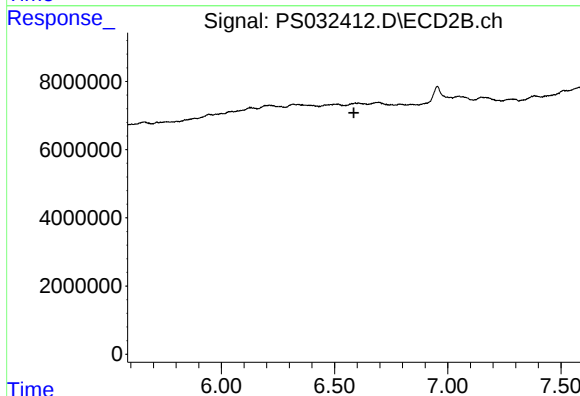


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

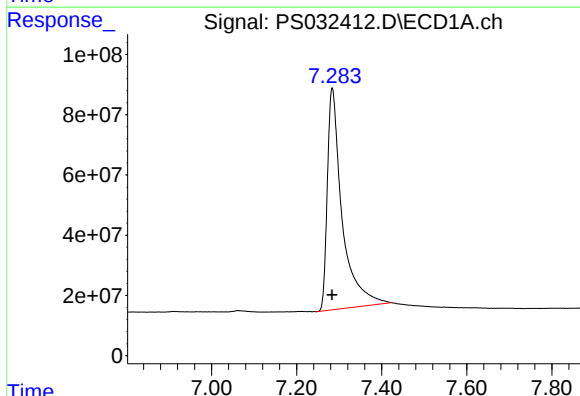


#4 2,4-DCAA

R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 1772658078
Conc: 391.21 ng/ml

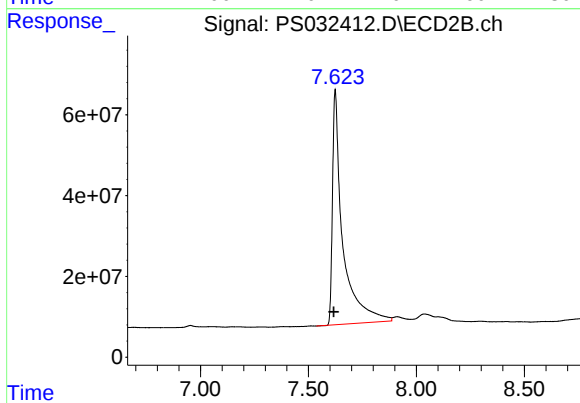

#4 2,4-DCAA


R.T.: 7.624 min
Delta R.T.: 0.007 min
Response: 1924874029
Conc: 528.01 ng/ml

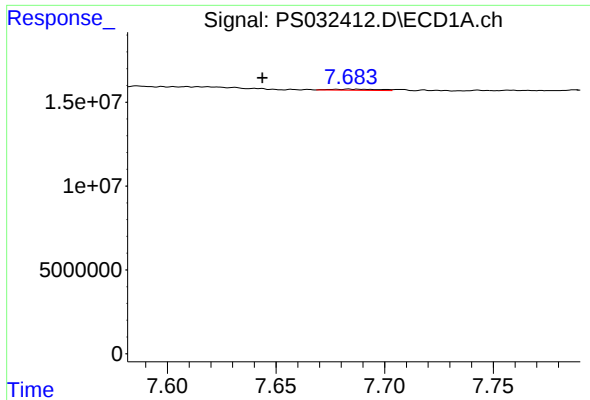

#6 MCPP

R.T.: 7.684 min
Delta R.T.: 0.040 min
Response: 1014274
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

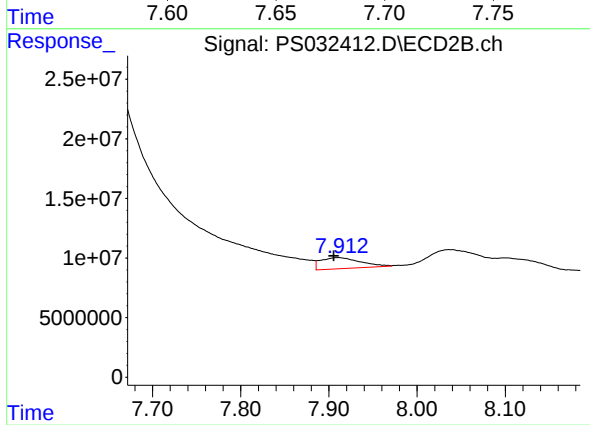

#6 MCPP

R.T.: 7.911 min
Delta R.T.: 0.006 min
Response: 28997180
Conc: 2.18 ug/ml