
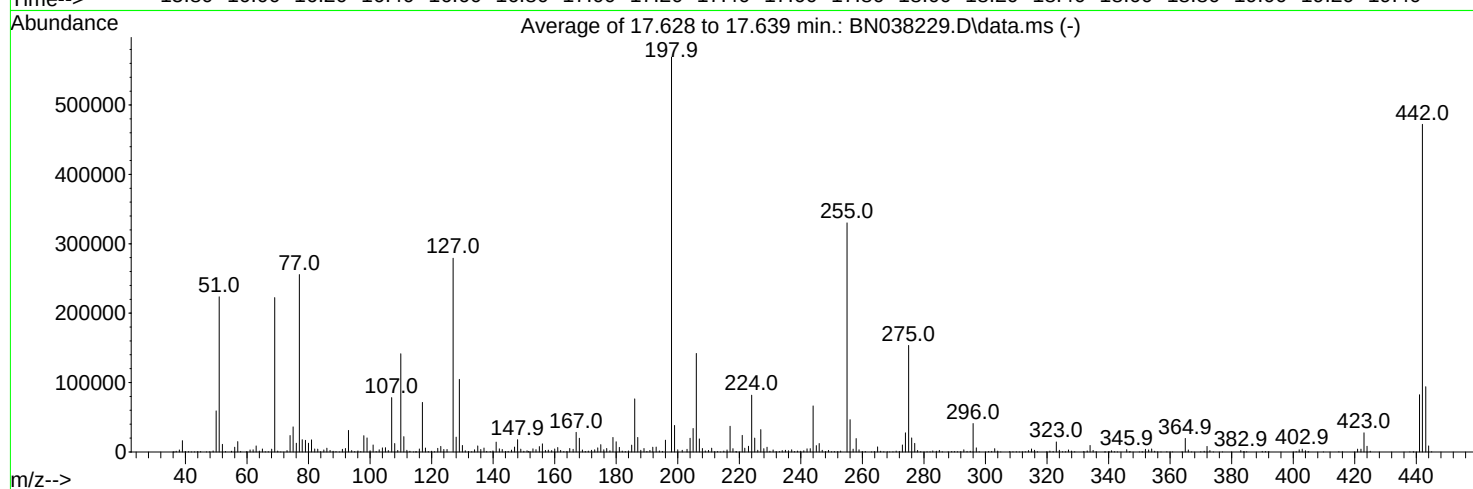


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN120125\  
Data File : BN038229.D  
Acq On : 01 Dec 2025 17:11  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN112725.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Nov 28 21:04:10 2025

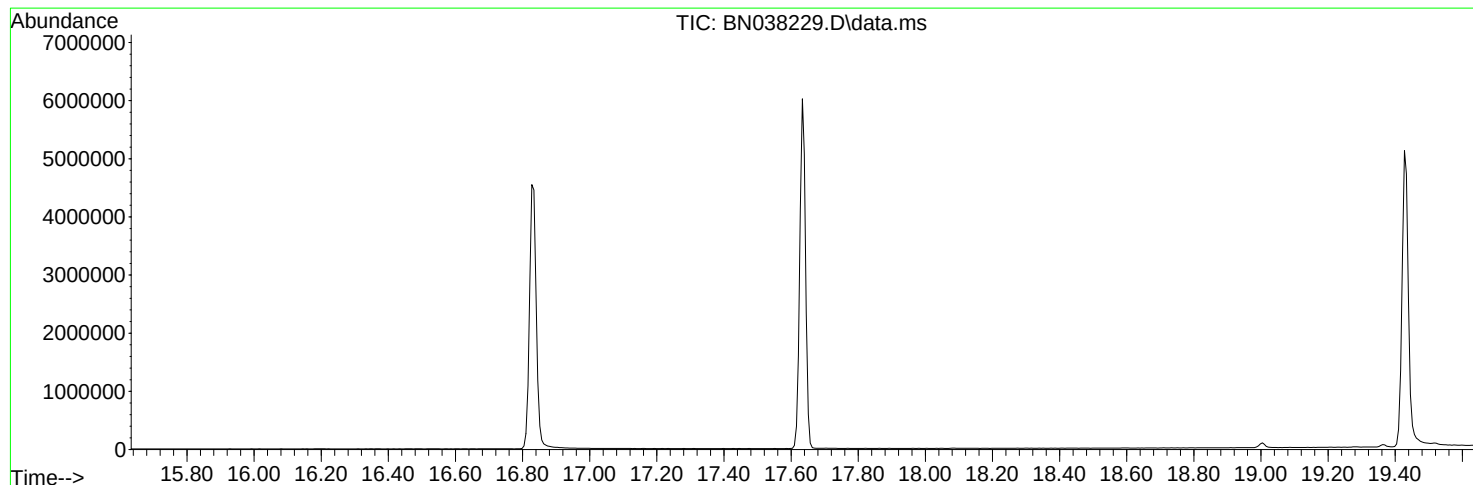




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 68     | 69      | 0.00   | 2      | 1.8   | 3958   | PASS      |
| 69     | 69      | 100    | 100    | 100.0 | 222464 | PASS      |
| 70     | 69      | 0.00   | 2      | 0.5   | 1221   | PASS      |
| 197    | 198     | 0.00   | 2      | 0.0   | 0      | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 569067 | PASS      |
| 199    | 198     | 5      | 9      | 6.7   | 38248  | PASS      |
| 365    | 198     | 1      | 100    | 3.4   | 19427  | PASS      |
| 441    | 443     | 0.01   | 150    | 87.9  | 82573  | PASS      |
| 442    | 442     | 100    | 100    | 100.0 | 472256 | PASS      |
| 443    | 442     | 15     | 24     | 19.9  | 93936  | PASS      |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN120125\  
Data File : BN038229.D  
Acq On : 01 Dec 2025 17:11  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Dec 01 17:45:52 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 01 17:45:43 2025  
Response via : Initial Calibration

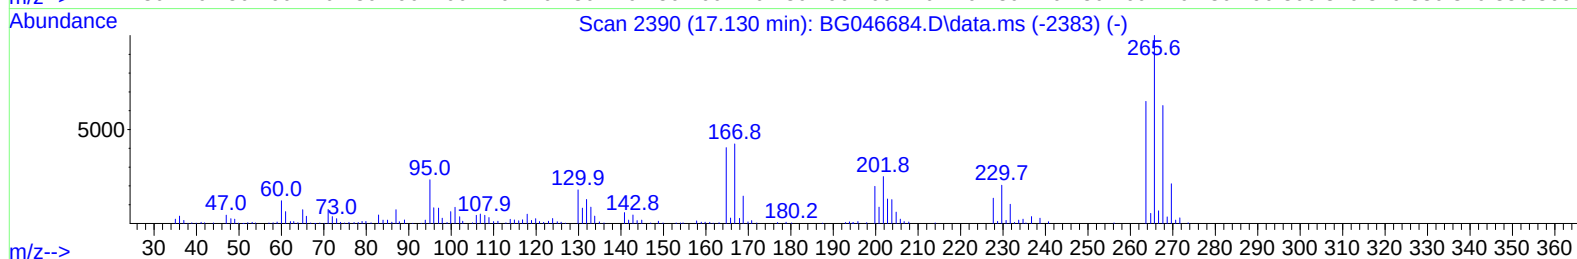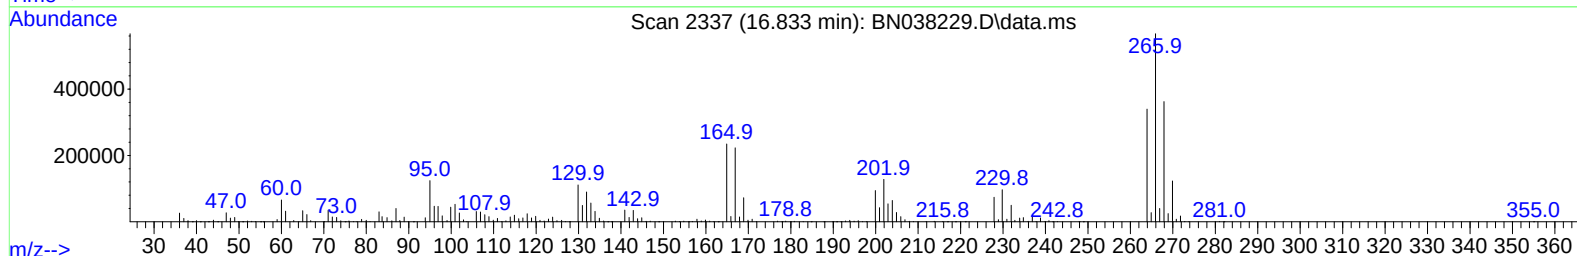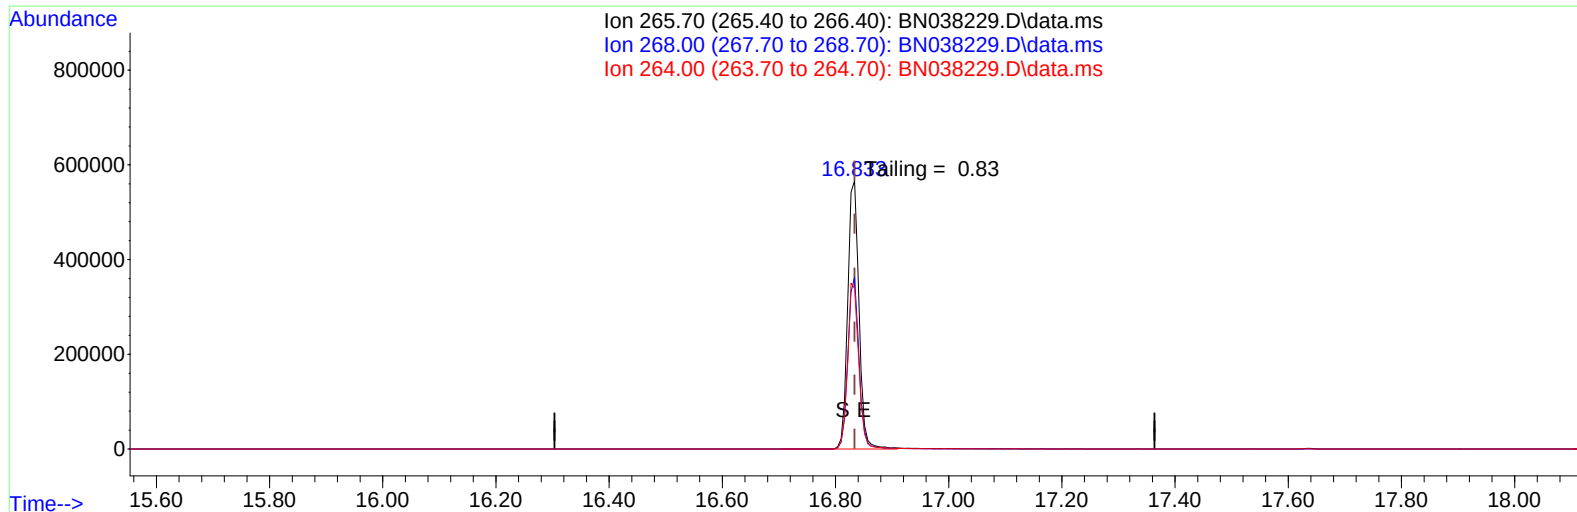

TIC: BN038229.D\data.ms

**(70) Pentachlorophenol (C)**

16.833min ( 0.000) 277.76 ng




response 785850

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.93  |
| 264.00 | 61.60  | 59.91  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN120125\  
Data File : BN038229.D  
Acq On : 01 Dec 2025 17:11  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Dec 01 17:45:52 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 01 17:45:43 2025  
Response via : Initial Calibration

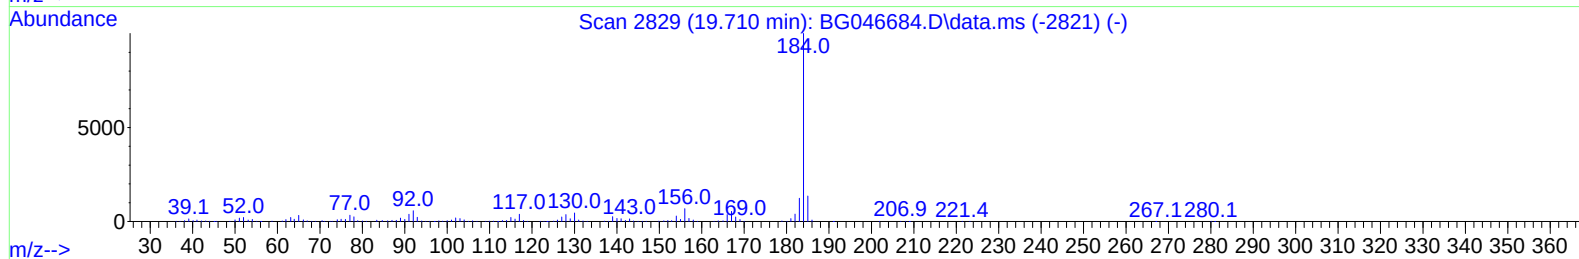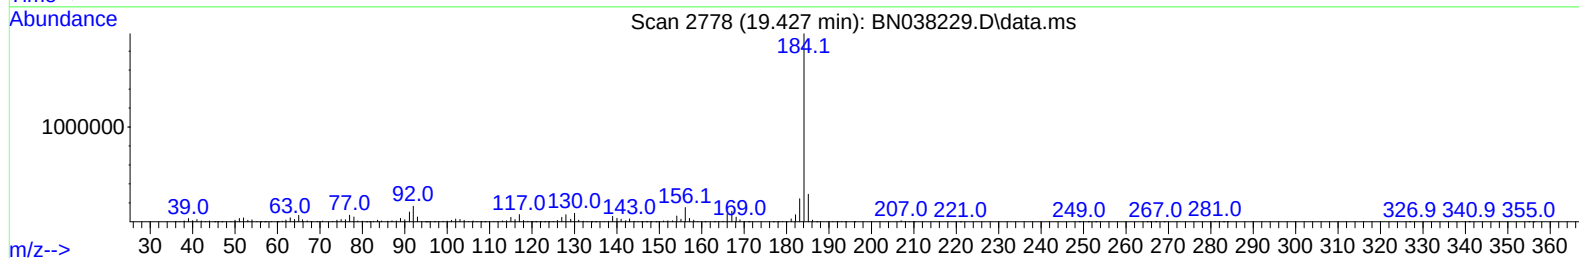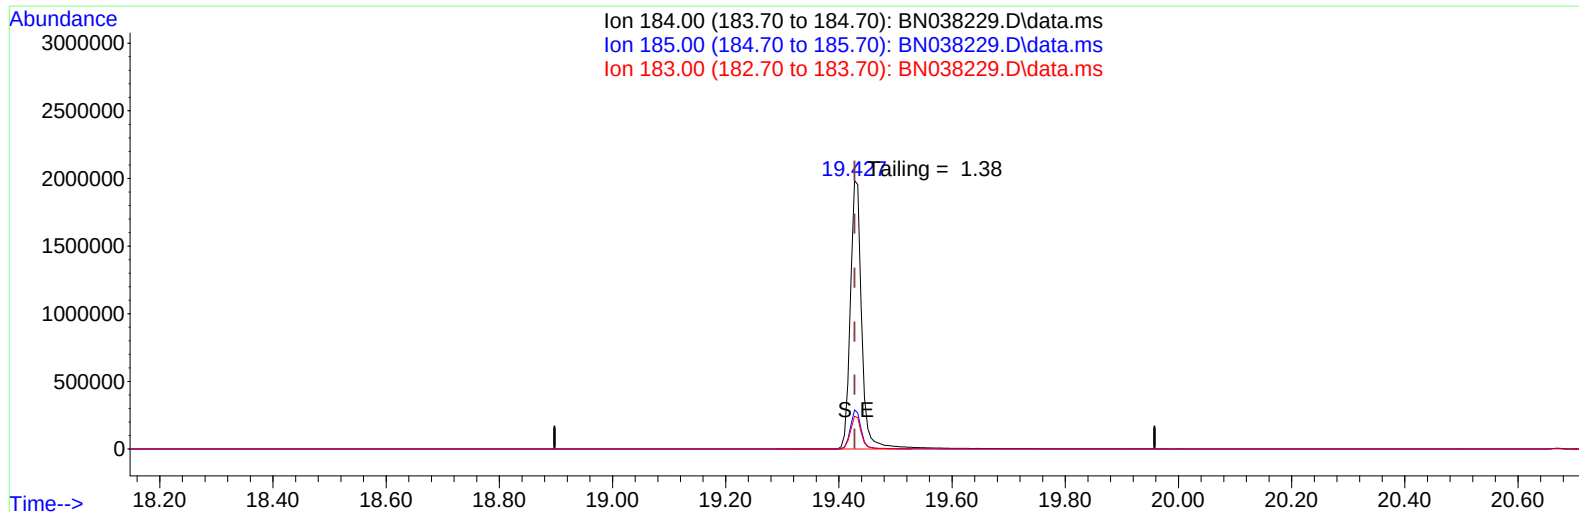

TIC: BN038229.D\data.ms

**(77) Benzidine**

19.427min ( 0.000) 0.00 ng

response 2797498

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.63  |
| 183.00 | 13.20  | 12.24  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 12/1/2025     | BNA_N            | <u>BN038229.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1521305          | 20.679             |
| DDD           | 52158            | 20.227             |
| DDE           | 1105             | 19.722             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 53263         | 1574568          | 3.38               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP