


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111225\
Data File : BG064744.D
Acq On : 12 Nov 2025 10:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

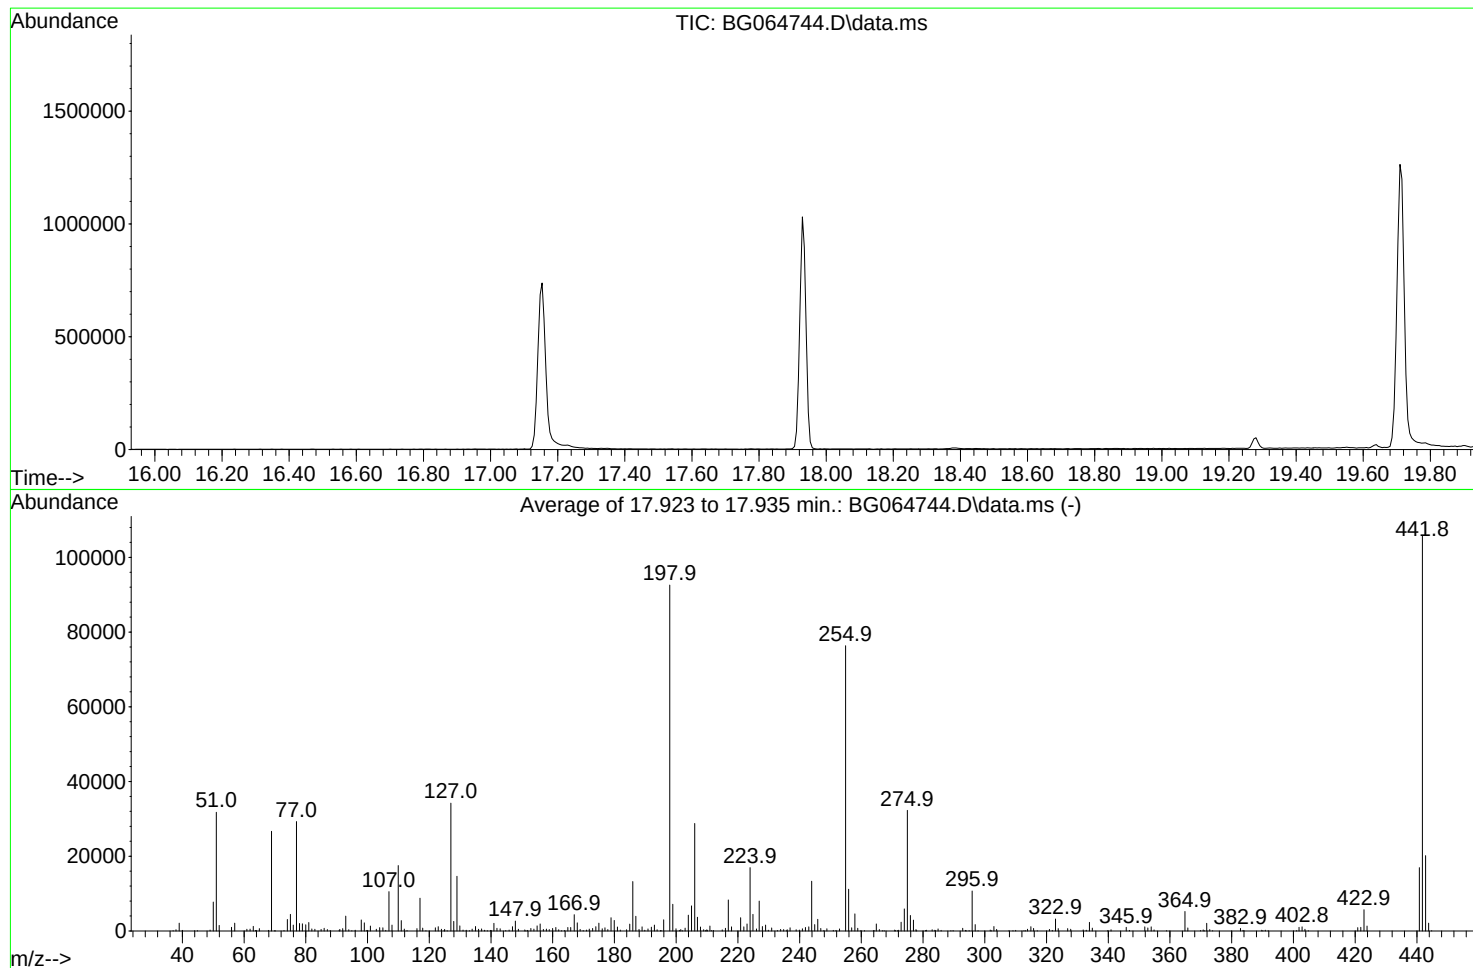




AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2519

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.6	163	PASS
69	69	100	100	100.0	26656	PASS
70	69	0.00	2	0.2	66	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92589	PASS
199	198	5	9	7.7	7122	PASS
365	198	1	100	5.6	5213	PASS
441	443	0.01	150	84.2	16956	PASS
442	442	100	100	100.0	105680	PASS
443	442	15	24	19.1	20135	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111225\
Data File : BG064744.D
Acq On : 12 Nov 2025 10:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 12 11:53:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 01:10:41 2025
Response via : Initial Calibration

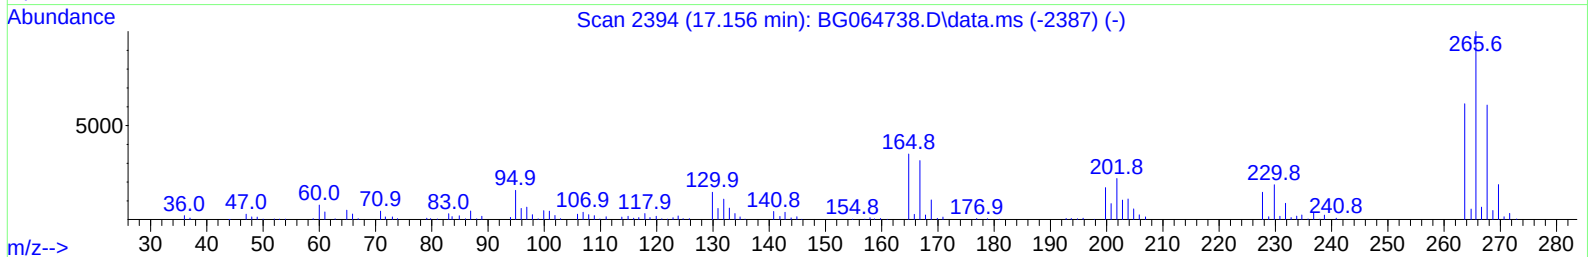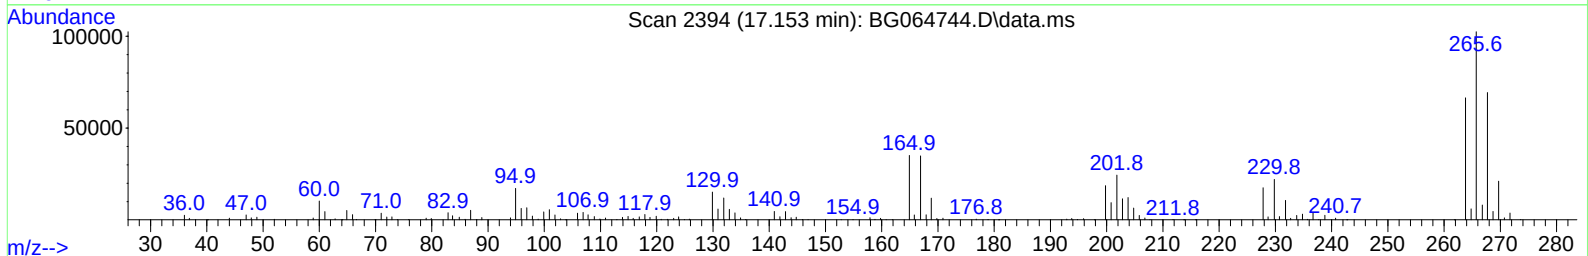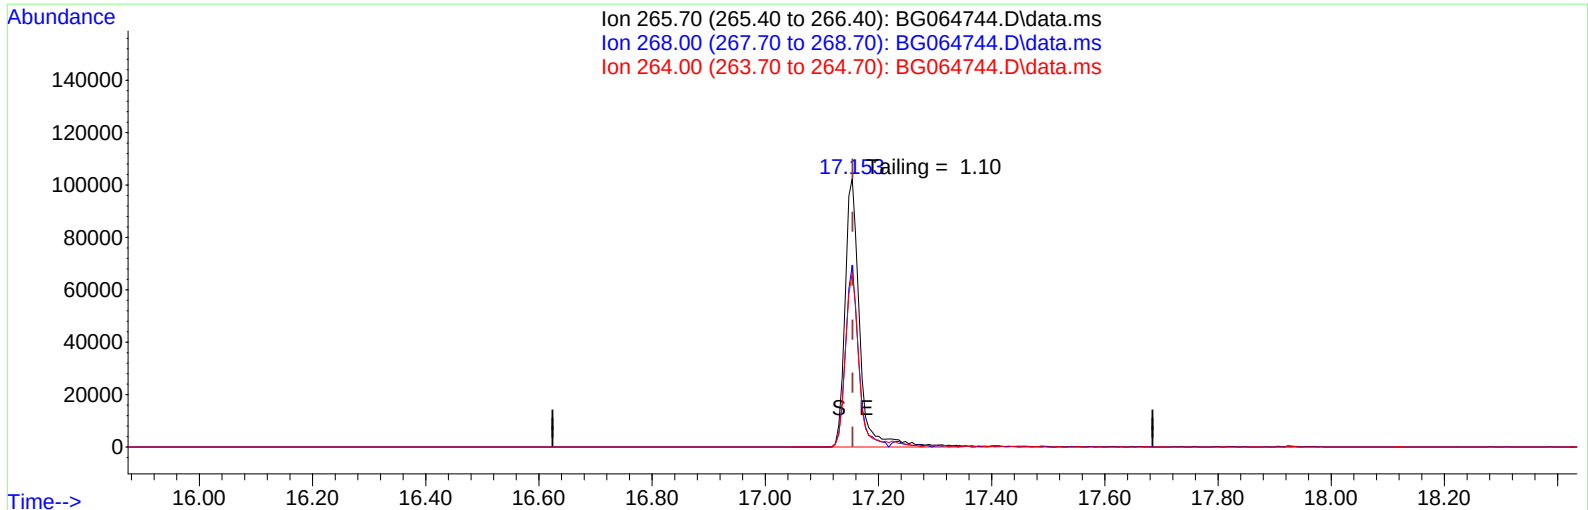

TIC: BG064744.D\data.ms

(70) Pentachlorophenol (C)

17.153min (-0.001) 31332.04 ng




response 182303

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	72.31
264.00	61.60	64.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111225\
Data File : BG064744.D
Acq On : 12 Nov 2025 10:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 12 11:53:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 01:10:41 2025
Response via : Initial Calibration

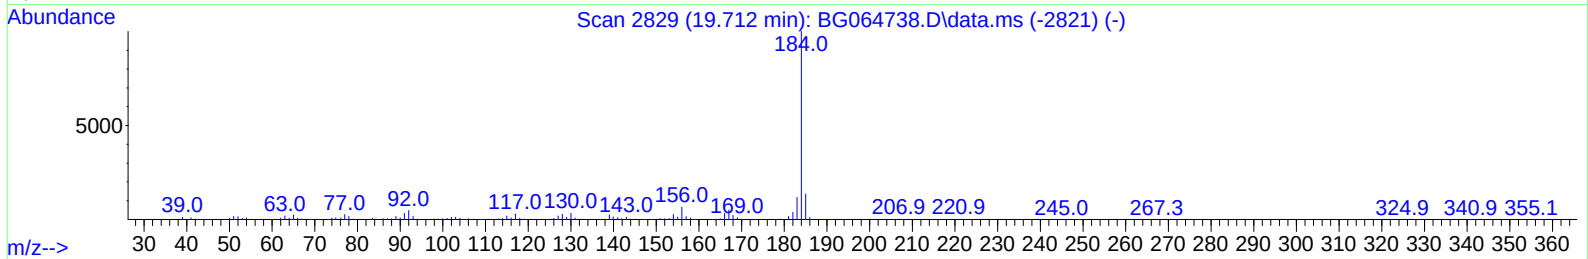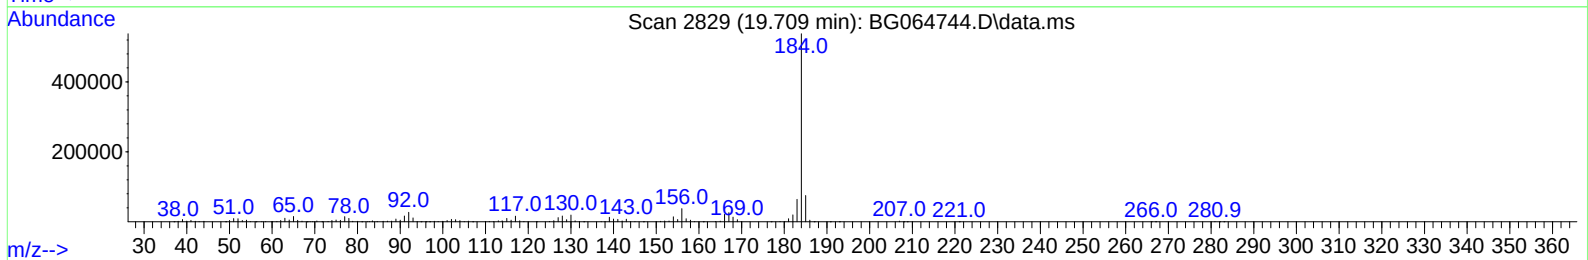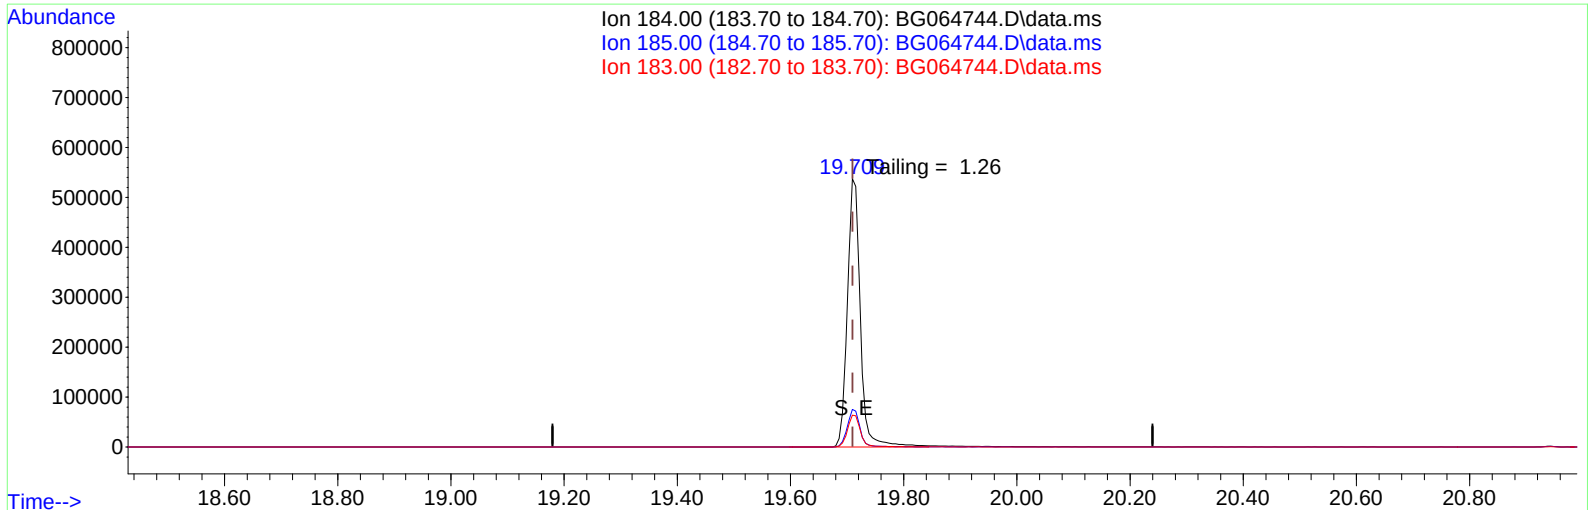

TIC: BG064744.D\data.ms

(77) Benzidine

19.709min (-0.000) 0.00 ng

response 866225

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.01
183.00	11.80	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/12/2025	BNA_G	<u>BG064744.D</u>
Compound Name	Response	Retention Time
DDT	495175	20.943
DDD	6870	20.502
DDE	65	19.275
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6935	502110	1.38

Instrument :
BNA_G
ClientSampleId :
DFTPP