


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111325\
Data File : BG064755.D
Acq On : 13 Nov 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

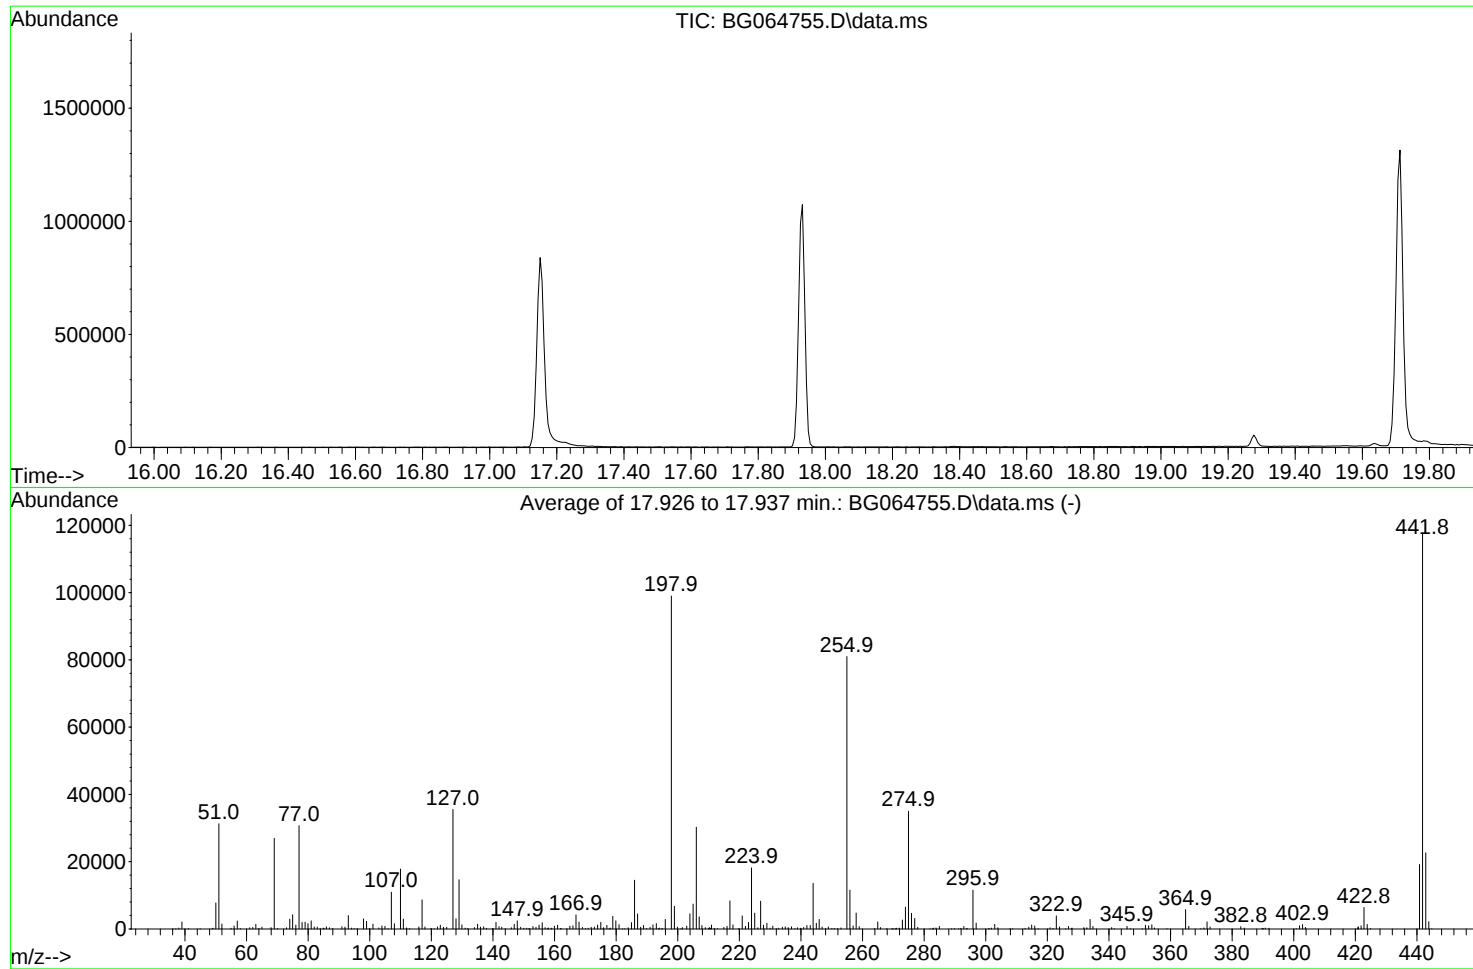




AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	427	PASS
69	69	100	100	100.0	26979	PASS
70	69	0.00	2	0.5	143	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98971	PASS
199	198	5	9	6.8	6743	PASS
365	198	1	100	5.8	5743	PASS
441	443	0.01	150	84.8	19173	PASS
442	442	100	100	100.0	117405	PASS
443	442	15	24	19.3	22621	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111325\
Data File : BG064755.D
Acq On : 13 Nov 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 13 15:48:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

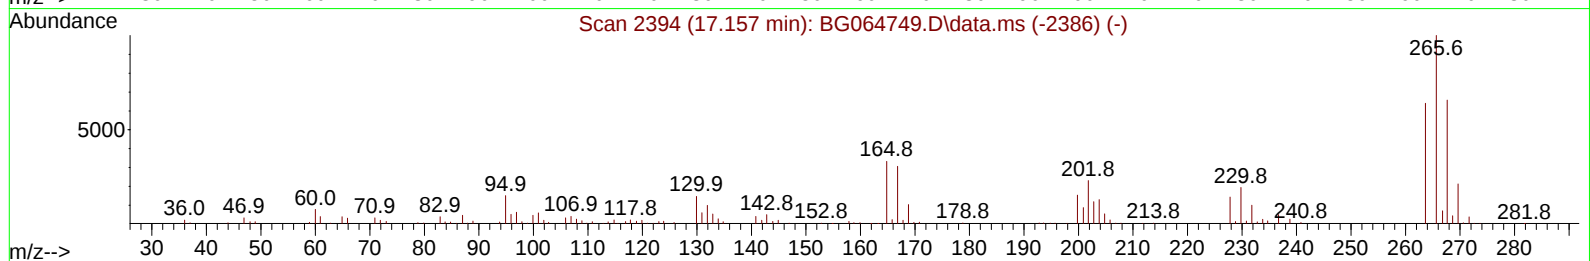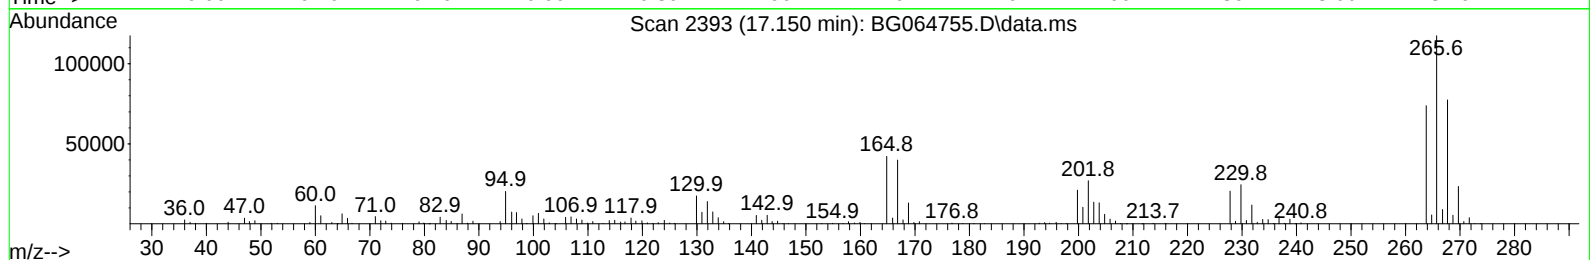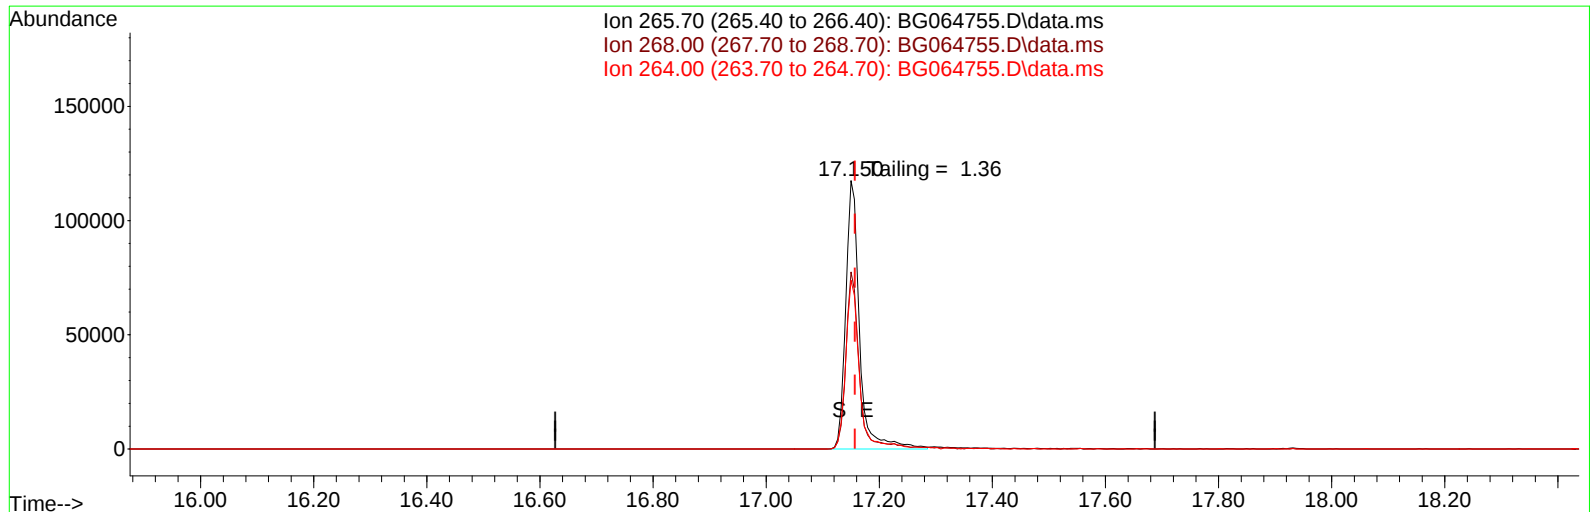

TIC: BG064755.D\data.ms

(70) Pentachlorophenol (C)

17.150min (-0.007) 321859.64 ng




response 200225

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	70.63
264.00	64.00	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111325\
Data File : BG064755.D
Acq On : 13 Nov 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 13 15:48:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

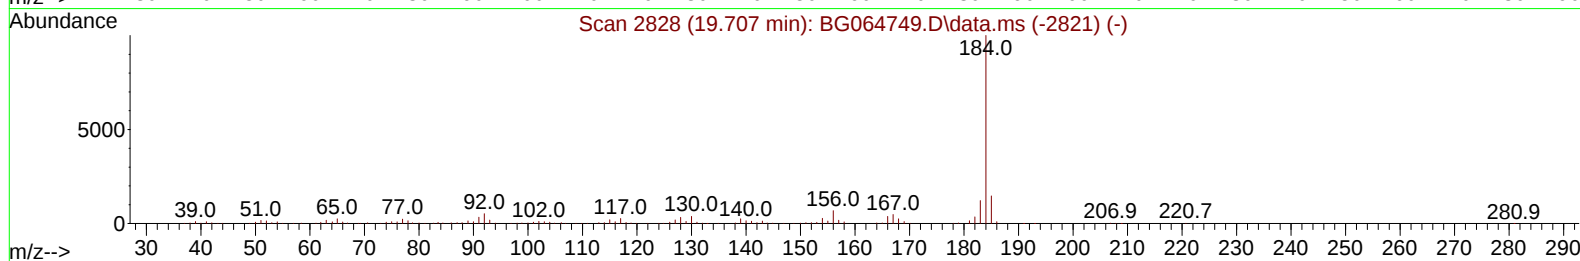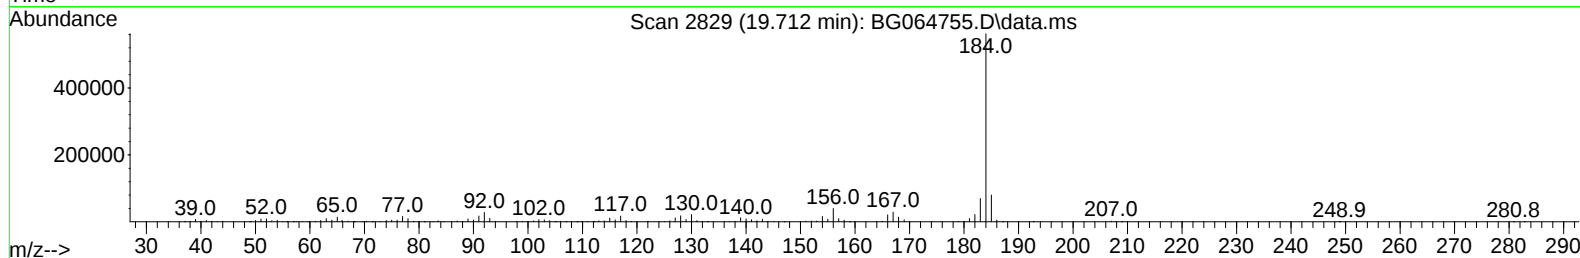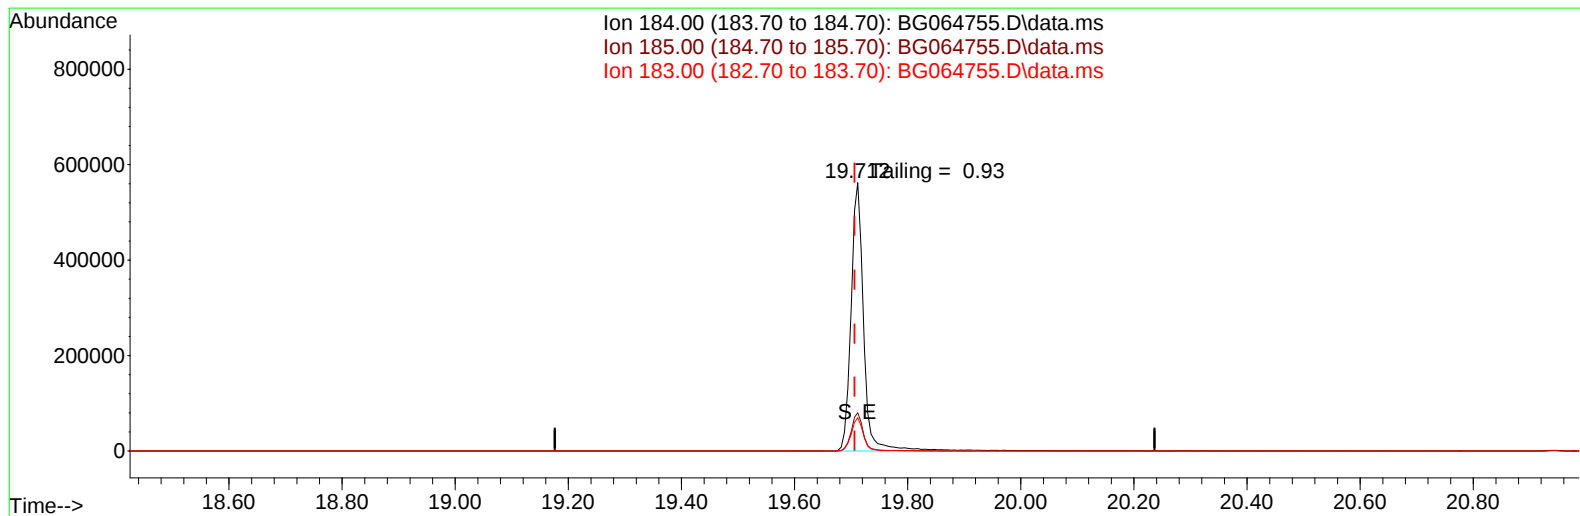

TIC: BG064755.D\data.ms

(77) Benzidine

19.712min (+ 0.005) 16479.67 ng

response 867643

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.24
183.00	12.20	12.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/13/2025	BNA_G	<u>BG064755.D</u>
Compound Name	Response	Retention Time
DDT	521912	20.94
DDD	6403	20.499
DDE	69	19.271
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6472	528384	1.22

Instrument :
BNA_G
ClientSampleId :
DFTPP