
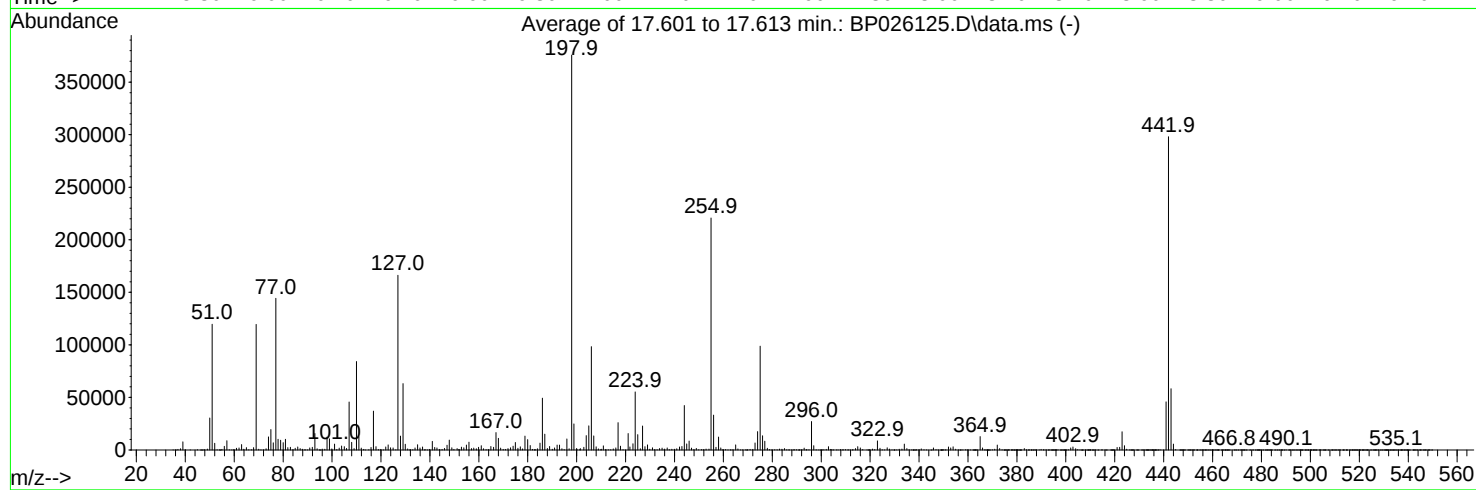


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111325\
Data File : BP026125.D
Acq On : 13 Nov 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 30 11:51:34 2025

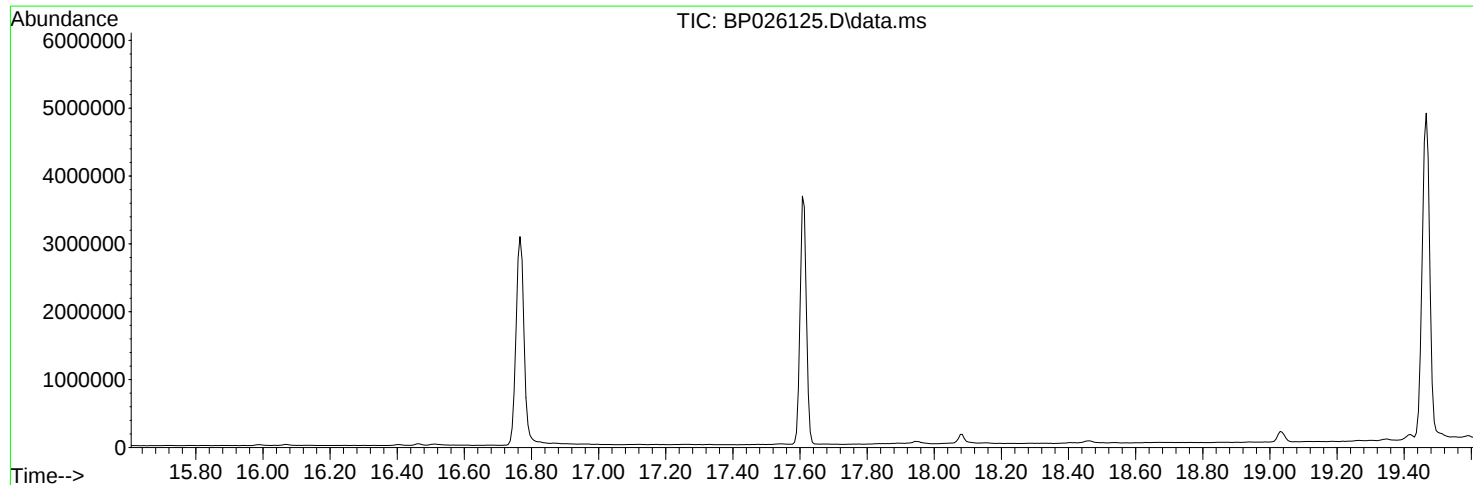




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2480

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	2215	PASS
69	69	100	100	100.0	119479	PASS
70	69	0.00	2	0.6	685	PASS
197	198	0.00	2	0.3	1166	PASS
198	198	100	100	100.0	375744	PASS
199	198	5	9	6.6	24792	PASS
365	198	1	100	3.4	12700	PASS
441	443	0.01	150	78.5	45741	PASS
442	442	100	100	100.0	298044	PASS
443	442	15	24	19.6	58288	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111325\
Data File : BP026125.D
Acq On : 13 Nov 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 13 13:44:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

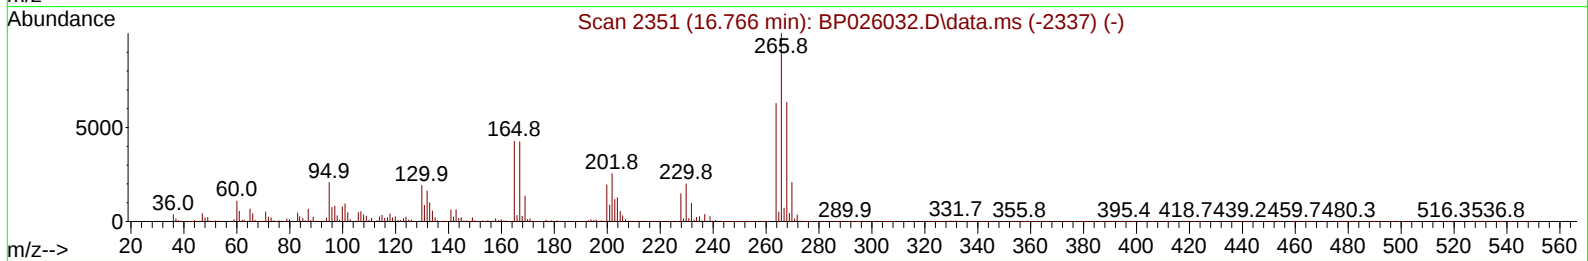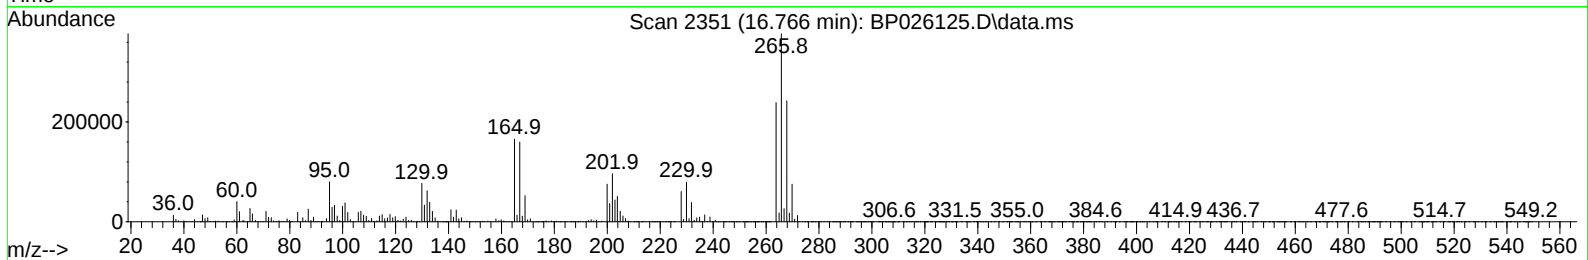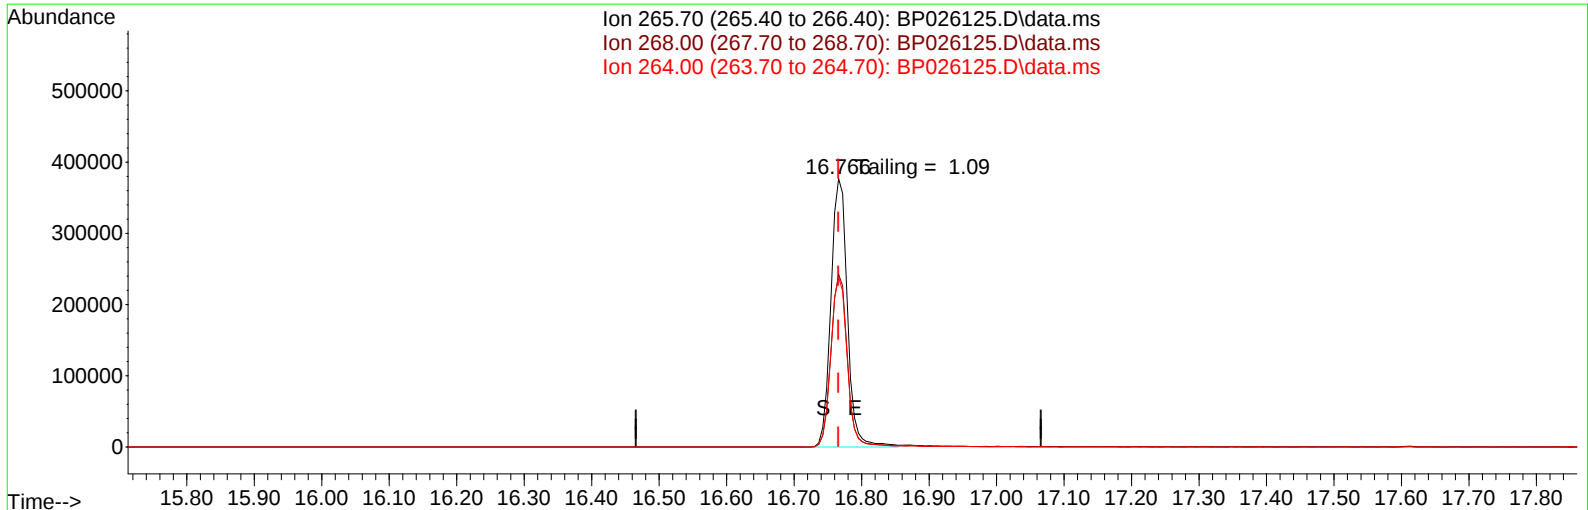

TIC: BP026125.D\data.ms

(70) Pentachlorophenol (C)

16.766min (+ 0.000) 23766.75 ng




response 641612

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.37
264.00	62.80	63.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111325\
Data File : BP026125.D
Acq On : 13 Nov 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 13 13:44:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

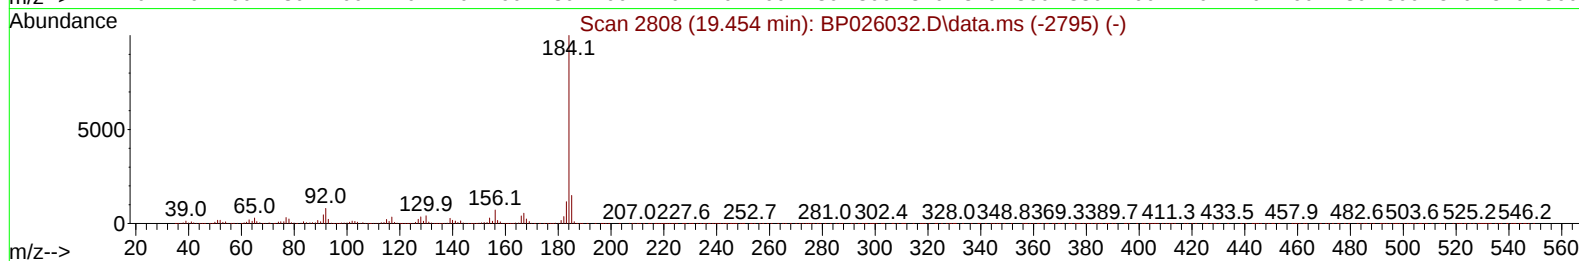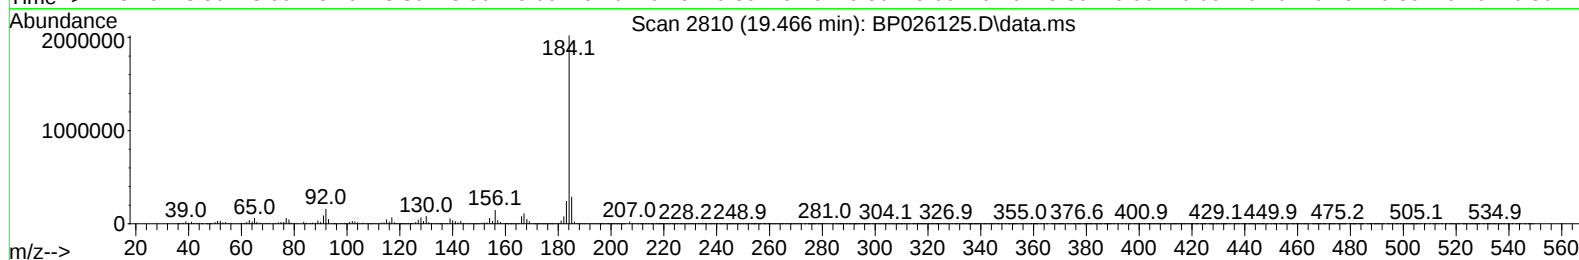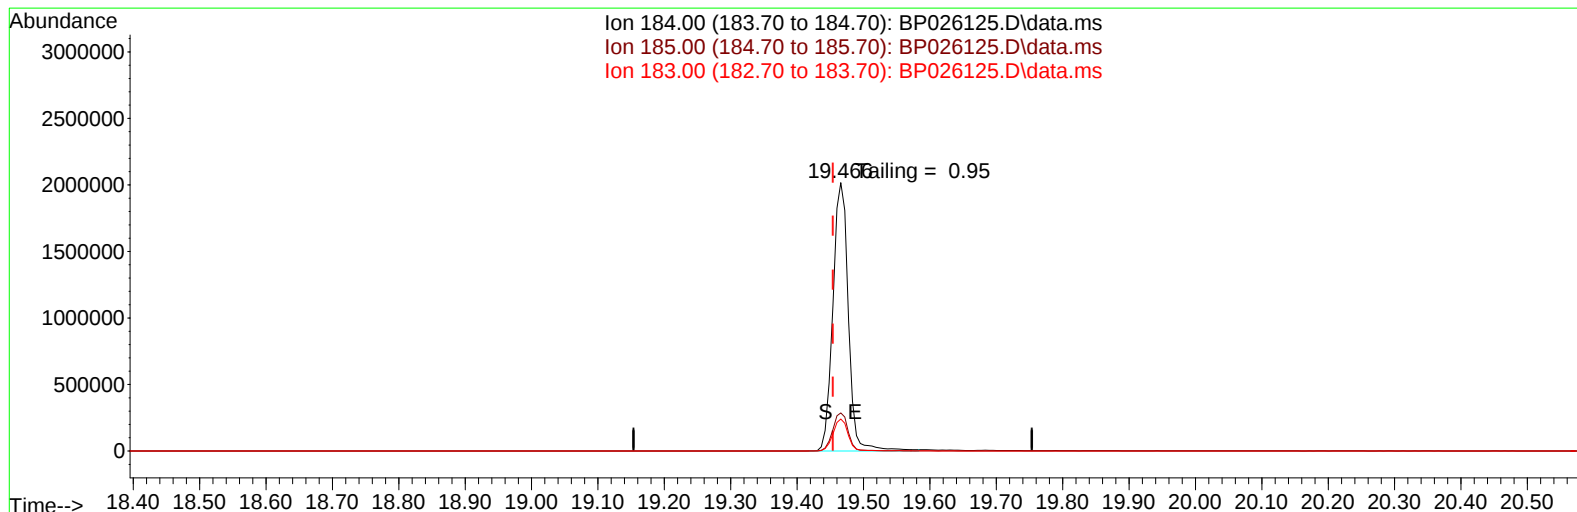

TIC: BP026125.D\data.ms

(77) Benzidine

19.466min (+ 0.012) 5212.36 ng

response 3270143

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.19
183.00	11.50	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/13/2025	BNA_P	<u>BP026125.D</u>
Compound Name	Response	Retention Time
DDT	1575875	20.772
DDD	56558	20.301
DDE	2992	19.777
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
59550	1635425	3.64

Instrument :
BNA_P
ClientSampleId :
DFTPP