
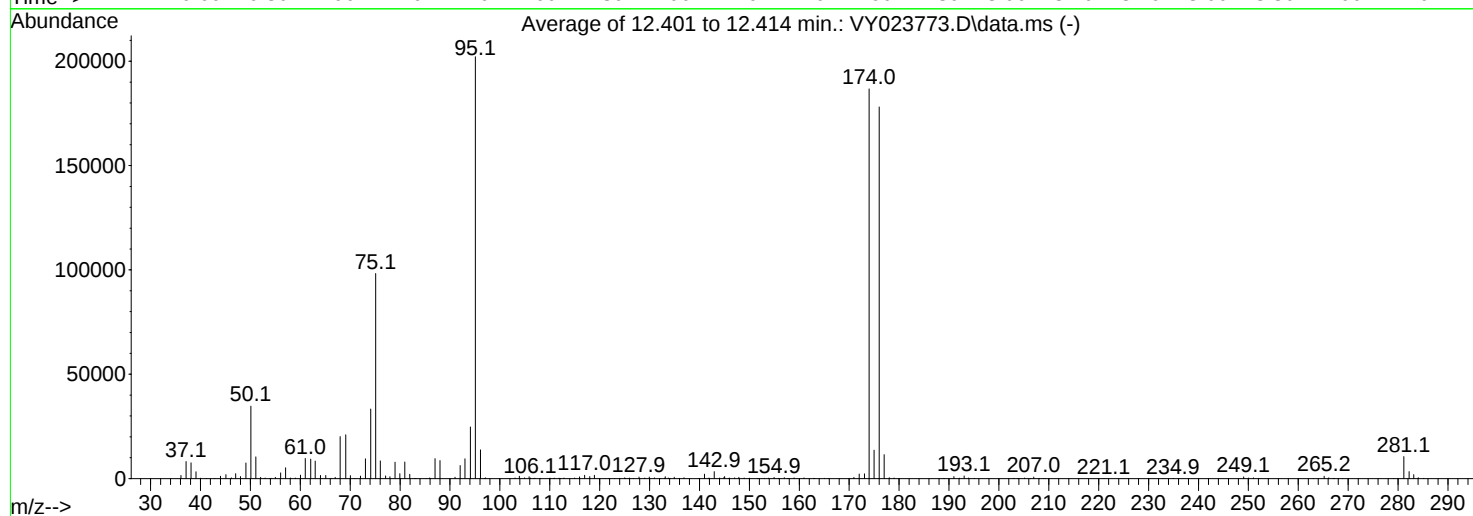


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY111325\  
Data File : VY023773.D  
Acq On : 13 Nov 2025 09:06  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y110425S.M  
Title : SW846 8260  
Last Update : Wed Nov 05 04:41:50 2025

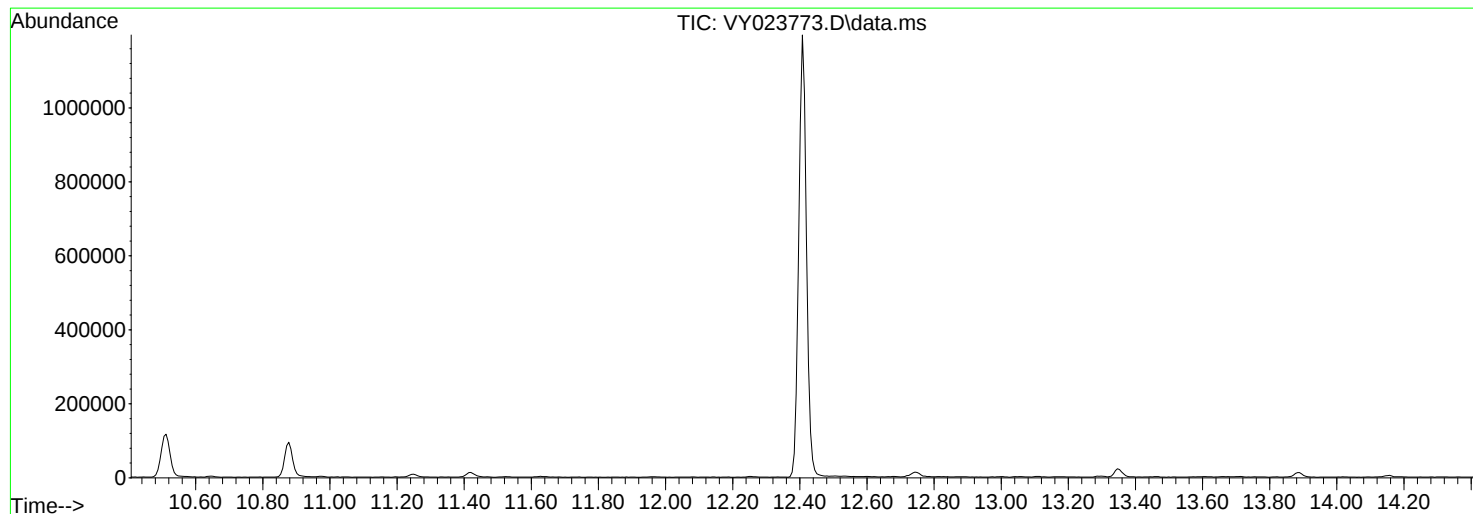

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 17.2         | 34712      | PASS                |
| 75             | 95              | 30              | 60              | 48.6         | 98232      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 202133     | PASS                |
| 96             | 95              | 5               | 9               | 6.8          | 13776      | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 2267       | PASS                |
| 174            | 95              | 50              | 100             | 92.4         | 186773     | PASS                |
| 175            | 174             | 5               | 9               | 7.3          | 13635      | PASS                |
| 176            | 174             | 95              | 101             | 95.4         | 178091     | PASS                |
| 177            | 176             | 5               | 9               | 6.4          | 11479      | PASS                |