
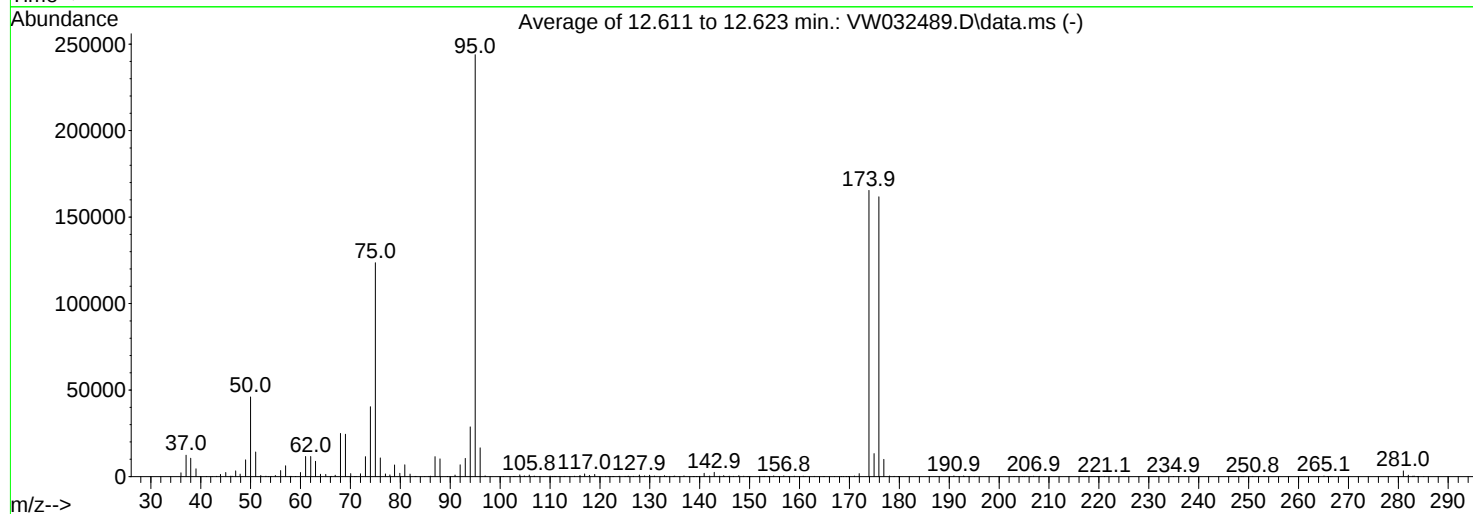


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111925\
Data File : VW032489.D
Acq On : 19 Nov 2025 09:32
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111025S.M
Title : SW846 8260
Last Update : Tue Nov 11 03:48:21 2025

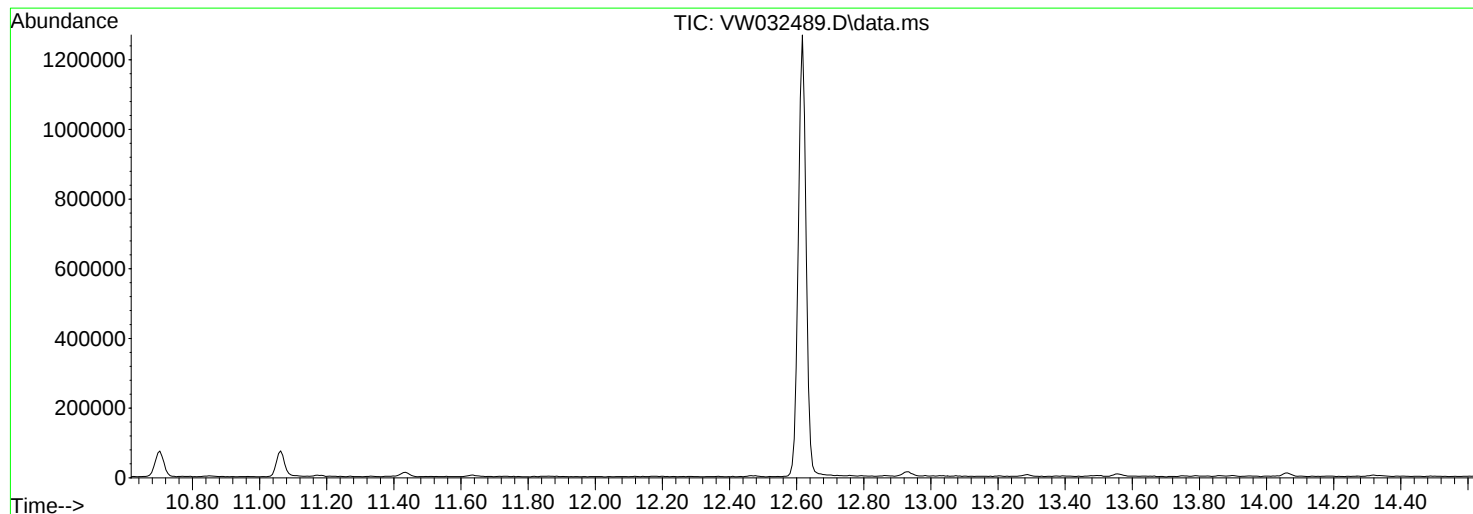

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1748

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	45992	PASS
75	95	30	60	50.7	123660	PASS
95	95	100	100	100.0	243861	PASS
96	95	5	9	6.8	16613	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.8	165419	PASS
175	174	5	9	8.0	13264	PASS
176	174	95	101	97.8	161728	PASS
177	176	5	9	6.2	9979	PASS