


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL111925\
Data File : VL043231.D
Acq On : 19 Nov 2025 08:43
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111825AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Nov 19 01:11:25 2025

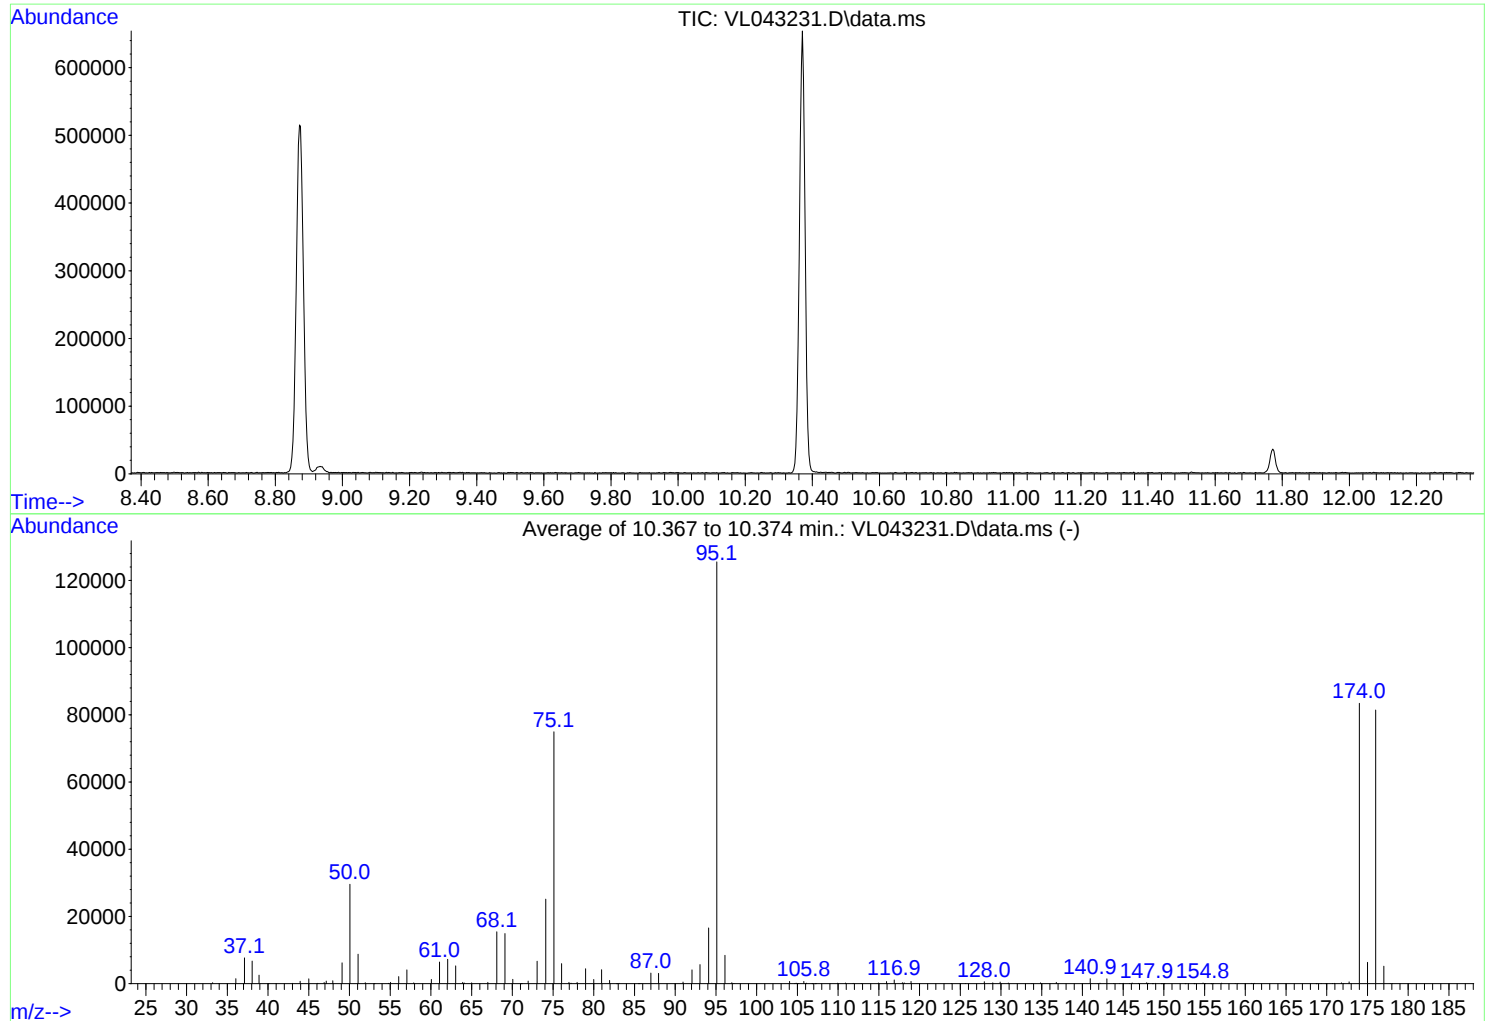

AutoFind: Scans 3176, 3177, 3178; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	29565	PASS
75	95	30	66	59.7	74981	PASS
95	95	100	100	100.0	125539	PASS
96	95	5	9	6.7	8409	PASS
173	174	0.00	2	0.6	526	PASS
174	95	50	120	66.5	83440	PASS
175	174	4	9	7.6	6330	PASS
176	174	93	101	97.6	81429	PASS
177	176	5	9	6.4	5212	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.20	305	46.10	102	56.05	2124	68.10	1544
34.00	55	46.90	316	57.05	4098	69.10	1491
36.05	1481	47.15	756	57.90	262	70.05	129
37.10	7656	47.95	880	60.05	1242	71.10	1
38.05	6712	49.10	6207	61.05	6441	71.95	750
38.90	2533	50.05	29565	62.05	7245	73.05	6678
40.00	1	51.05	8747	63.05	5288	74.10	25157
41.00	43	51.95	278	63.90	365	75.10	74981
43.00	117	53.00	26	64.10	180	76.05	5967
43.95	738	54.80	109	65.00	241	76.95	378
45.00	1454	55.05	367	67.00	374	77.20	165

Average of 10.367 to 10.374 min.: VL043231.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.95	393	90.95	470	105.10	73	116.90	1107
79.00	4436	92.05	4081	105.80	692	117.90	299
80.00	1224	93.05	5648	106.10	141	118.10	239
80.95	4170	94.10	16585	106.80	27	118.95	691
81.95	980	95.10	125539	107.20	24	123.90	48
82.80	25	96.10	8409	109.95	150	125.65	51
83.10	97	96.95	268	110.90	201	127.95	557
85.50	31	97.20	62	111.85	81	129.00	257
85.80	37	104.05	650	112.85	52	129.90	463
87.00	3145	104.70	50	114.95	215	130.90	192
87.95	3053	104.85	169	115.95	601	133.80	39

Average of 10.367 to 10.374 min.: VL043231.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
134.85	229	146.90	107	155.10	43	170.70	33
136.80	365	147.90	285	155.80	24	170.95	127
140.95	1489	148.10	107	156.10	35	171.80	216
141.90	79	148.60	24	157.10	130	172.10	59
142.15	150	148.95	97	158.75	72	172.75	526
143.00	1415	149.70	29	159.10	35	174.00	83440
143.85	63	150.00	30	160.80	94	175.00	6330
144.60	69	152.60	23	161.10	127	176.00	81429
145.00	97	153.00	39	168.70	22	177.00	5212
145.80	44	153.70	17	169.30	58	177.80	77
146.10	207	154.80	191	169.90	27	178.05	76

Instrument :

MSVOA_L

ClientSampleId :

BFB