
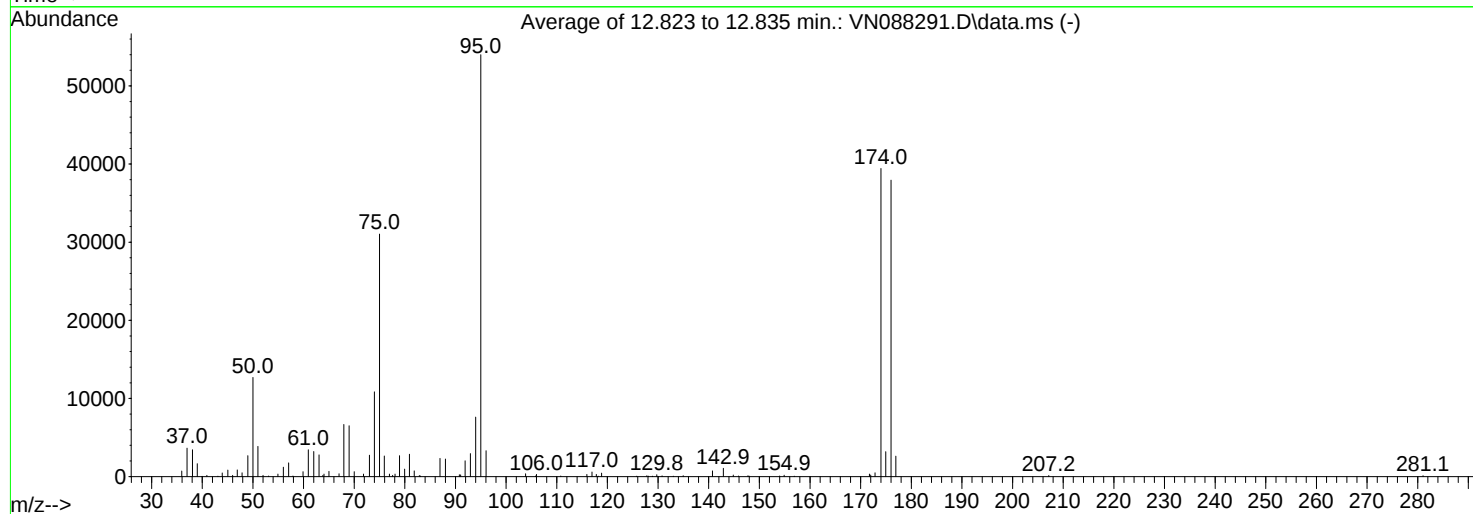


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111725\
Data File : VN088291.D
Acq On : 17 Nov 2025 08:32
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 19 01:25:31 2025

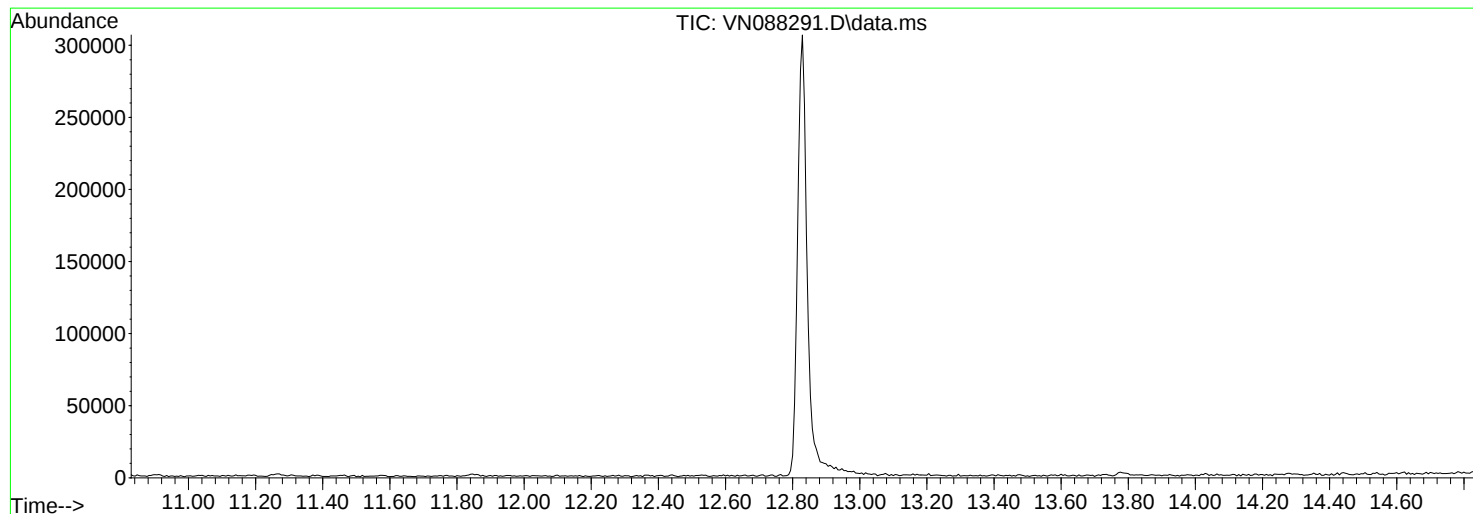

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	12690	PASS
75	95	30	60	57.5	31029	PASS
95	95	100	100	100.0	53987	PASS
96	95	5	9	6.1	3298	PASS
173	174	0.00	2	1.2	476	PASS
174	95	50	100	73.1	39440	PASS
175	174	5	9	8.1	3185	PASS
176	174	95	101	96.2	37944	PASS
177	176	5	9	6.9	2603	PASS