


LB137932
INSTRUMENT ID : CV1

Reviewed By: jaswal
On: 11/18/2025 5:35:32 PM
Inst Id : CV1
LB : LB137932

7471B

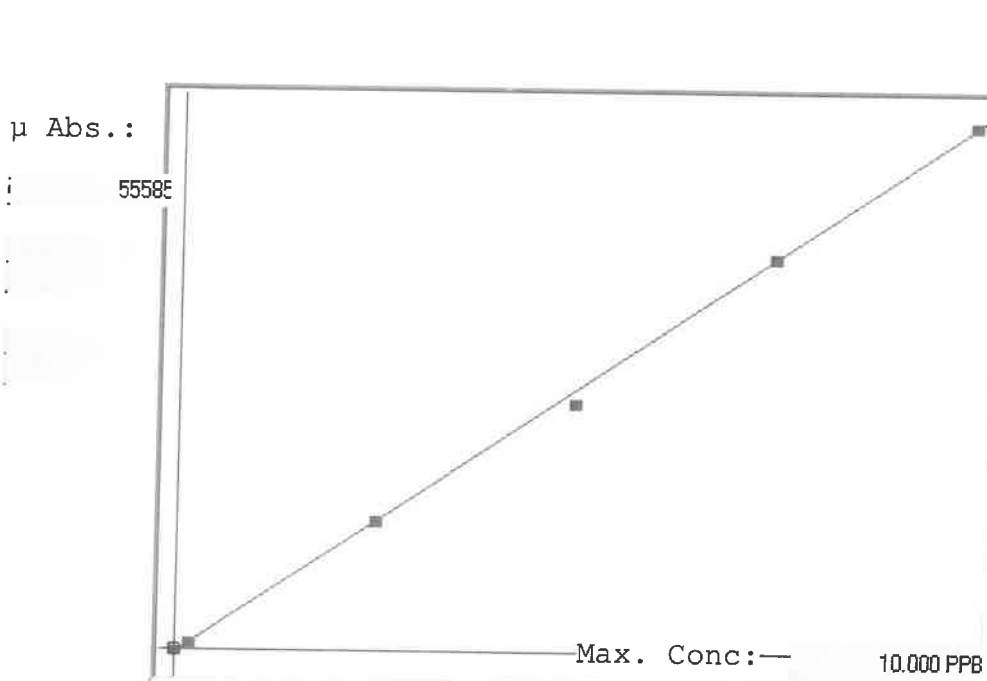

Linear

A= 0.0000e+000

B= 1.7980e-004

C= 5.9952e-002

Rho= 0.9996477

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.076	0.076	88	0.000	88				
0.2	0.200	0.208	0.008	822	0.0 %	822				
2.5	2.500	2.520	0.020	13683	0.0 %	13683				
5.0	5.000	4.787	-0.213	26290	0.0 %	26290				
7.5	7.500	7.555	0.055	41684	0.0 %	41684				
10.0	10.000	10.054	0.054	55585	0.0 %	55585				

LB137932 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 18 Nov 2025 08:57:53

Type	Sample ID	Extended ID	Conc.	µ Abs	Units	Type	Std Cond Method	Date
S	0.0 - 1	50	-	88	PPB	Std	0.00007471B	18 Nov 2025 09:36:01
S	0.2 - 1	50.2	-	822	PPB	Std	0.20007471B	18 Nov 2025 09:41:13
S	2.5 - 1	52.5	-	13683	PPB	Std	2.50007471B	18 Nov 2025 09:43:30
S	5.0 - 1	55.0	-	26290	PPB	Std	5.00007471B	18 Nov 2025 09:45:47
S	7.5 - 1	57.5	-	41684	PPB	Std	7.50007471B	18 Nov 2025 09:48:04
S	10.0 - 1	510.0	-	55585	PPB	Std	10.00007471B	18 Nov 2025 09:50:21
U	ICV119 - 1	ICV119	4.2190	23131	PPB	SMPL	-7471B	18 Nov 2025 09:54:14
U	ICB119 - 1	ICB119	0.0490	-61	PPB	SMPL	-7471B	18 Nov 2025 09:56:29
U	CCV07 - 1	CCV07	4.9039	26940	PPB	SMPL	-7471B	18 Nov 2025 10:01:18
U	CCB07 - 1	CCB07	0.0484	-64	PPB	SMPL	-7471B	18 Nov 2025 10:03:33
U	CRA - 1	CRA	0.2095	832	PPB	SMPL	-7471B	18 Nov 2025 10:05:49
U	HighStd - 1	HighStd	10.1337	56026	PPB	SMPL	-7471B	18 Nov 2025 10:08:13
U	ChkStd - 1	ChkStd	7.1156	39241	PPB	SMPL	-7471B	18 Nov 2025 10:10:36
U	PB170581BL - 1	PBS	0.0267	-185	PPB	SMPL	-7471B	18 Nov 2025 10:13:02
U	PB170581BS - 1	LCSS	4.1737	22879	PPB	SMPL	-7471B	18 Nov 2025 10:18:21
U	Q3645-01 - 1	HD-02-11142025	0.2104	837	PPB	SMPL	-7471B	18 Nov 2025 10:20:36
U	Q3646-01 - 1	SU-03-11142025	0.7247	3697	PPB	SMPL	-7471B	18 Nov 2025 10:22:55
U	Q3647-01 - 1	VNJ-212	0.0891	162	PPB	SMPL	-7471B	18 Nov 2025 10:25:12
U	Q3648-01 - 1	OR-02-111425	15.3996	85313	PPB	SMPL	-7471B	18 Nov 2025 10:27:29
U	Q3649-01 - 1	B5-0.0-0.5-20251114	-0.1087	-938	PPB	SMPL	-7471B	18 Nov 2025 10:29:44
U	CCV08 - 1	CCV08	4.6922	25763	PPB	SMPL	-7471B	18 Nov 2025 10:32:13
U	CCB08 - 1	CCB08	0.0355	-136	PPB	SMPL	-7471B	18 Nov 2025 10:34:28
U	Q3649-03 - 1	DUPE-0.0-0.5-20251114	0.6098	3058	PPB	SMPL	-7471B	18 Nov 2025 10:36:53
U	Q3649-06 - 1	B4-0.0-0.5-20251114	0.2915	1288	PPB	SMPL	-7471B	18 Nov 2025 10:44:10
U	Q3649-06DUP - 1	B4-0.0-0.5-20251114DUP	0.2809	1229	PPB	SMPL	-7471B	18 Nov 2025 10:46:26
U	Q3649-06MS - 1	B4-0.0-0.5-20251114MS	3.2322	17643	PPB	SMPL	-7471B	18 Nov 2025 10:48:41
U	Q3649-06MSD - 1	B4-0.0-0.5-20251114MSD	3.5165	19224	PPB	SMPL	-7471B	18 Nov 2025 10:53:39
U	Q3649-08 - 1	B3-0.0-0.5-20251114	0.2372	986	PPB	SMPL	-7471B	18 Nov 2025 10:55:55
U	Q3649-06LX5 - 1		0.1240	356	PPB	SMPL	-7471B	18 Nov 2025 10:58:13
U	Q3649-06A - 1		4.2870	23509	PPB	SMPL	-7471B	18 Nov 2025 11:00:30
U	CCV09 - 1	CCV09	4.9263	27065	PPB	SMPL	-7471B	18 Nov 2025 11:02:47
U	CCB09 - 1	CCB09	0.0535	-36	PPB	SMPL	-7471B	18 Nov 2025 11:05:04
U	Q3652-01 - 1		0.2673	1153	PPB	SMPL	-7471B	18 Nov 2025 11:07:22
U	Q3656-01 - 1		0.1820	679	PPB	SMPL	-7471B	18 Nov 2025 11:09:37
U	Q3658-01 - 1		0.3721	1736	PPB	SMPL	-7471B	18 Nov 2025 11:11:53
U	Q3648-01DLX5 - 1		2.1786	11783	PPB	SMPL	-7471B	18 Nov 2025 11:14:08
U	CCV10 - 1	CCV10	4.6459	25505	PPB	SMPL	-7471B	18 Nov 2025 11:16:24
U	CCB10 - 1	CCB10	0.0573	-15	PPB	SMPL	-7471B	18 Nov 2025 11:21:38