

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111725\
 Data File : PO115146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2025 17:35
 Operator : YP/AJ
 Sample : Q3649-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B4-0.0-0.5-20251114

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/19/2025
 Supervised By :Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 01:39:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347	3.647	152.1E6	97667617	21.616	21.865
2) SA Decachlor...	9.930	8.638	86798819	80150134	19.637m	20.531

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111725\
Data File : PO115146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2025 17:35
Operator : YP/AJ
Sample : Q3649-06
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B4-0.0-0.5-20251114


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/19/2025
Supervised By :Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:39:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

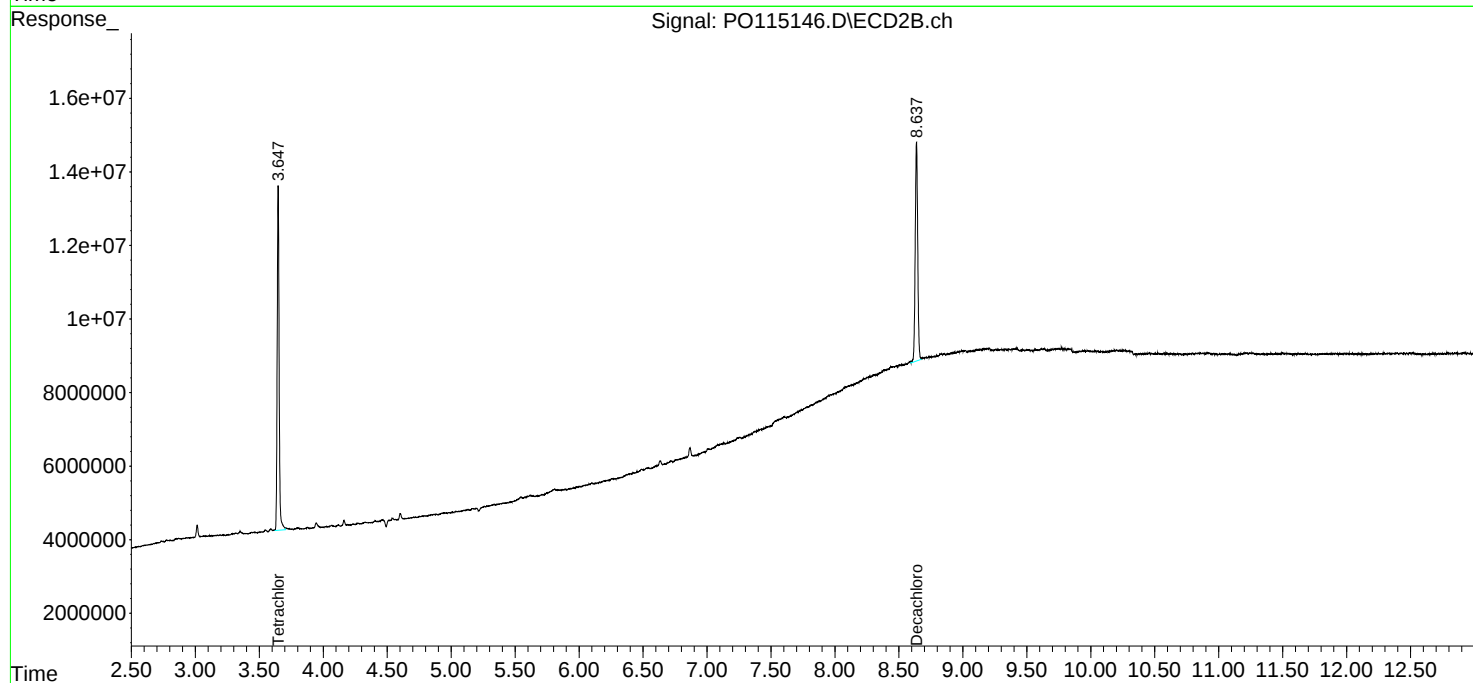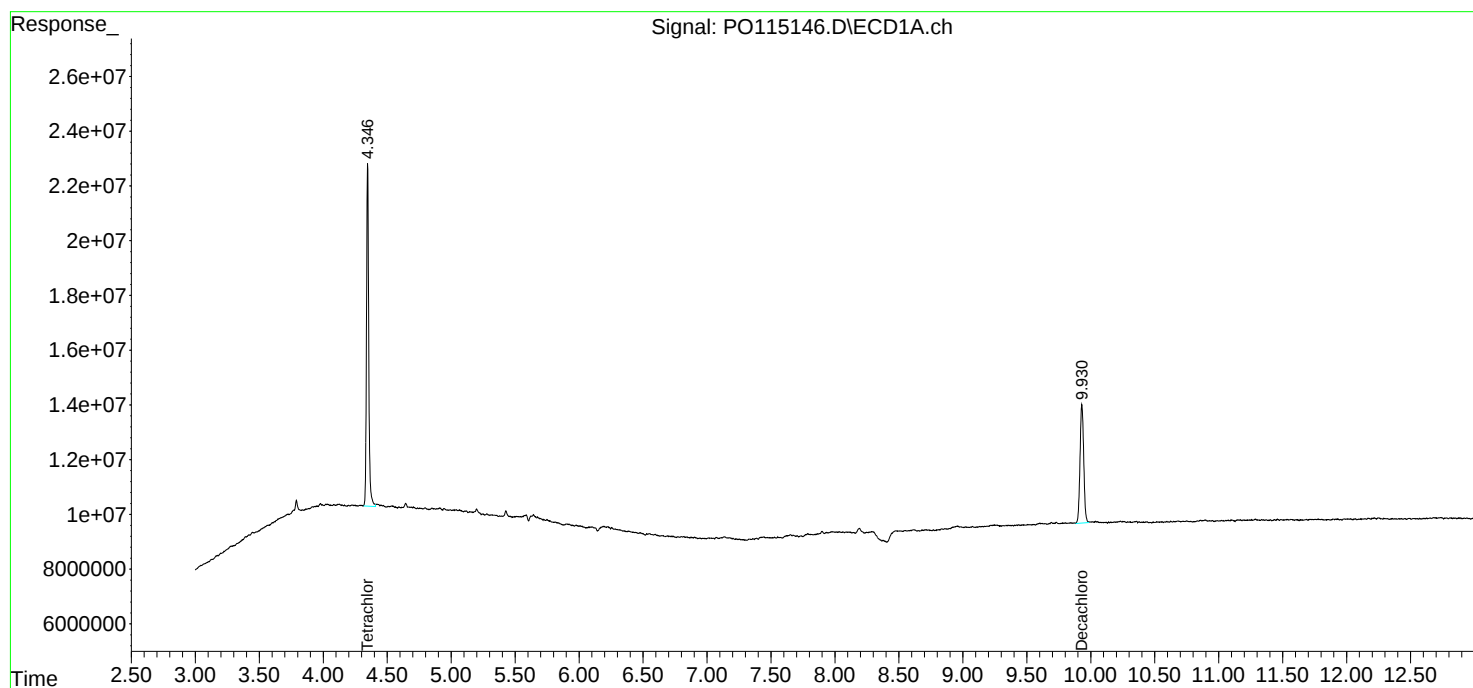

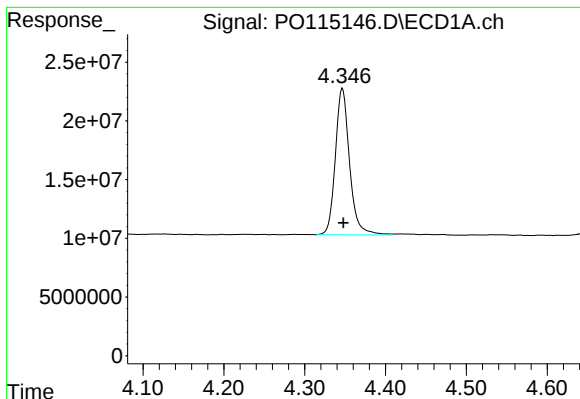


#1 Tetrachloro-m-xylene

R.T.: 4.347 min
Delta R.T.: -0.001 min
Response: 152135796
Conc: 21.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
B4-0.0-0.5-20251114


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/19/2025
Supervised By :Sohil Jodhani 11/19/2025

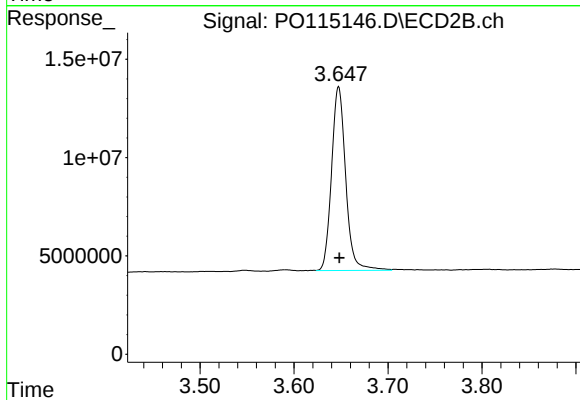


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 97667617
Conc: 21.87 ng/ml

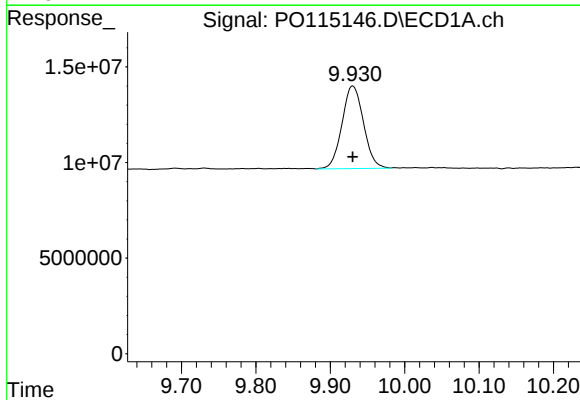

#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: 0.000 min
Response: 86798819
Conc: 19.64 ng/ml m

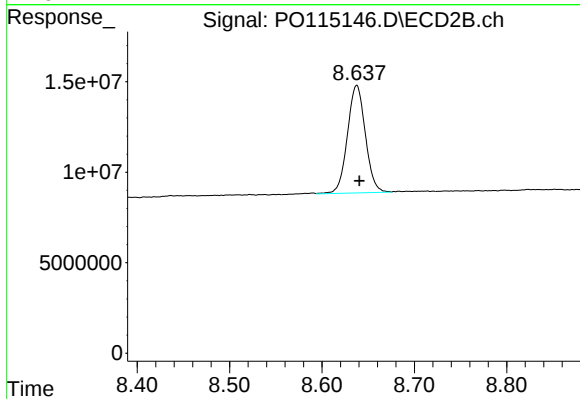

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: -0.003 min
Response: 80150134
Conc: 20.53 ng/ml