


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111725\
Data File : BF144262.D
Acq On : 17 Nov 2025 12:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

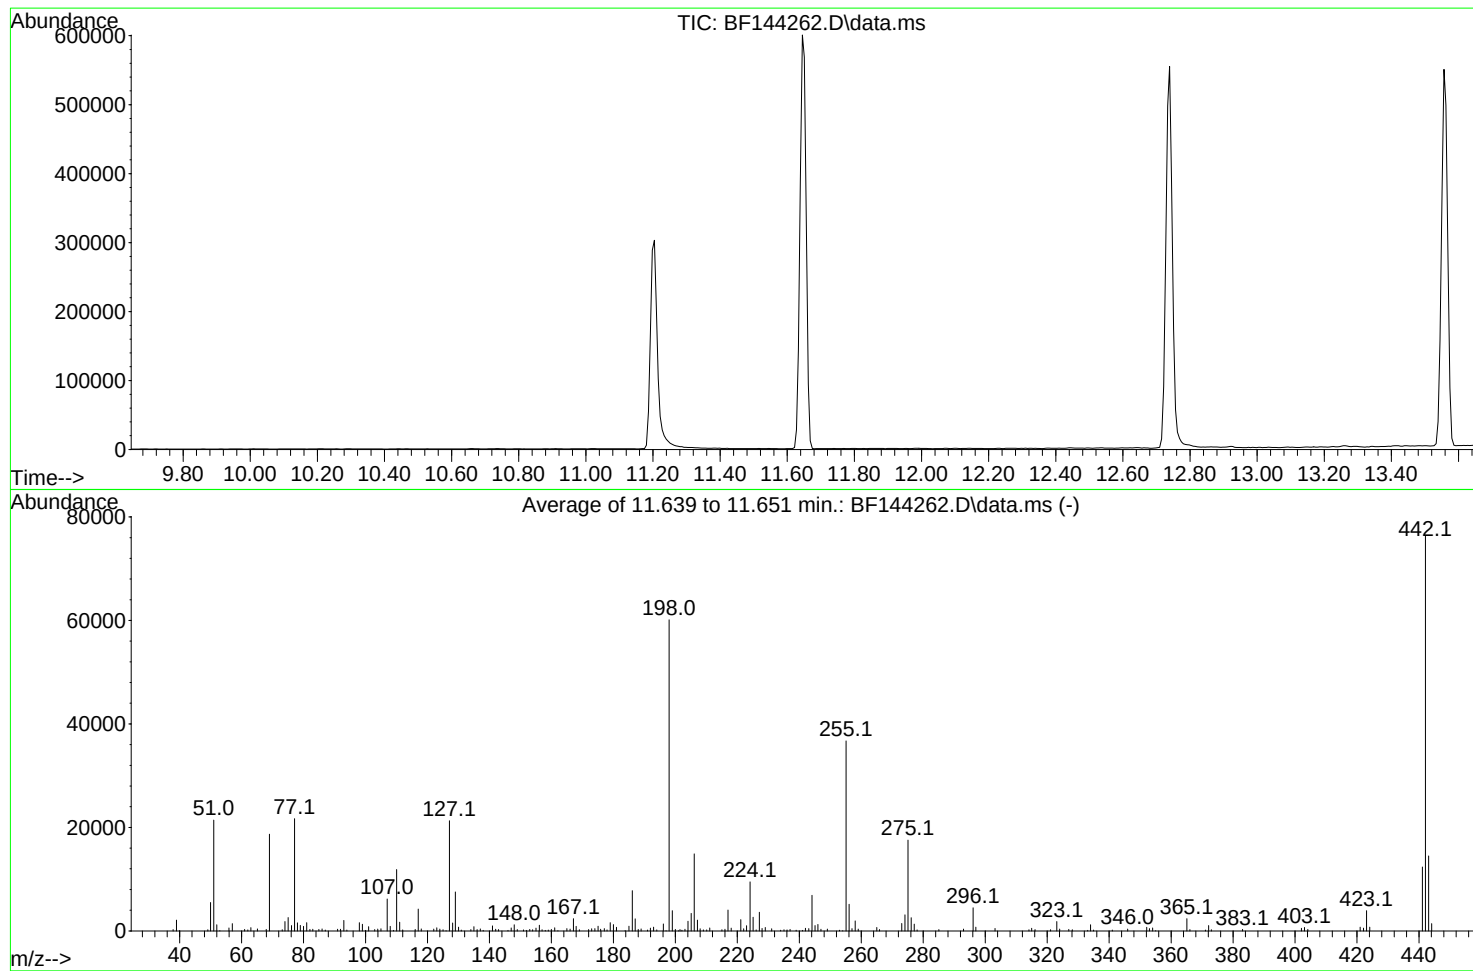




AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1600

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	311	PASS
69	69	100	100	100.0	18691	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.1	53	PASS
198	198	100	100	100.0	60120	PASS
199	198	5	9	6.5	3923	PASS
365	198	1	100	3.9	2374	PASS
441	443	0.01	150	85.2	12351	PASS
442	442	100	100	100.0	76299	PASS
443	442	15	24	19.0	14500	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111725\
Data File : BF144262.D
Acq On : 17 Nov 2025 12:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 17 12:57:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

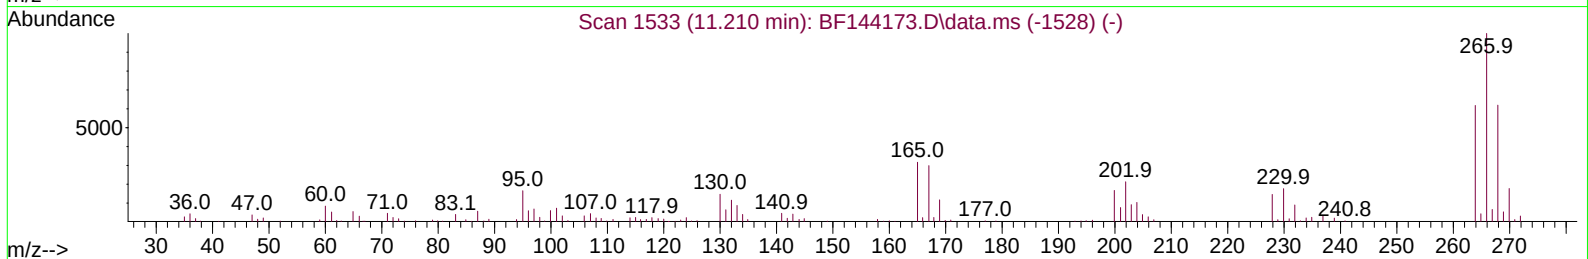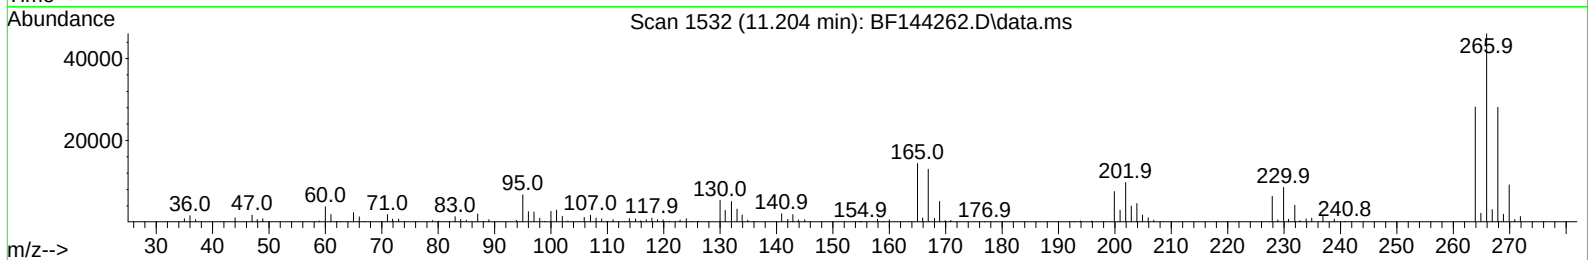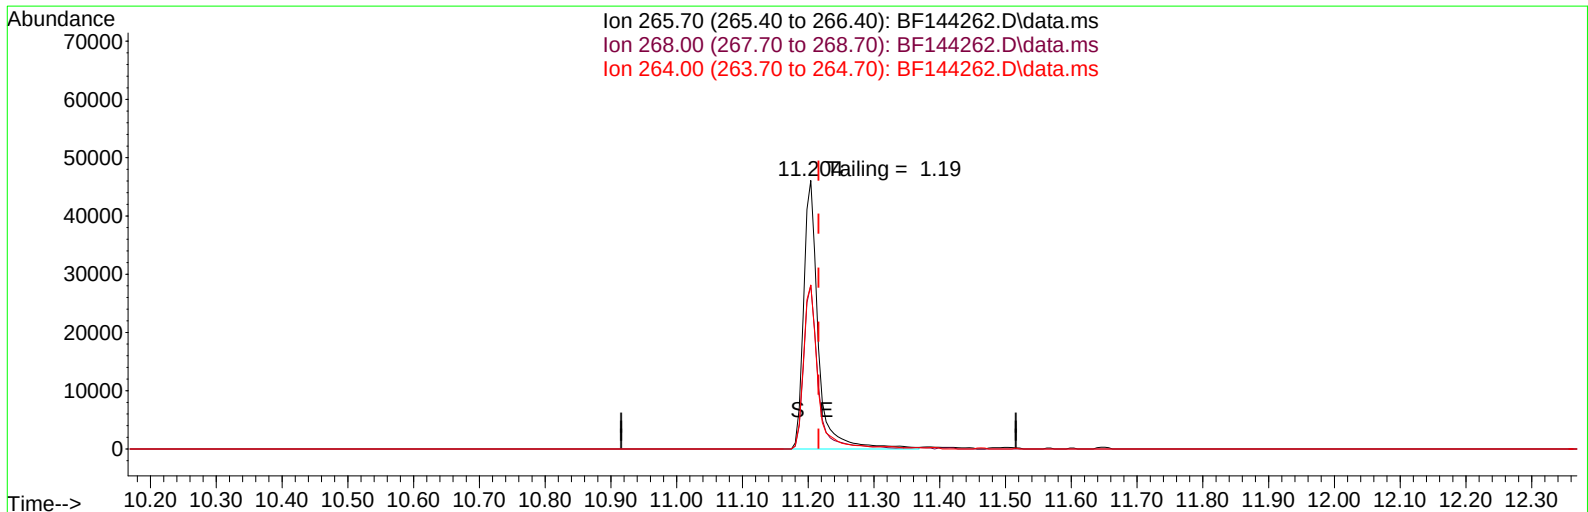

TIC: BF144262.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.012) 32389.41 ng




response 72018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	60.95
264.00	61.80	61.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111725\
Data File : BF144262.D
Acq On : 17 Nov 2025 12:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 17 12:57:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

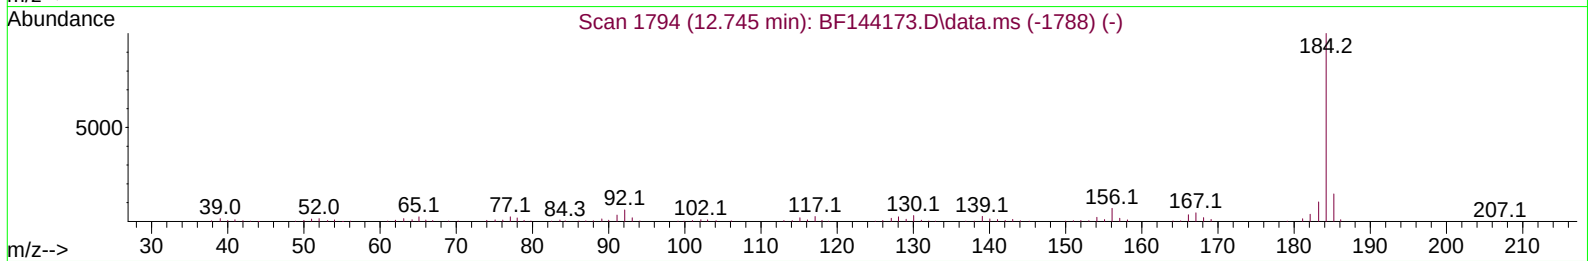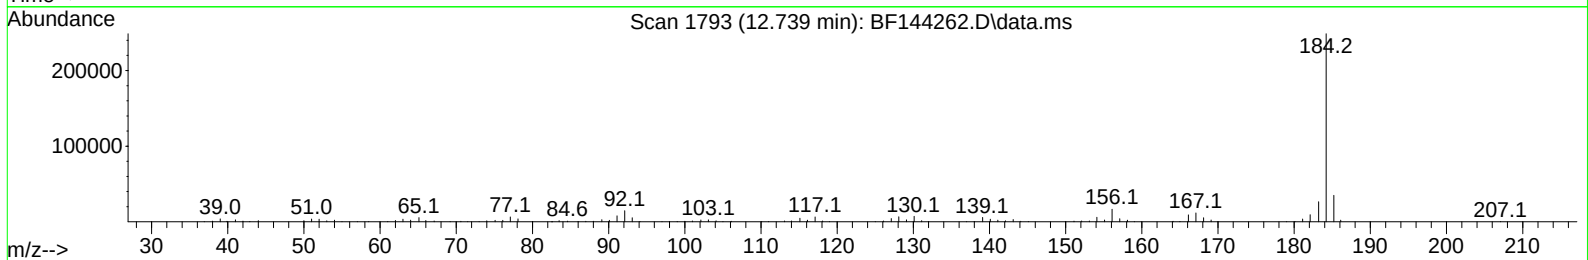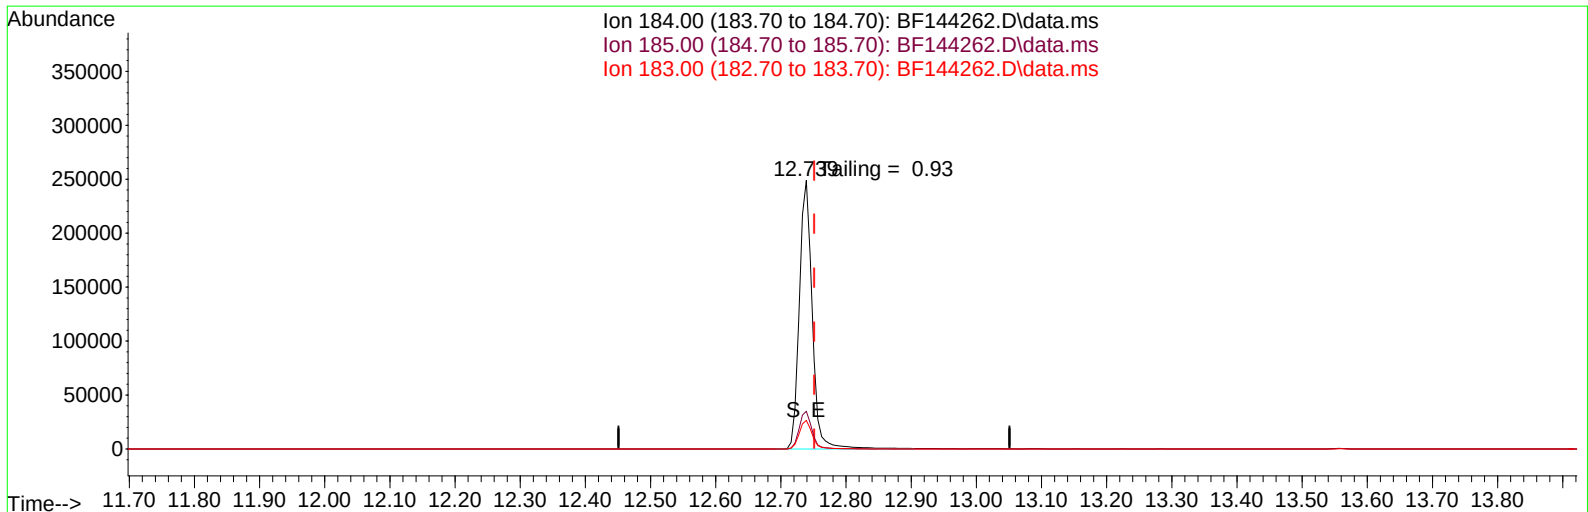

TIC: BF144262.D\data.ms

(77) Benzidine

12.739min (-0.012) 0.00 ng

response 342050

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.06
183.00	10.40	10.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/17/2025	BNA_F	<u>BF144262.D</u>
Compound Name	Response	Retention Time
DDT	152055	13.557
DDD	2007	13.263
DDE	581	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2588	154643	1.67

Instrument :
BNA_F
ClientSampleId :
DFTPP