
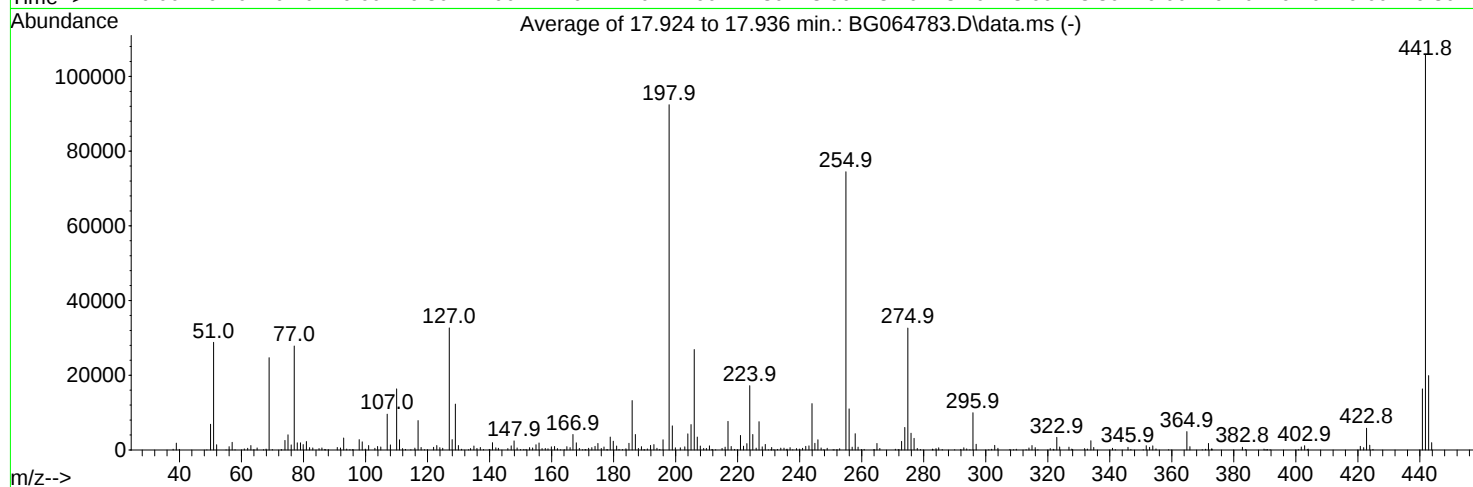


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111725\
Data File : BG064783.D
Acq On : 17 Nov 2025 12:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

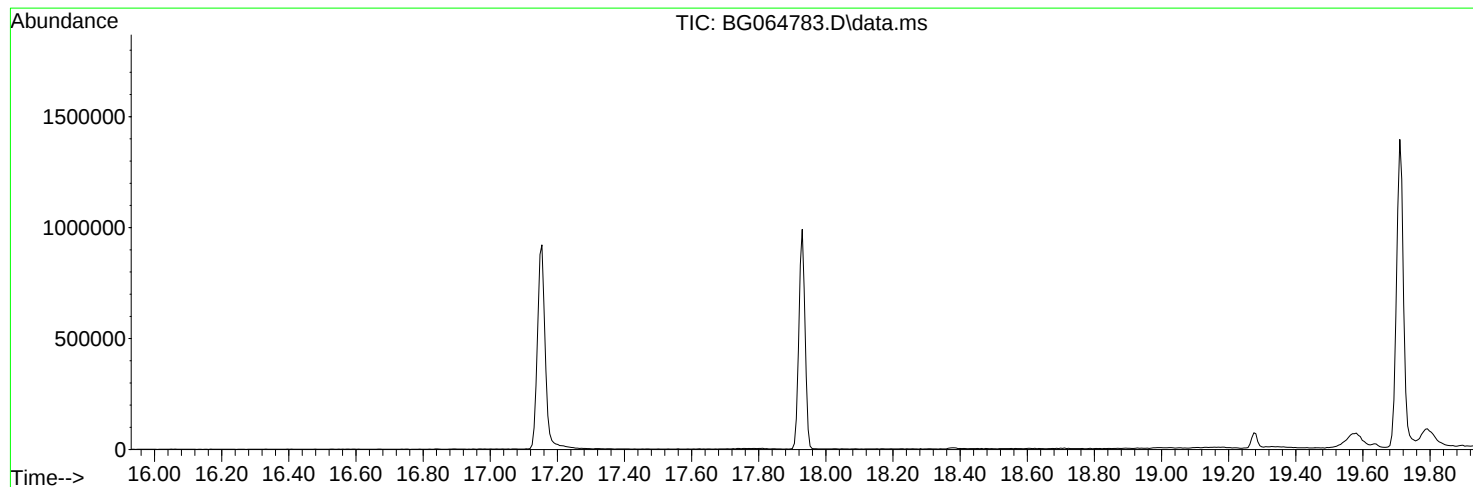

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.9	220	PASS
69	69	100	100	100.0	24677	PASS
70	69	0.00	2	0.5	129	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92429	PASS
199	198	5	9	7.0	6451	PASS
365	198	1	100	5.3	4890	PASS
441	443	0.01	150	82.0	16332	PASS
442	442	100	100	100.0	105707	PASS
443	442	15	24	18.8	19907	PASS