

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111925\
 Data File : PO115209.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2025 11:00
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/20/2025
 Supervised By :Sohil Jodhani 11/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 01:38:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.342	3.645	177.3E6	110.5E6	25.192	24.731
2) SA Decachlor...	9.920	8.632	117.6E6	106.4E6	26.602m	27.259

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111925\
Data File : PO115209.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2025 11:00
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/20/2025
Supervised By :Sohil Jodhani 11/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 01:38:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

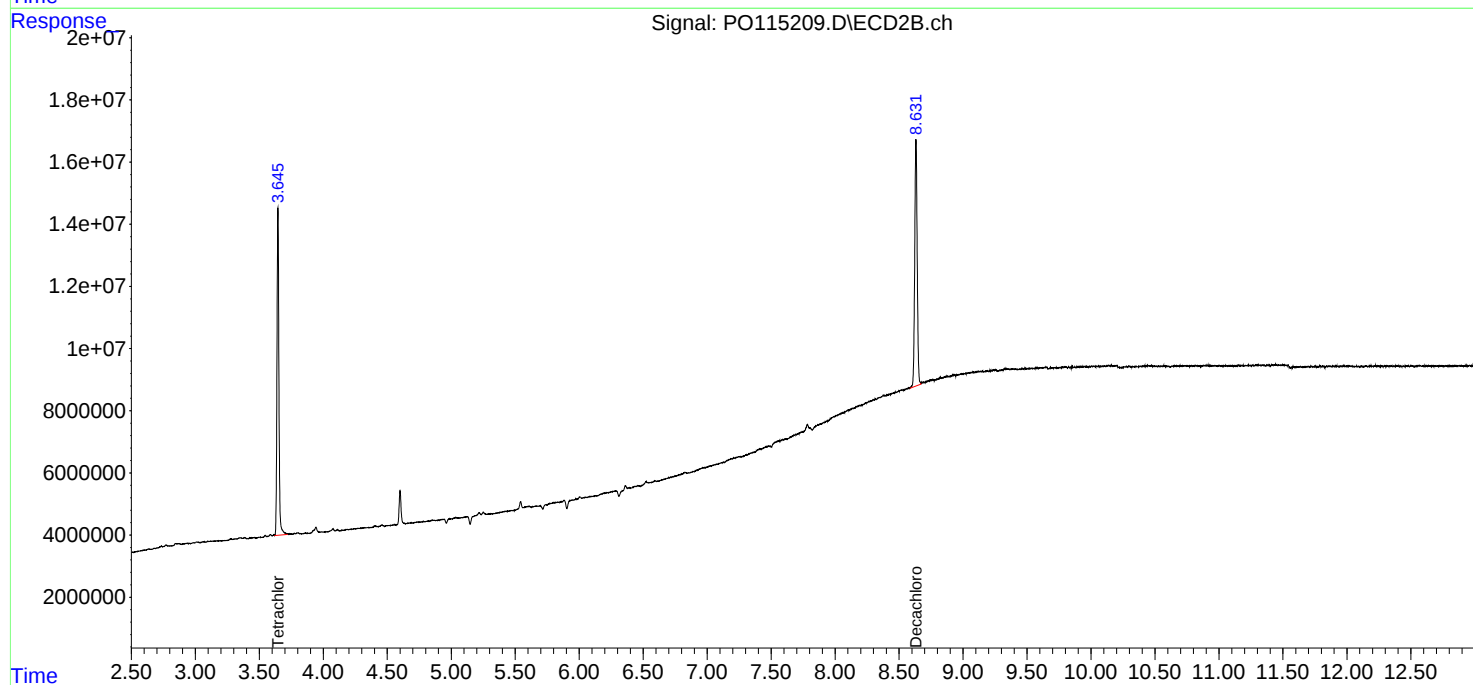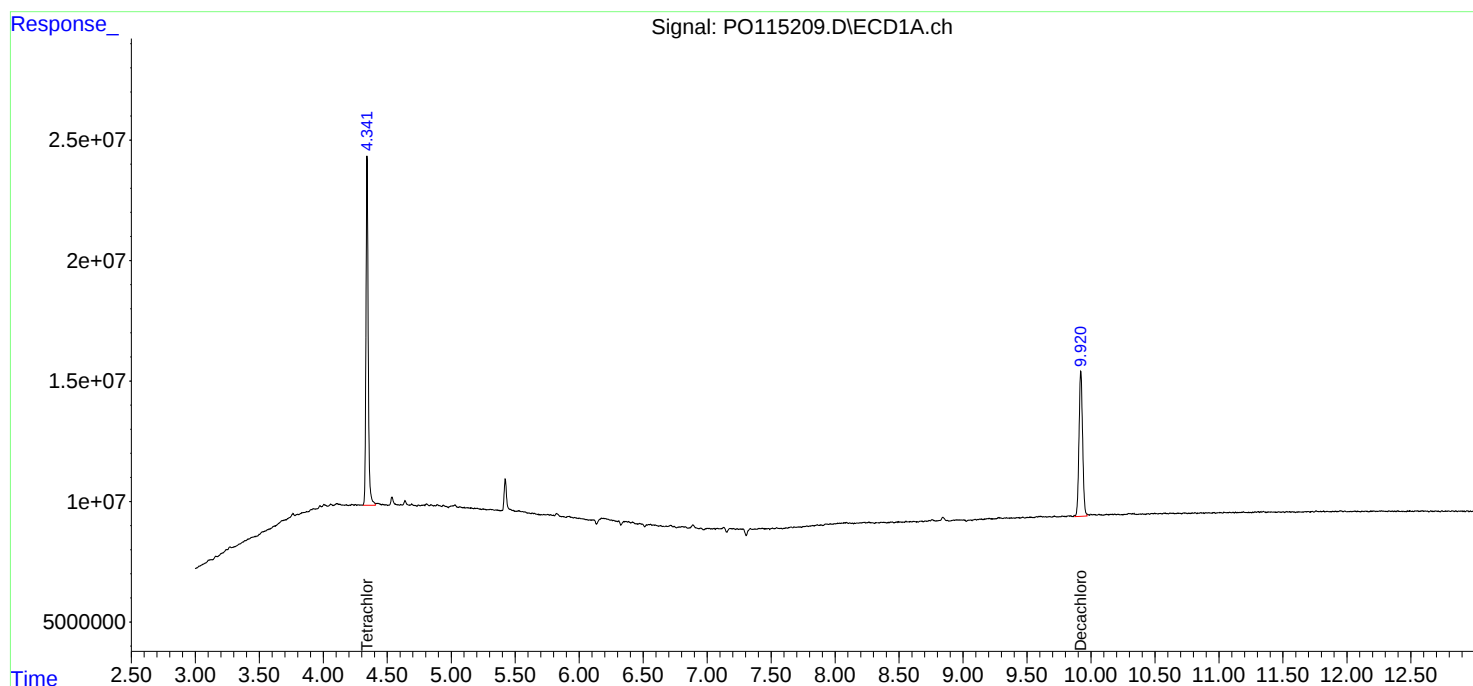

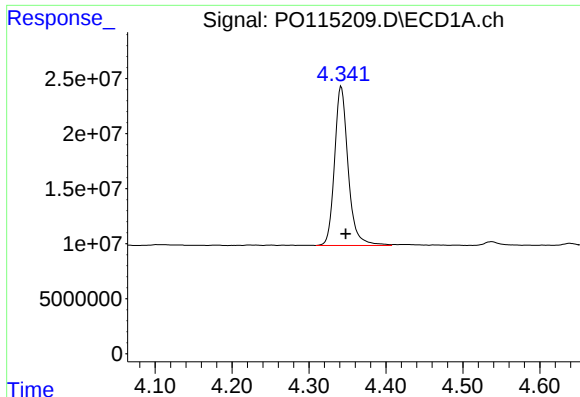


#1 Tetrachloro-m-xylene

R.T.: 4.342 min
Delta R.T.: -0.006 min
Response: 177302984
Conc: 25.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/20/2025
Supervised By :Sohil Jodhani 11/20/2025

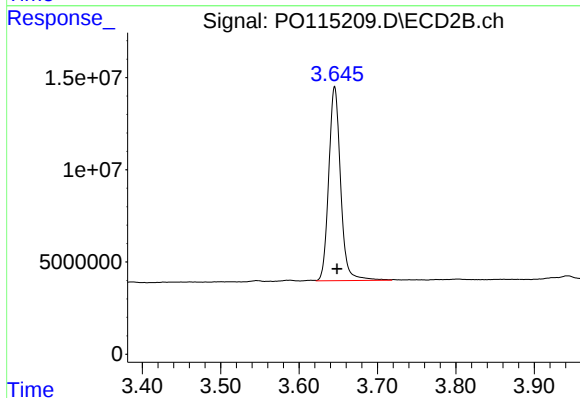


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.003 min
Response: 110467682
Conc: 24.73 ng/ml

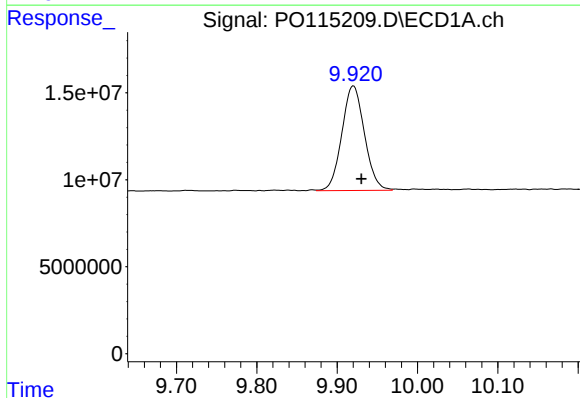

#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.011 min
Response: 117586316
Conc: 26.60 ng/ml m

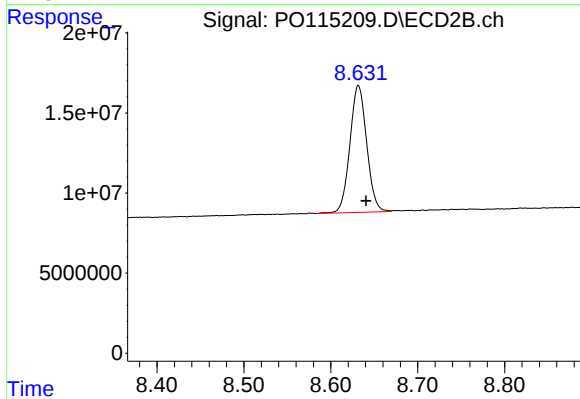

#2 Decachlorobiphenyl

R.T.: 8.632 min
Delta R.T.: -0.009 min
Response: 106415883
Conc: 27.26 ng/ml