


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112625\
Data File : BN038209.D
Acq On : 26 Nov 2025 18:07
Operator : RC/JU
Sample : SSTD3.296
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTD3.2230

Quant Time: Nov 28 21:36:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 28 21:34:25 2025
Response via : Initial Calibration

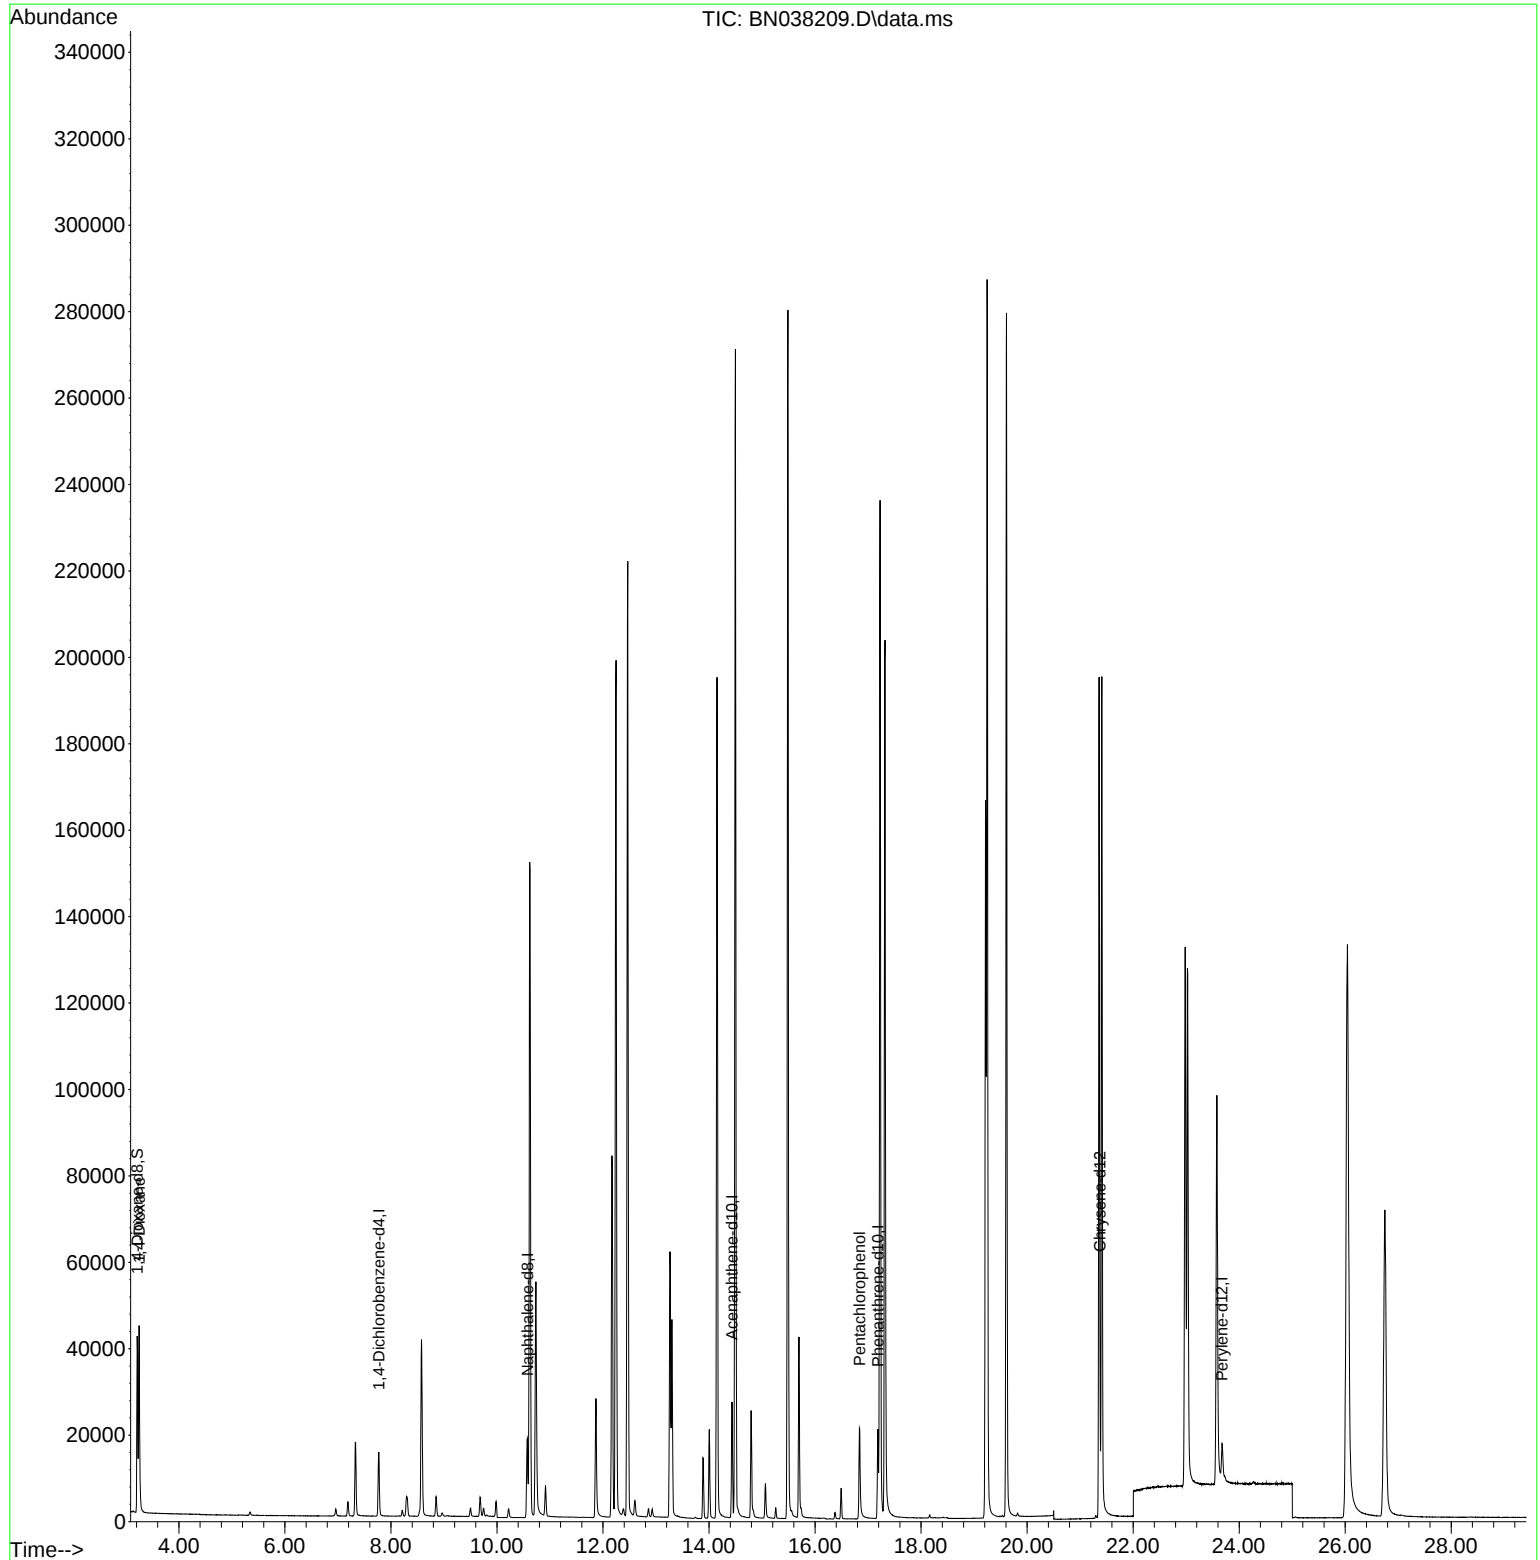

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112625\
 Data File : BN038209.D
 Acq On : 26 Nov 2025 18:07
 Operator : RC/JU
 Sample : SSTD3.296
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD3.2230

Quant Time: Nov 28 21:36:08 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 28 21:34:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.771	152	7804	0.400	ng/u1	0.00
4) Naphthalene-d8	10.573	136	25246	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.432	164	14374	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.184	188	24669	0.400	ng/u1	0.00
17) Chrysene-d12	21.374	240	14639	0.400	ng/u1	0.00
23) Perylene-d12	23.677	264	12532	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	24869	3.015	ng/u1	0.00
6) 2-Methylnaphthalene-d10	0.000	152	0d	0.000	ng/u1	
18) Fluoranthene-d10	0.000	212	0d	0.000	ng/u1	
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.248	88	28311	3.252	ng/u1	89
14) Pentachlorophenol	16.838	266	16804	2.907	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed