


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
Data File : BN038262.D
Acq On : 02 Dec 2025 19:28
Operator : RC/JU
Sample : Q3688-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
M-30I

Manual Integrations
APPROVED

Sohil
12/3/2025 3:29:37 PM

Quant Time: Dec 03 01:15:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 16:36:13 2025
Response via : Initial Calibration

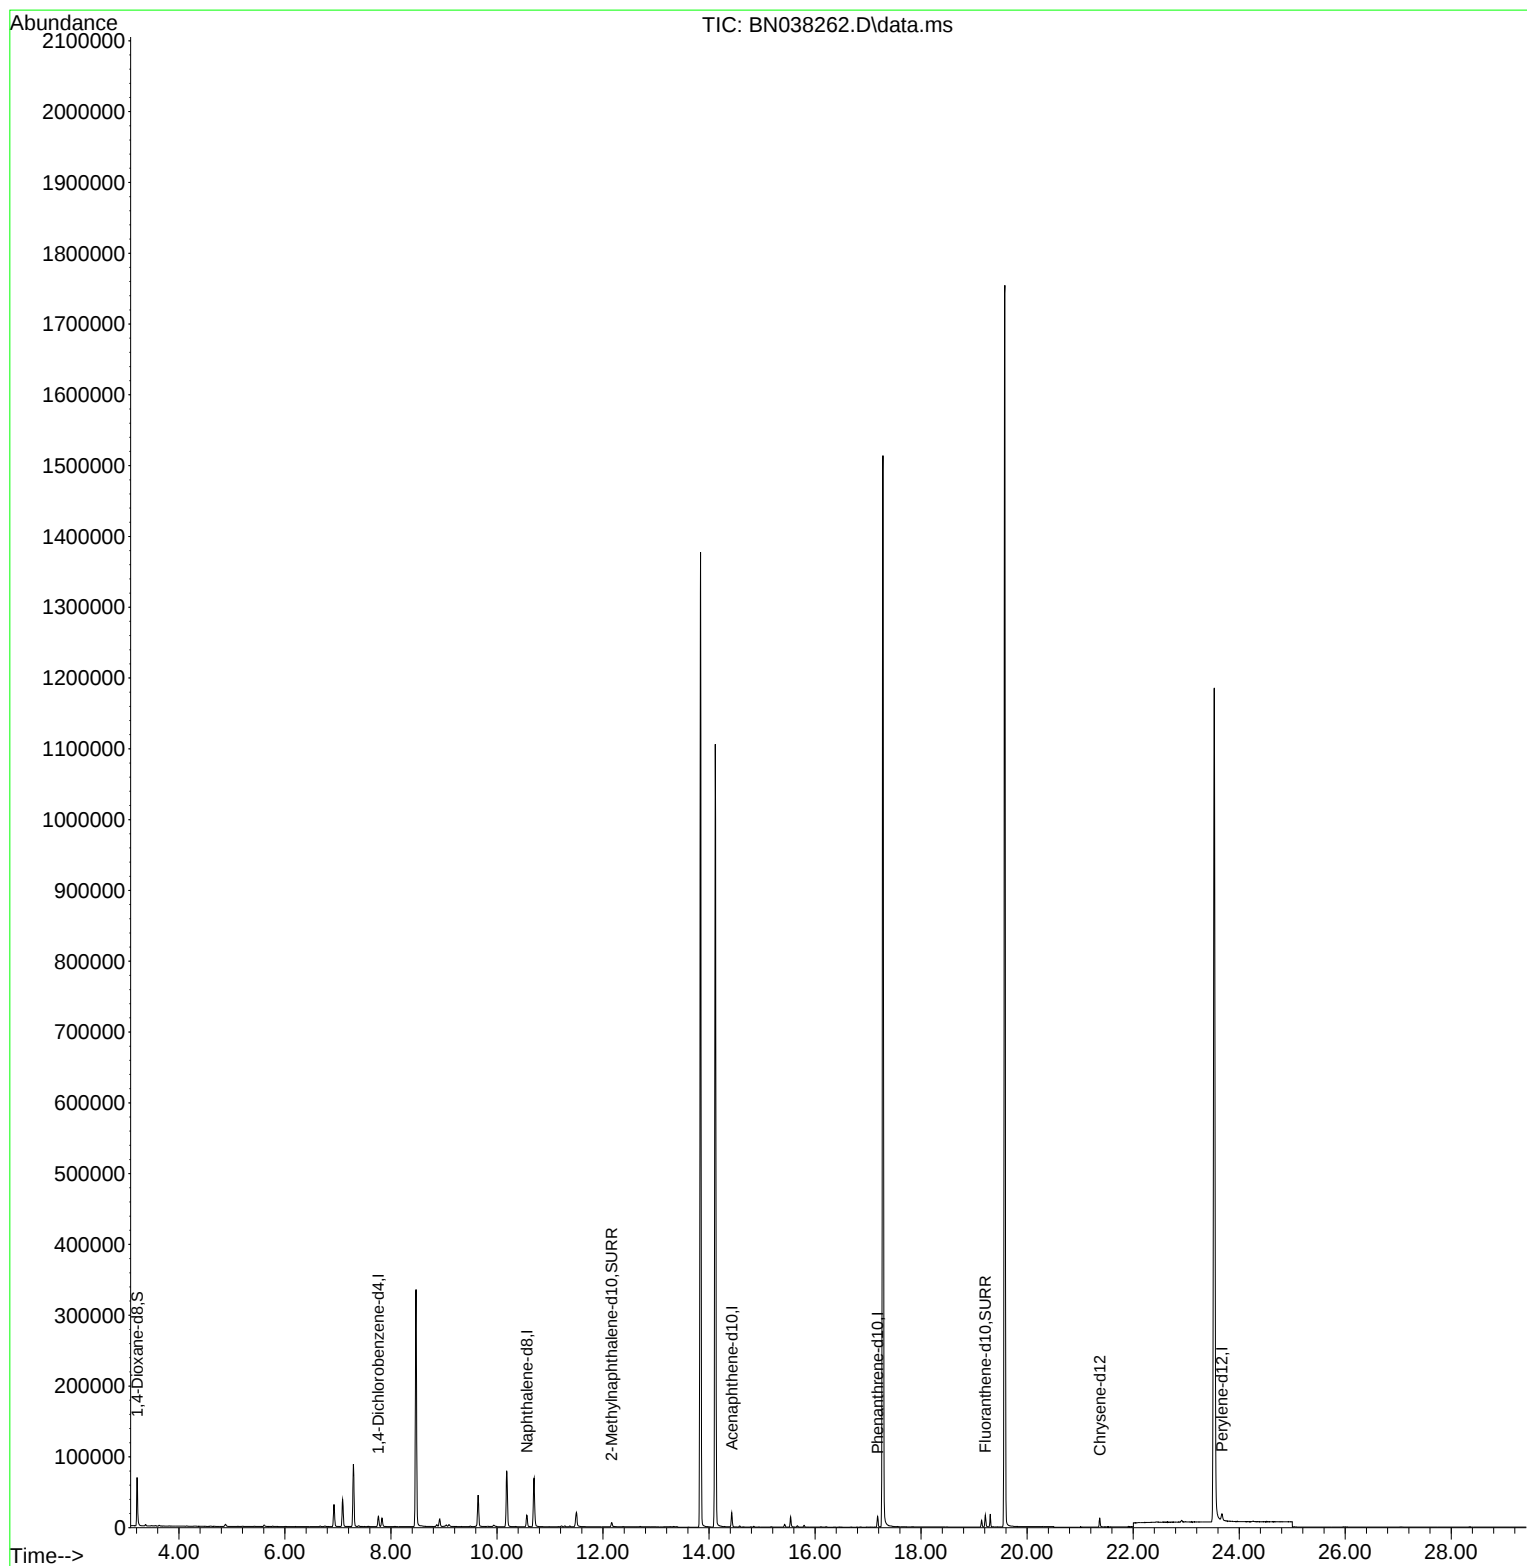

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120225\
 Data File : BN038262.D
 Acq On : 02 Dec 2025 19:28
 Operator : RC/JU
 Sample : Q3688-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 M-30I

Manual Integrations
 APPROVED

Sohil
 12/3/2025 3:29:37 PM

Quant Time: Dec 03 01:15:23 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN112625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 01 16:36:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.762	152	7205	0.400	ng/u1	0.00
4) Naphthalene-d8	10.562	136	21641	0.400	ng/u1	-0.01
9) Acenaphthene-d10	14.428	164	10686	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.179	188	17105m	0.400	ng/u1	0.00
17) Chrysene-d12	21.371	240	12386m	0.400	ng/u1	0.00
23) Perylene-d12	23.674	264	10853m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	41140	5.442	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.162	152	8062	0.261	ng/u1	-0.01
18) Fluoranthene-d10	19.211	212	17868m	0.371	ng/u1	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed