

SOP ID: MSFAM01.1-Sample Prep-3

Clean Up SOP #: N/A

Extraction Start Date : 11/25/2025

Matrix : Water

Extraction Start Time : 08:50

Weigh By: N/A

Extraction By: RS

Extraction End Date : 11/25/2025

Balance check: N/A

Filter By: RS

Extraction End Time : 16:20

Balance ID: N/A

pH Meter ID: N/A

Concentration By: EH

pH Strip Lot#: E3870

Hood ID: 6,7

Supervisor By : RUPESH

Extraction Method: ☐ Separatory Funnel ☒ Continuous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☐ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	0.5ML	0.8 PPM	SP6933
Surrogate	0.5ML	0.8 PPM	SP6934
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3986
Baked Na2SO4	N/A	EP2663
H2SO4 1:1	N/A	EP2657
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

pH Adjusted <2 with 1:1 H2SO4, 1.5ML Vial Lot # 2210443.

KD Bath ID: WATER BATH-1,2

Envap ID: N-EVAP-02

KD Bath Temperature: 60 °C


Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
11/25/25	RS (Ext Lab)	RCI/Post PCB
16:25	Preparation Group	Analysis Group

Analytical Method: MSFAM01.1-Sample Prep-3

Concentration Date: 11/25/2025

Sample ID	Client Sample ID	Test	g / ml	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB170742BL	SBLK742	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			
PB170742BS	SLCS742	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			
Q3688-22	RBGW-20251124	SVOC-SIMGrou p1	990	6	RUPESH	ritesh	1	E		
Q3688-23	M-285	SVOC-SIMGrou p1	960	6	RUPESH	ritesh	1	E		

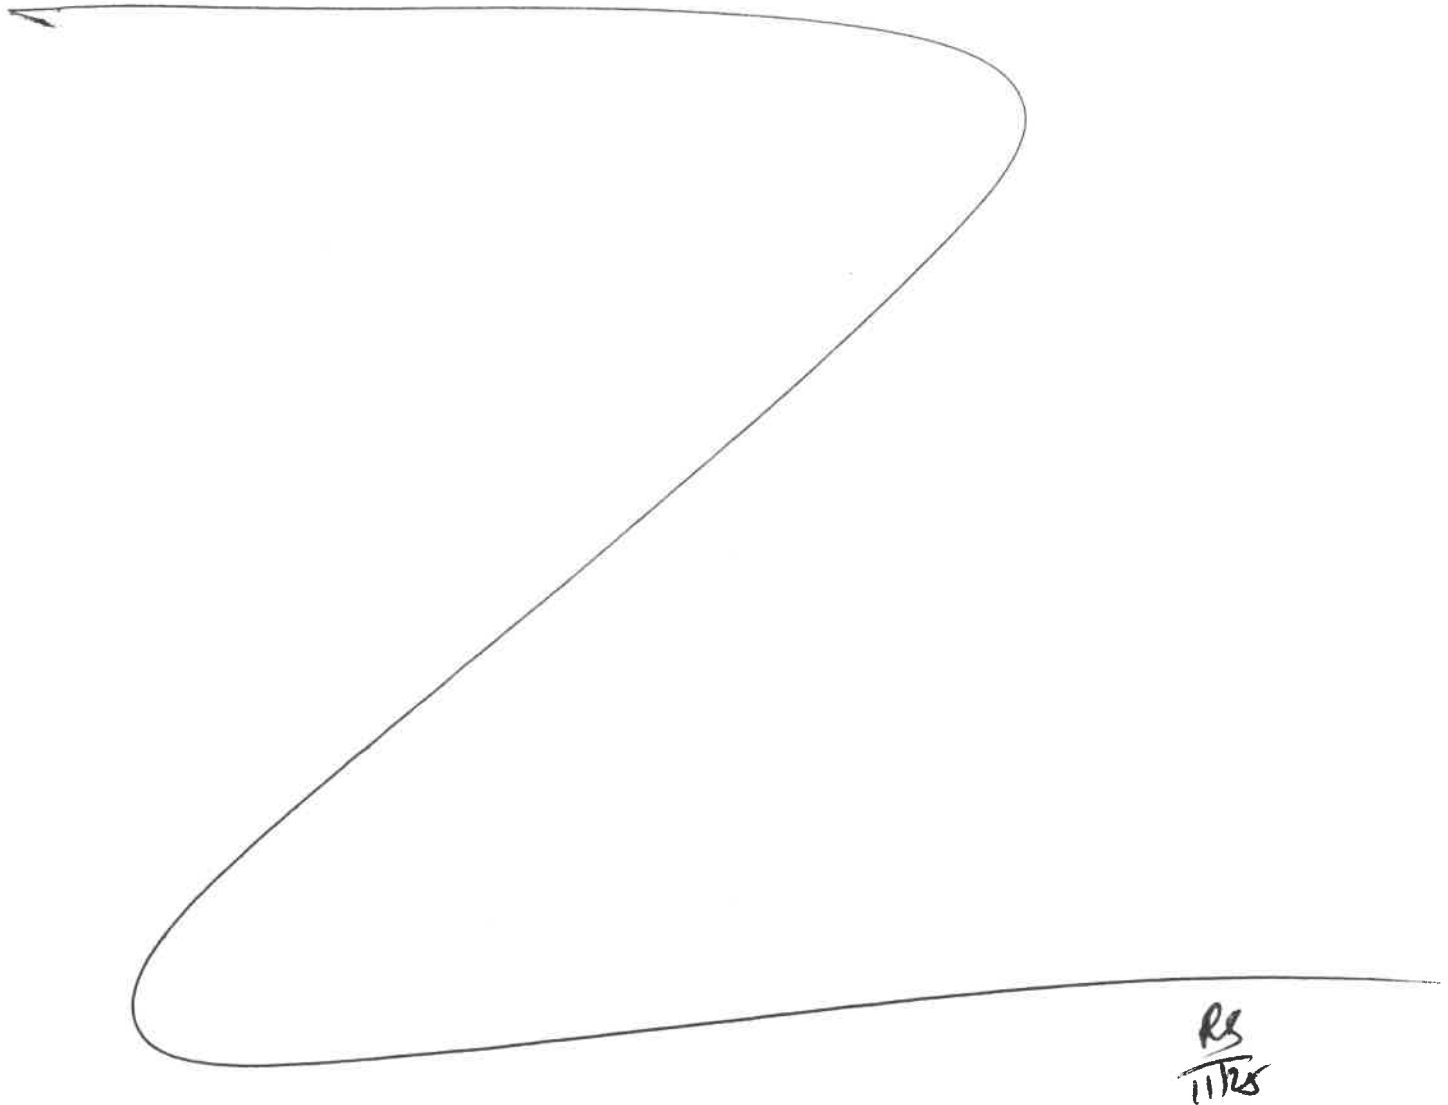

RS
11/25