

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
 Data File : BG064857.D
 Acq On : 25 Nov 2025 12:28
 Operator : RC/JU
 Sample : PB170717BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK717

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG064857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	3	6	14	rVB5	7286	14541	0.92%	0.112%
2	3.205	16	20	26	rVV	26348	38021	2.40%	0.293%
3	3.475	62	66	72	rVB3	9316	13356	0.84%	0.103%
4	3.904	134	139	151	rBV	129008	221362	13.99%	1.709%
5	4.262	197	200	205	rVB4	2779	3748	0.24%	0.029%
6	7.294	708	716	728	rBV	123260	236576	14.95%	1.826%
7	7.370	728	729	734	rVB3	1731	1997	0.13%	0.015%
8	7.464	736	745	754	rBV	93095	165620	10.47%	1.278%
9	7.676	775	781	794	rVV	128907	234893	14.85%	1.813%
10	7.764	794	796	801	rVB3	2051	2351	0.15%	0.018%
11	8.152	853	862	875	rBV	112216	206095	13.03%	1.591%
12	8.845	973	980	988	rBV	155386	286933	18.13%	2.215%
13	9.309	1051	1059	1070	rBV	115450	219711	13.89%	1.696%
14	10.038	1174	1183	1196	rBV2	92983	183121	11.57%	1.414%
15	10.578	1267	1275	1284	rBV	142533	283382	17.91%	2.187%
16	10.966	1331	1341	1353	rBV	152774	293582	18.55%	2.266%
17	11.090	1355	1362	1376	rVV	128923	278712	17.61%	2.151%
18	12.553	1606	1611	1617	rVB2	2065	3918	0.25%	0.030%
19	14.162	1878	1885	1894	rBV	340909	539200	34.08%	4.162%
20	14.462	1929	1936	1947	rBV	396267	650643	41.12%	5.022%
21	14.768	1977	1988	2002	rBV	310702	501251	31.68%	3.869%
22	14.938	2010	2017	2029	rBV	85794	194381	12.28%	1.500%
23	15.079	2039	2041	2045	rVV4	1551	2393	0.15%	0.018%
24	15.114	2045	2047	2050	rVB2	2156	2242	0.14%	0.017%
25	15.749	2147	2155	2167	rBV	539527	883353	55.83%	6.819%
26	15.849	2167	2172	2188	rVV	121095	217197	13.73%	1.677%
27	15.954	2188	2190	2192	rVV2	2245	2540	0.16%	0.020%
28	15.990	2192	2196	2201	rVB4	3047	4937	0.31%	0.038%
29	17.288	2415	2417	2421	rVB3	1995	1612	0.10%	0.012%
30	17.494	2444	2452	2462	rBV2	450339	713060	45.07%	5.504%
31	17.594	2462	2469	2485	rVB	656136	1092249	69.03%	8.431%
32	17.882	2513	2518	2522	rVB4	1242	2197	0.14%	0.017%
33	18.140	2560	2562	2565	rBV2	1568	1623	0.10%	0.013%
34	18.446	2611	2614	2618	rVB3	1563	2313	0.15%	0.018%
35	18.845	2680	2682	2688	rVV3	1923	3395	0.21%	0.026%
36	19.262	2749	2753	2761	rBV3	3400	7972	0.50%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
 Data File : BG064857.D
 Acq On : 25 Nov 2025 12:28
 Operator : RC/JU
 Sample : PB170717BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK717

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
 Title : SVOA CALIBRATION

37	19.433	2778	2782	2789	rVB4	11994	18345	1.16%	0.142%
38	19.503	2789	2794	2798	rBV2	9689	15053	0.95%	0.116%
39	19.538	2798	2800	2805	rVB4	1546	2261	0.14%	0.017%
40	19.774	2837	2840	2844	rVB5	3988	5374	0.34%	0.041%
41	19.862	2849	2855	2869	rBV	962594	1490117	94.18%	11.502%
42	20.161	2905	2906	2908	rBV	2784	2386	0.15%	0.018%
43	20.808	3014	3016	3018	rVB3	3254	2197	0.14%	0.017%
44	21.178	3077	3079	3081	rBV2	2817	1933	0.12%	0.015%
45	21.295	3096	3099	3100	rBV2	3383	3385	0.21%	0.026%
46	21.742	3168	3175	3189	rBV	539122	1009224	63.78%	7.790%
47	22.188	3249	3251	3252	rBV2	3189	1650	0.10%	0.013%
48	22.541	3308	3311	3316	rVB6	15102	22434	1.42%	0.173%
49	23.240	3428	3430	3431	rBV2	4483	3068	0.19%	0.024%
50	23.434	3459	3463	3471	rVB8	18660	42702	2.70%	0.330%
51	24.274	3604	3606	3607	rVB2	4220	2330	0.15%	0.018%
52	24.409	3627	3629	3630	rBV2	3608	2756	0.17%	0.021%
53	24.515	3642	3647	3657	rVB8	21351	53855	3.40%	0.416%
54	24.774	3680	3691	3707	rBV	531193	1582271	100.00%	12.214%
55	24.997	3717	3729	3743	rBV	366200	1091704	69.00%	8.427%
56	26.184	3921	3931	3938	rBV8	14365	49018	3.10%	0.378%
57	29.556	4497	4505	4506	rBV8	12988	24567	1.55%	0.190%
58	30.896	4731	4733	4735	rBV3	3608	3087	0.20%	0.024%
59	31.225	4787	4789	4790	rBV2	4833	3879	0.25%	0.030%
60	31.366	4811	4813	4814	rBV2	3691	2385	0.15%	0.018%
61	31.536	4841	4842	4844	rBV2	5423	4589	0.29%	0.035%
62	31.947	4911	4912	4917	rVB3	5955	3707	0.23%	0.029%




Sum of corrected areas: 12954754

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
Data File : BG064857.D
Acq On : 25 Nov 2025 12:28
Operator : RC/JU
Sample : PB170717BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK717

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

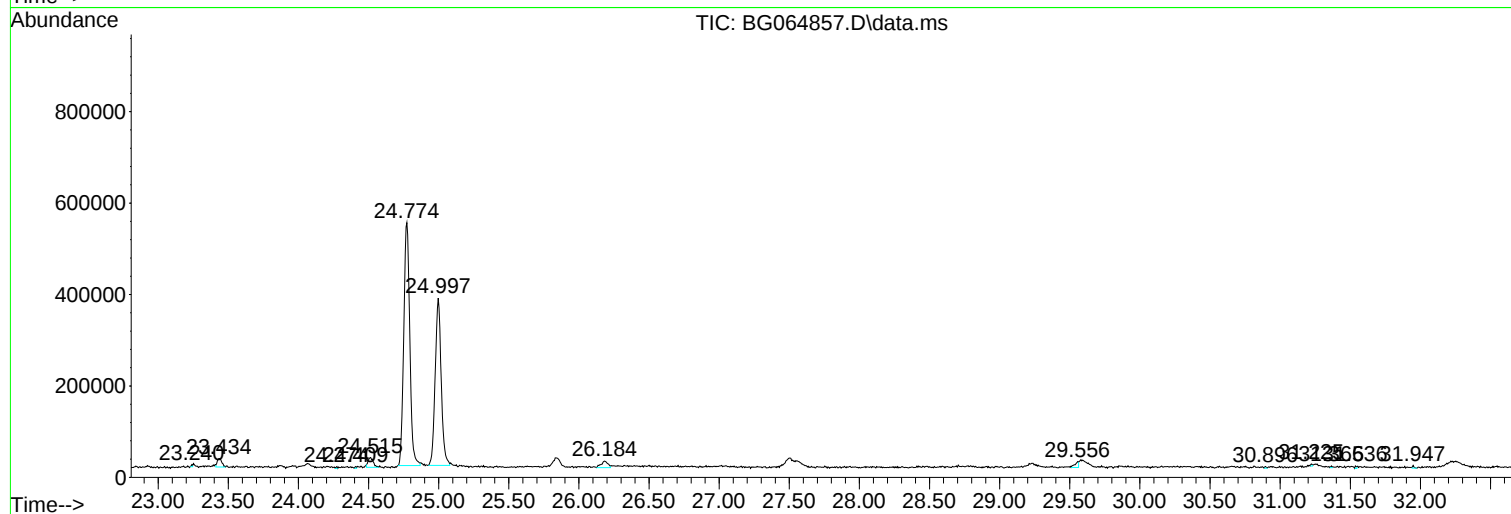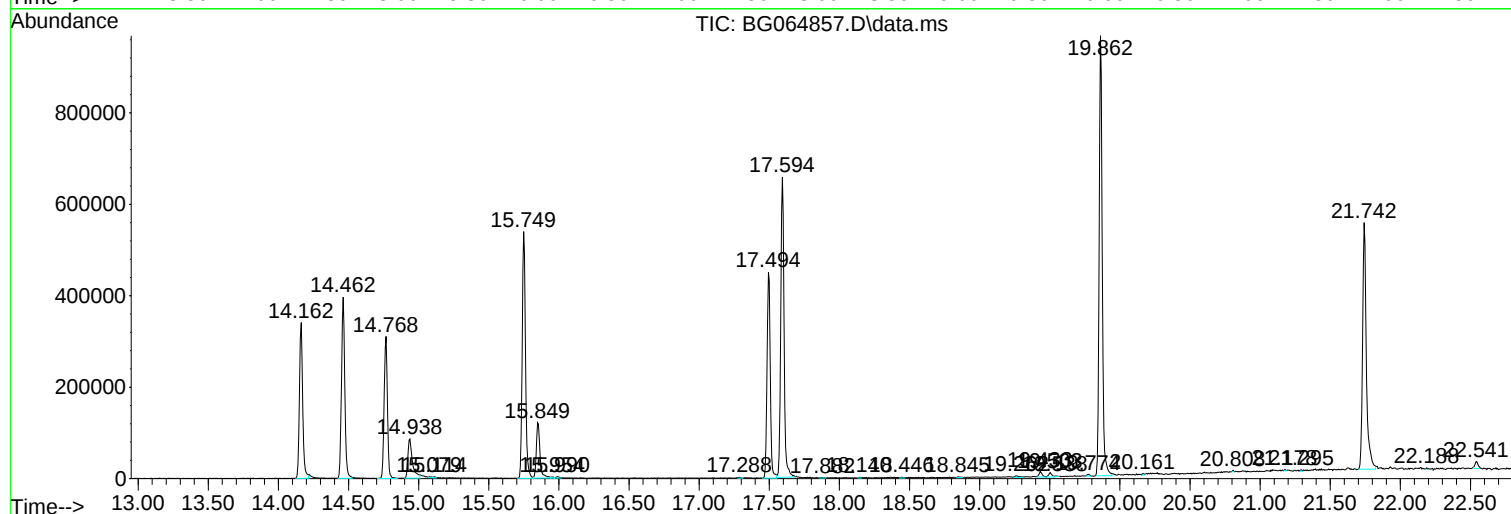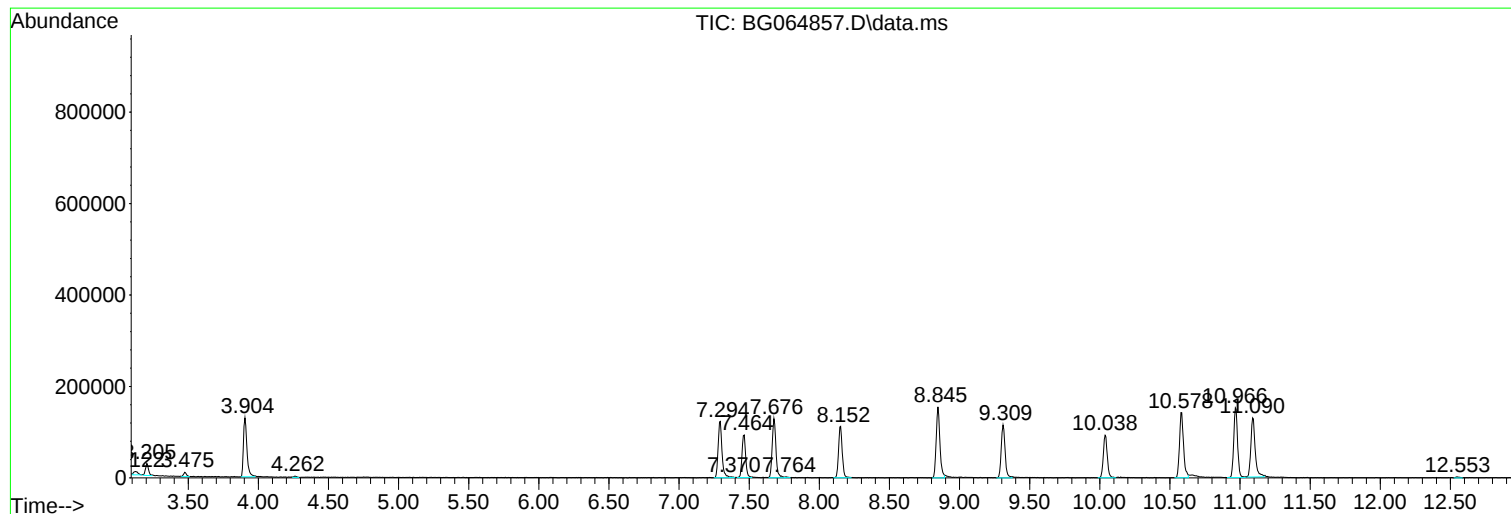

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
Data File : BG064857.D
Acq On : 25 Nov 2025 12:28
Operator : RC/JU
Sample : PB170717BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK717

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112525\
Data File : BG064857.D
Acq On : 25 Nov 2025 12:28
Operator : RC/JU
Sample : PB170717BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK717

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
