


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111725\
Data File : VU063719.D
Acq On : 17 Nov 2025 10:37
Operator : MD/SY
Sample : BFB090
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB090

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Title : VOC Analysis
Last Update : Wed Nov 19 04:47:02 2025

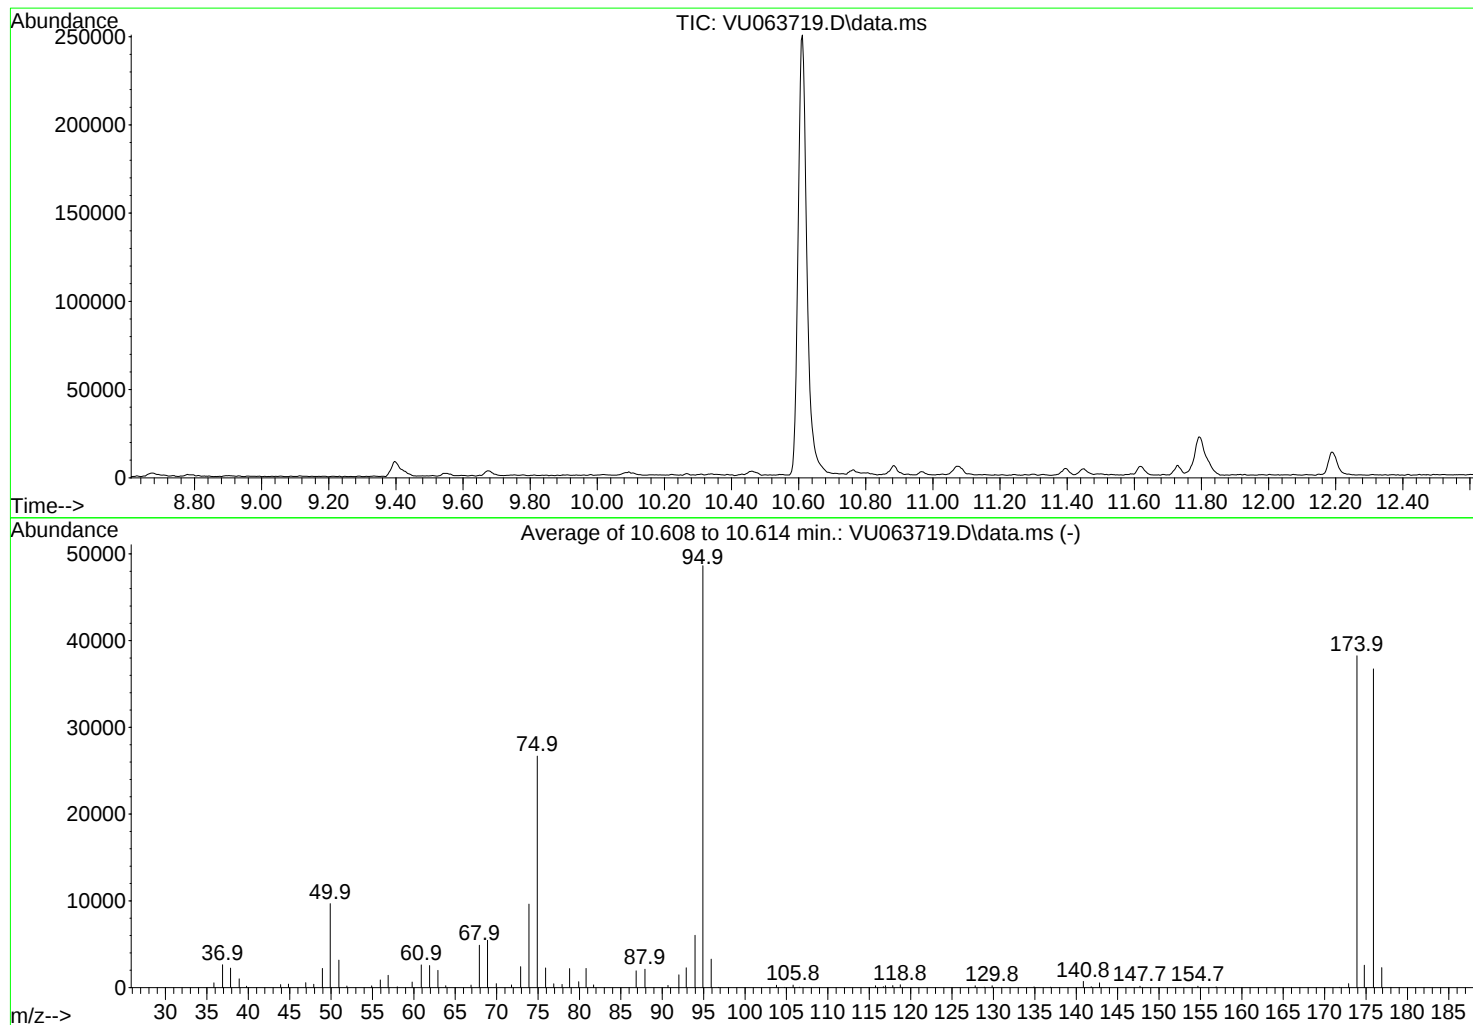

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2886

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	9684	PASS
75	95	30	80	54.9	26696	PASS
95	95	100	100	100.0	48637	PASS
96	95	5	9	6.7	3278	PASS
173	174	0.00	2	1.2	446	PASS
174	95	50	120	78.7	38264	PASS
175	174	5	9	6.7	2566	PASS
176	174	95	101	96.0	36739	PASS
177	176	5	9	6.3	2306	PASS

m/z	Abundance
35.80	589.0
37.70	228.0
39.80	209.0
43.90	546.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090

m/z	Abundance
35.90	1114.0
36.90	2921.0
37.90	2644.0
38.90	1052.0
39.80	363.0
43.90	905.0
44.90	409.0
47.00	580.0
47.90	359.0
48.90	2203.0
49.90	10067.0
51.00	3250.0
52.00	184.0
54.90	196.0
56.00	953.0
56.90	1494.0
59.80	696.0
60.90	2844.0
61.90	2609.0
62.90	2116.0
63.80	207.0
66.90	256.0
67.90	4743.0
68.90	5643.0
70.00	494.0
71.80	362.0
72.90	2574.0
73.90	9598.0
74.90	27944.0
75.90	2358.0
76.90	425.0
77.90	312.0
78.80	2250.0
79.90	745.0
80.80	2163.0
81.70	342.0
86.80	1944.0
87.90	2095.0
90.70	218.0
92.00	1430.0
92.90	2279.0
94.00	6062.0
94.90	49472.0
95.90	3335.0
96.80	100.0
103.80	277.0
104.80	102.0
105.80	280.0
106.60	125.0
115.80	217.0
117.00	312.0
117.80	240.0
118.80	304.0
127.80	207.0
129.90	219.0
134.90	144.0
140.80	670.0
141.90	117.0
142.80	490.0
147.70	174.0
154.70	135.0
156.90	131.0
172.90	457.0
173.90	37576.0
174.80	2589.0
175.90	36272.0
176.90	2510.0
178.00	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090

m/z	Abundance
35.90	1191.0
36.90	2655.0
37.90	2546.0
38.90	1041.0
39.80	376.0
43.90	904.0
44.90	409.0
47.00	590.0
47.90	396.0
48.90	2265.0
49.90	9898.0
50.90	3229.0
51.90	196.0
54.90	201.0
56.00	890.0
56.90	1460.0
58.00	112.0
59.80	649.0
60.90	2686.0
61.90	2611.0
62.90	2020.0
63.80	217.0
66.90	315.0
67.90	4967.0
68.90	5529.0
69.90	461.0
71.80	293.0
72.90	2499.0
73.90	9977.0
74.90	27448.0
75.90	2347.0
76.90	460.0
77.90	389.0
78.80	2281.0
79.90	686.0
80.80	2274.0
81.70	312.0
86.90	1951.0
87.90	2173.0
90.70	269.0
92.00	1562.0
92.90	2364.0
94.00	6148.0
94.90	49832.0
95.90	3334.0
103.80	274.0
105.80	303.0
115.70	228.0
116.90	312.0
117.80	247.0
118.80	329.0
127.80	223.0
129.80	224.0
134.90	134.0
140.80	747.0
141.80	109.0
142.80	568.0
147.70	154.0
154.70	164.0
156.90	107.0
171.80	100.0
172.90	444.0
173.90	39288.0
174.80	2618.0
175.90	37648.0
176.90	2325.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090

m/z	Abundance
35.90	1109.0
36.90	2301.0
37.90	2245.0
38.90	932.0
39.80	339.0
43.90	859.0
44.80	374.0
46.90	550.0
47.90	365.0
49.00	2171.0
49.90	9088.0
50.90	3038.0
51.80	171.0
54.90	198.0
55.90	791.0
56.90	1301.0
58.00	155.0
59.80	543.0
60.90	2322.0
61.90	2389.0
62.90	1825.0
63.90	201.0
66.90	267.0
67.90	4921.0
68.90	5184.0
69.90	395.0
71.80	282.0
72.90	2160.0
73.90	9308.0
74.90	24696.0
75.90	2101.0
76.90	423.0
77.90	399.0
78.80	2053.0
79.90	578.0
80.80	2186.0
81.70	283.0
86.90	1889.0
87.90	2084.0
90.70	249.0
92.00	1437.0
92.90	2200.0
93.90	5888.0
94.90	46608.0
95.90	3165.0
103.80	230.0
105.80	280.0
115.80	213.0
116.70	331.0
117.90	209.0
118.70	338.0
127.80	207.0
128.90	123.0
129.80	196.0
136.90	121.0
140.90	734.0
141.70	105.0
142.80	580.0
147.70	127.0
154.70	155.0
172.90	437.0
173.90	37928.0
174.80	2491.0
175.90	36296.0
176.90	2084.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090