
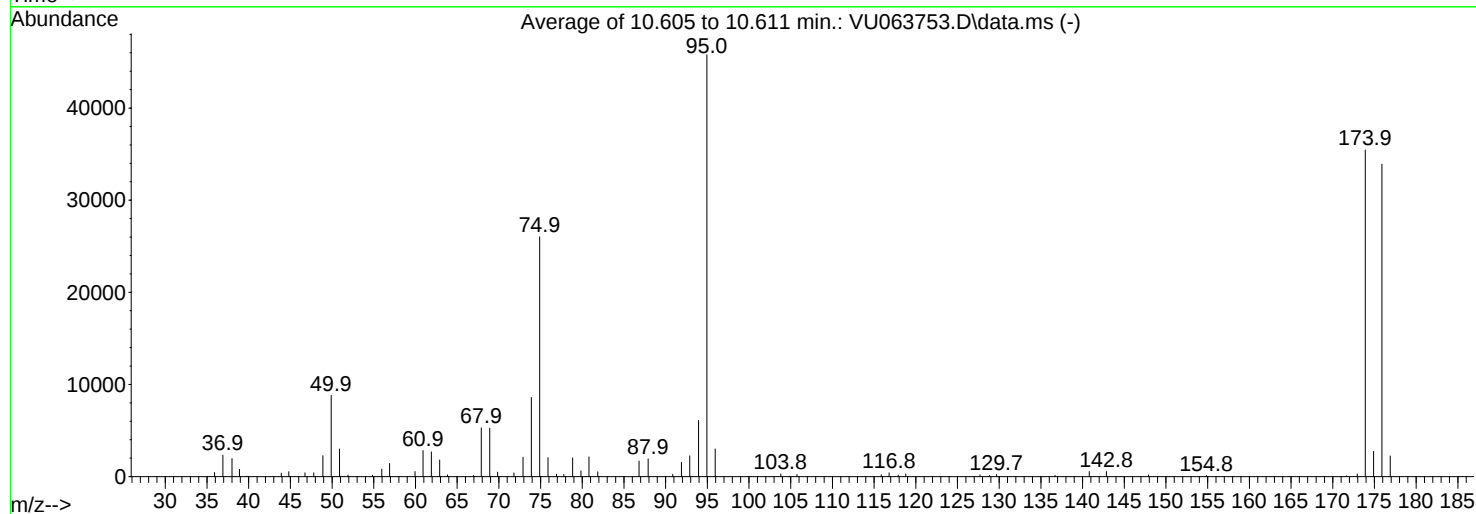


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063753.D
Acq On : 21 Nov 2025 07:50
Operator : MD/SY
Sample : BFB092
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB092

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Title : VOC Analysis
Last Update : Tue Nov 25 00:22:49 2025

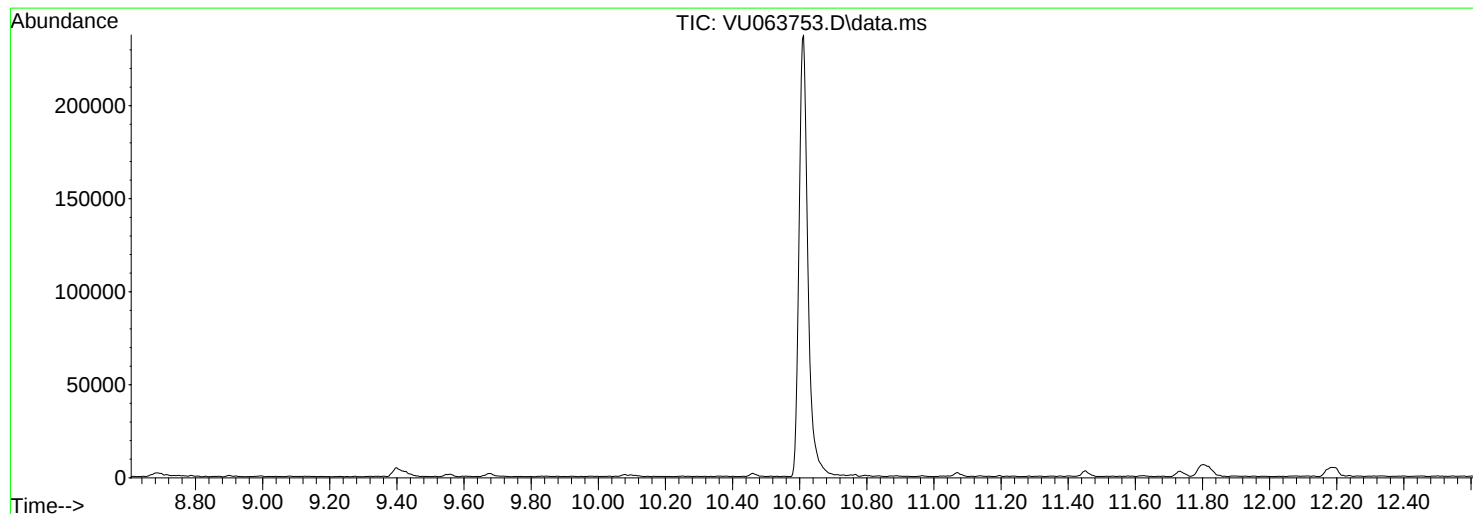

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2886

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	8811	PASS
75	95	30	80	56.9	26032	PASS
95	95	100	100	100.0	45787	PASS
96	95	5	9	6.5	2989	PASS
173	174	0.00	2	0.8	284	PASS
174	95	50	120	77.4	35459	PASS
175	174	5	9	7.7	2732	PASS
176	174	95	101	95.7	33917	PASS
177	176	5	9	6.6	2240	PASS

Scan 2886 (10.570 min): VU063753.D\data.ms
BFB092

m/z	Abundance
39.80	168.0
43.90	526.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
35.90	453.0
36.90	2192.0
38.00	1903.0
38.90	803.0
39.80	242.0
43.90	873.0
44.80	534.0
46.70	316.0
47.80	378.0
48.90	2155.0
49.90	8332.0
50.90	2869.0
51.90	188.0
54.80	131.0
55.90	792.0
56.90	1296.0
59.90	460.0
60.90	2749.0
61.90	2629.0
62.90	1597.0
63.80	199.0
67.00	128.0
67.90	4787.0
68.90	5055.0
69.80	448.0
71.80	362.0
72.90	2054.0
73.90	8165.0
74.90	24720.0
75.90	1951.0
76.90	246.0
77.80	147.0
78.90	1947.0
79.90	645.0
80.80	2000.0
81.80	475.0
86.80	1582.0
87.90	1815.0
90.80	230.0
91.90	1423.0
92.90	2132.0
94.00	5466.0
95.00	43160.0
96.00	2825.0
103.80	318.0
105.70	203.0
115.80	205.0
116.80	375.0
117.90	161.0
118.80	249.0
127.70	181.0
128.80	109.0
129.70	245.0
136.70	118.0
140.80	594.0
142.80	498.0
147.80	126.0
154.80	100.0
171.60	110.0
172.90	260.0
173.90	33088.0
174.90	2495.0
175.90	30760.0
176.90	2235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
35.90	461.0
36.90	2371.0
38.00	1990.0
38.90	753.0
39.80	205.0
43.90	927.0
44.80	566.0
46.80	407.0
47.80	403.0
48.90	2330.0
49.90	8954.0
50.90	3179.0
51.90	161.0
54.80	160.0
56.00	828.0
56.90	1421.0
60.00	584.0
60.90	2873.0
61.90	2781.0
62.90	1824.0
63.80	183.0
67.00	101.0
67.90	5385.0
68.90	5316.0
69.90	495.0
71.80	413.0
72.90	2145.0
73.90	8827.0
74.90	26816.0
75.90	2120.0
76.90	270.0
77.80	257.0
78.90	2055.0
79.90	658.0
80.80	2229.0
81.80	521.0
86.80	1680.0
87.90	1992.0
90.80	246.0
91.90	1574.0
92.90	2314.0
93.90	6266.0
95.00	47240.0
95.90	3065.0
103.80	297.0
105.80	233.0
115.90	218.0
116.80	429.0
117.90	171.0
118.80	242.0
127.70	211.0
128.90	119.0
129.70	249.0
136.70	136.0
140.80	568.0
142.90	561.0
147.90	184.0
154.90	121.0
171.70	120.0
172.90	273.0
173.90	36160.0
174.90	2732.0
175.90	34792.0
176.90	2311.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
35.90	446.0
36.90	2391.0
38.00	1983.0
38.90	752.0
39.80	168.0
43.90	882.0
44.80	481.0
46.80	491.0
47.80	431.0
48.90	2294.0
49.90	9147.0
50.90	2948.0
51.90	139.0
54.90	166.0
56.00	821.0
56.90	1513.0
60.00	605.0
60.90	2858.0
61.90	2638.0
62.90	1967.0
63.90	187.0
66.90	102.0
67.90	5688.0
68.90	5401.0
69.90	466.0
71.80	394.0
72.90	2097.0
73.90	8799.0
74.90	26560.0
75.90	2106.0
76.90	239.0
77.80	280.0
78.80	2056.0
79.80	571.0
80.80	2147.0
81.90	534.0
86.80	1774.0
87.90	1941.0
90.90	266.0
91.90	1641.0
92.90	2330.0
93.90	6513.0
94.90	46960.0
95.90	3076.0
103.80	247.0
104.80	106.0
105.80	256.0
115.90	180.0
116.80	428.0
117.90	193.0
118.70	189.0
118.90	190.0
127.70	224.0
128.90	119.0
129.70	201.0
136.70	156.0
140.80	494.0
142.90	600.0
148.00	231.0
154.90	141.0
173.00	318.0
173.90	37128.0
174.90	2970.0
175.90	36200.0
176.90	2173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092