

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063776.D
 Acq On : 24 Nov 2025 14:33
 Operator : MD/SY
 Sample : VU1124WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK132

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M

Title : VOC Analysis

Signal : TIC: VU063776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.583	84	91	102	rBV	183402	201437	15.30%	2.009%
2	1.895	179	188	200	rBV	139942	182532	13.86%	1.820%
3	2.541	377	389	409	rBV	280532	461259	35.03%	4.600%
4	2.760	453	457	458	rBV2	1006	668	0.05%	0.007%
5	2.878	491	494	497	rBV3	467	269	0.02%	0.003%
6	2.901	498	501	509	rBV	355	382	0.03%	0.004%
7	3.010	528	535	536	rBV2	2503	1975	0.15%	0.020%
8	3.075	553	555	559	rVB2	442	280	0.02%	0.003%
9	3.113	565	567	571	rBV	313	251	0.02%	0.003%
10	3.152	571	579	583	rBV2	1425	2016	0.15%	0.020%
11	3.329	628	634	636	rBV3	1129	1167	0.09%	0.012%
12	3.486	680	683	686	rBV2	329	247	0.02%	0.002%
13	3.695	744	748	754	rVB2	242	296	0.02%	0.003%
14	3.734	754	760	765	rBV2	242	346	0.03%	0.003%
15	4.042	852	856	863	rVB2	294	374	0.03%	0.004%
16	4.595	1019	1028	1056	rBV	87697	243556	18.50%	2.429%
17	5.030	1145	1163	1199	rBV	227142	533138	40.49%	5.317%
18	5.351	1258	1263	1264	rBV2	637	500	0.04%	0.005%
19	5.396	1273	1277	1283	rBV3	451	474	0.04%	0.005%
20	5.489	1303	1306	1309	rBV2	311	259	0.02%	0.003%
21	5.695	1350	1370	1409	rBV2	443402	1316716	100.00%	13.132%
22	5.956	1448	1451	1454	rVB3	1038	690	0.05%	0.007%
23	5.975	1454	1457	1460	rVB2	336	271	0.02%	0.003%
24	6.001	1462	1465	1468	rBV2	314	257	0.02%	0.003%
25	6.222	1521	1534	1570	rBV	370835	778883	59.15%	7.768%
26	6.512	1614	1624	1635	rBV6	5953	11808	0.90%	0.118%
27	6.660	1657	1670	1705	rBV	278556	587908	44.65%	5.863%
28	7.004	1772	1777	1784	rVV2	289	367	0.03%	0.004%
29	7.081	1799	1801	1805	rVB	370	250	0.02%	0.002%
30	7.171	1823	1829	1830	rBV	260	242	0.02%	0.002%
31	7.200	1834	1838	1843	rVV2	506	533	0.04%	0.005%
32	7.274	1859	1861	1866	rVV2	385	322	0.02%	0.003%
33	7.541	1932	1944	1967	rBV	135013	254293	19.31%	2.536%
34	7.660	1978	1981	1983	rBV2	410	252	0.02%	0.003%
35	7.737	2000	2005	2007	rVB2	588	419	0.03%	0.004%
36	7.769	2011	2015	2016	rBV3	665	432	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063776.D
 Acq On : 24 Nov 2025 14:33
 Operator : MD/SY
 Sample : VU1124WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK132

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.785	2016	2020	2033	rVB7	1276	1894	0.14%	0.019%
38	7.872	2034	2047	2084	rBV	569075	1070932	81.33%	10.680%
39	8.155	2125	2135	2156	rBV2	86076	158417	12.03%	1.580%
40	8.332	2188	2190	2194	rVB3	348	272	0.02%	0.003%
41	8.377	2200	2204	2206	rBV2	600	577	0.04%	0.006%
42	8.402	2210	2212	2216	rVB	412	259	0.02%	0.003%
43	8.531	2242	2252	2264	rVB7	1775	2884	0.22%	0.029%
44	8.615	2264	2278	2319	rBV3	217586	571061	43.37%	5.695%
45	9.139	2436	2441	2443	rBV	407	368	0.03%	0.004%
46	9.283	2479	2486	2490	rBV2	358	416	0.03%	0.004%
47	9.338	2499	2503	2507	rVB	262	237	0.02%	0.002%
48	9.393	2507	2520	2559	rBV	543575	992474	75.37%	9.898%
49	9.550	2564	2569	2578	rVV3	2180	3282	0.25%	0.033%
50	9.586	2578	2580	2583	rVB2	591	260	0.02%	0.003%
51	9.679	2601	2609	2617	rBV3	2086	3418	0.26%	0.034%
52	9.743	2626	2629	2634	rBV	348	362	0.03%	0.004%
53	10.094	2726	2738	2742	rBV7	2006	4027	0.31%	0.040%
54	10.164	2755	2760	2762	rBV2	344	275	0.02%	0.003%
55	10.222	2774	2778	2781	rVB2	358	233	0.02%	0.002%
56	10.290	2796	2799	2802	rVB	450	281	0.02%	0.003%
57	10.463	2844	2853	2863	rVB4	2005	3177	0.24%	0.032%
58	10.598	2887	2895	2897	rBV2	296	311	0.02%	0.003%
59	10.730	2923	2936	2956	rBV	391115	654573	49.71%	6.528%
60	10.843	2966	2971	2976	rVB3	406	466	0.04%	0.005%
61	10.875	2979	2981	2984	rVV2	361	233	0.02%	0.002%
62	10.904	2987	2990	2993	rVB2	318	243	0.02%	0.002%
63	10.930	2993	2998	3002	rVB2	254	258	0.02%	0.003%
64	10.952	3002	3005	3009	rBV2	290	269	0.02%	0.003%
65	11.013	3018	3024	3026	rBV	236	256	0.02%	0.003%
66	11.065	3034	3040	3041	rBV2	1800	1492	0.11%	0.015%
67	11.248	3089	3097	3101	rBV2	256	353	0.03%	0.004%
68	11.367	3130	3134	3138	rBV	266	315	0.02%	0.003%
69	11.451	3153	3160	3173	rVB3	3080	4510	0.34%	0.045%
70	11.727	3238	3246	3253	rBV3	4429	6713	0.51%	0.067%
71	11.788	3253	3265	3291	rVV	554039	955193	72.54%	9.526%
72	11.959	3316	3318	3323	rVB4	463	363	0.03%	0.004%
73	12.168	3370	3383	3408	rBV	545750	936641	71.13%	9.341%
74	12.393	3450	3453	3456	rBV2	542	413	0.03%	0.004%
75	12.422	3460	3462	3469	rVB2	488	470	0.04%	0.005%
76	12.454	3469	3472	3477	rBV2	338	306	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063776.D
 Acq On : 24 Nov 2025 14:33
 Operator : MD/SY
 Sample : VU1124WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK132

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	12.479	3477	3480	3484	rVB2	400	313	0.02%	0.003%
78	12.508	3484	3489	3493	rBV2	523	491	0.04%	0.005%
79	12.586	3504	3513	3517	rBV2	336	440	0.03%	0.004%
80	12.859	3593	3598	3602	rBV2	358	293	0.02%	0.003%
81	12.888	3602	3607	3611	rVB2	436	453	0.03%	0.005%
82	12.920	3612	3617	3619	rBV2	390	350	0.03%	0.003%
83	12.994	3637	3640	3643	rVV2	566	443	0.03%	0.004%
84	13.055	3656	3659	3665	rVB2	479	447	0.03%	0.004%
85	13.132	3679	3683	3686	rBV3	393	343	0.03%	0.003%
86	13.203	3697	3705	3718	rBV5	4125	7109	0.54%	0.071%
87	13.447	3776	3781	3784	rBV3	538	605	0.05%	0.006%
88	13.743	3870	3873	3877	rBV2	357	313	0.02%	0.003%
89	13.791	3885	3888	3889	rBV2	462	278	0.02%	0.003%
90	13.823	3890	3898	3907	rVB3	7927	11944	0.91%	0.119%
91	14.071	3966	3975	3985	rBV2	12105	21628	1.64%	0.216%
92	14.264	4031	4035	4038	rBV4	521	363	0.03%	0.004%
93	14.309	4038	4049	4058	rBV4	8189	14317	1.09%	0.143%
94	14.373	4066	4069	4074	rVB2	505	386	0.03%	0.004%
95	14.663	4157	4159	4166	rVB3	395	255	0.02%	0.003%
96	14.743	4181	4184	4188	rBV3	527	365	0.03%	0.004%
97	15.193	4322	4324	4329	rVB3	608	337	0.03%	0.003%
98	15.418	4392	4394	4399	rBV4	590	467	0.04%	0.005%
99	15.511	4421	4423	4424	rBV	539	249	0.02%	0.002%
100	15.637	4458	4462	4467	rBV5	1106	1280	0.10%	0.013%




Sum of corrected areas: 10027022

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063776.D
Acq On : 24 Nov 2025 14:33
Operator : MD/SY
Sample : VU1124WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

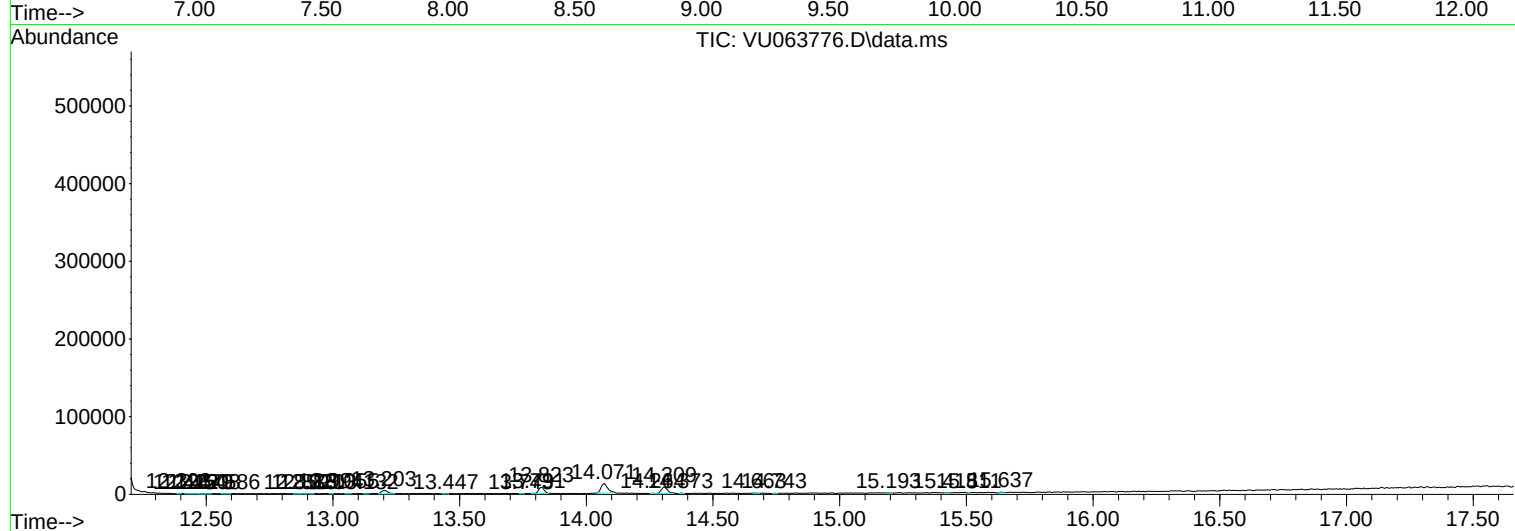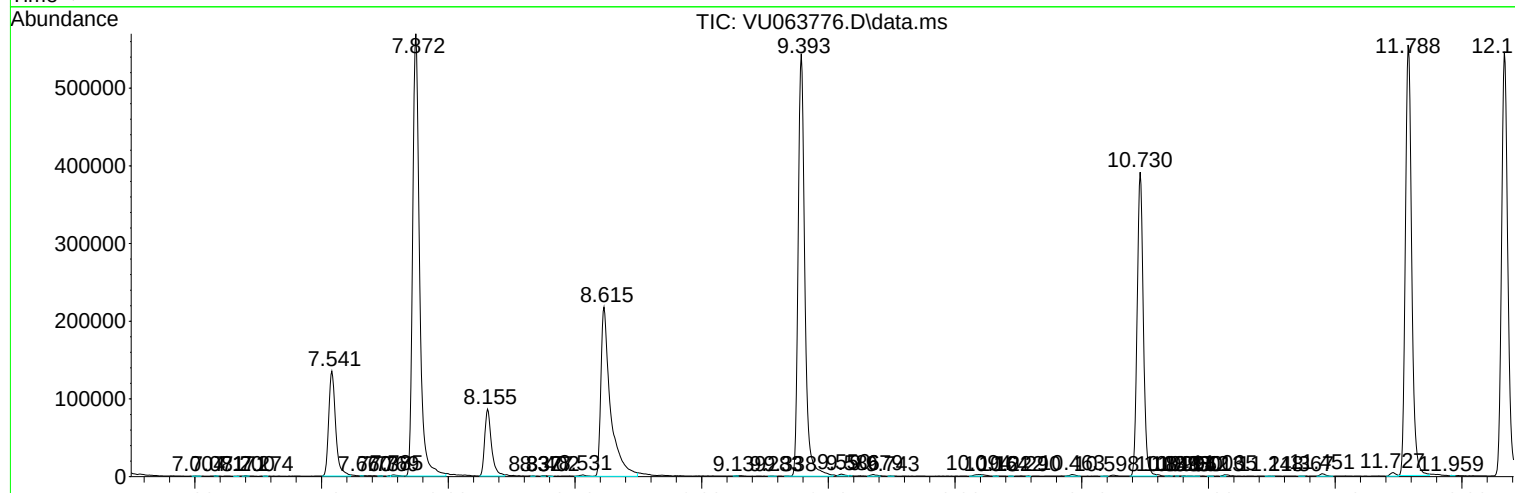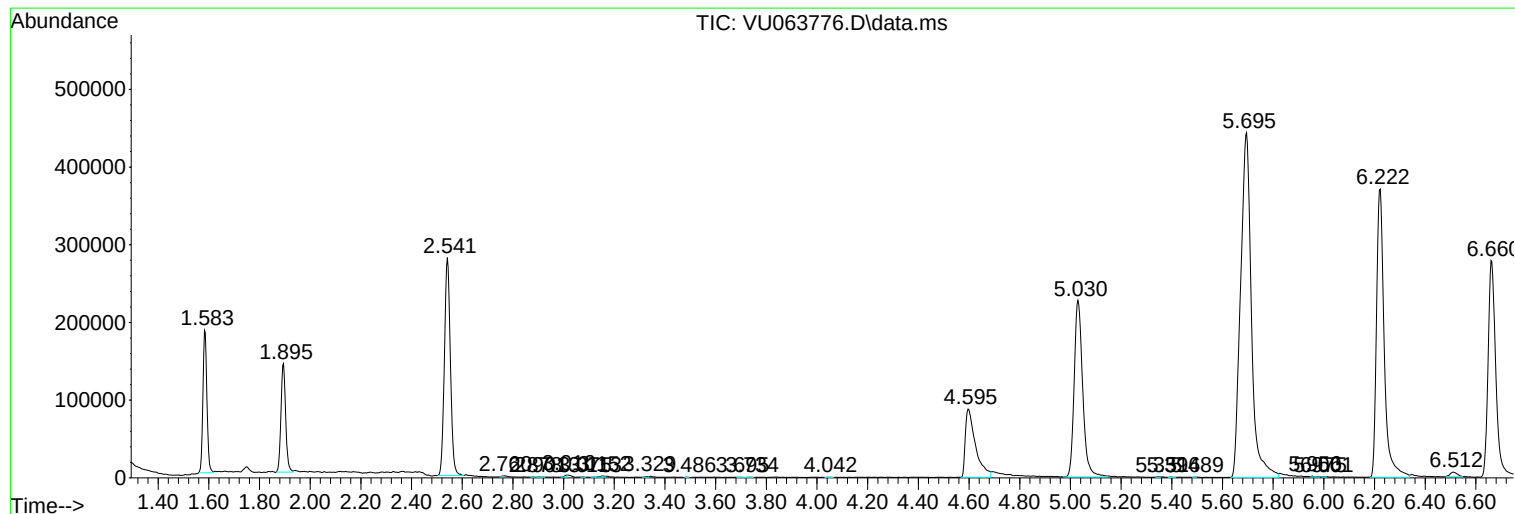

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063776.D
Acq On : 24 Nov 2025 14:33
Operator : MD/SY
Sample : VU1124WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063776.D
Acq On : 24 Nov 2025 14:33
Operator : MD/SY
Sample : VU1124WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
