



Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU112125\  
Data File : VU063757.D  
Acq On : 21 Nov 2025 10:05  
Operator : MD/SY  
Sample : Q3688-04  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
RBGW-20251119

Quant Time: Nov 21 22:29:09 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMULM111725WMA.M  
Quant Title : VOC Analysis  
QLast Update : Fri Nov 21 22:28:08 2025  
Response via : Initial Calibration



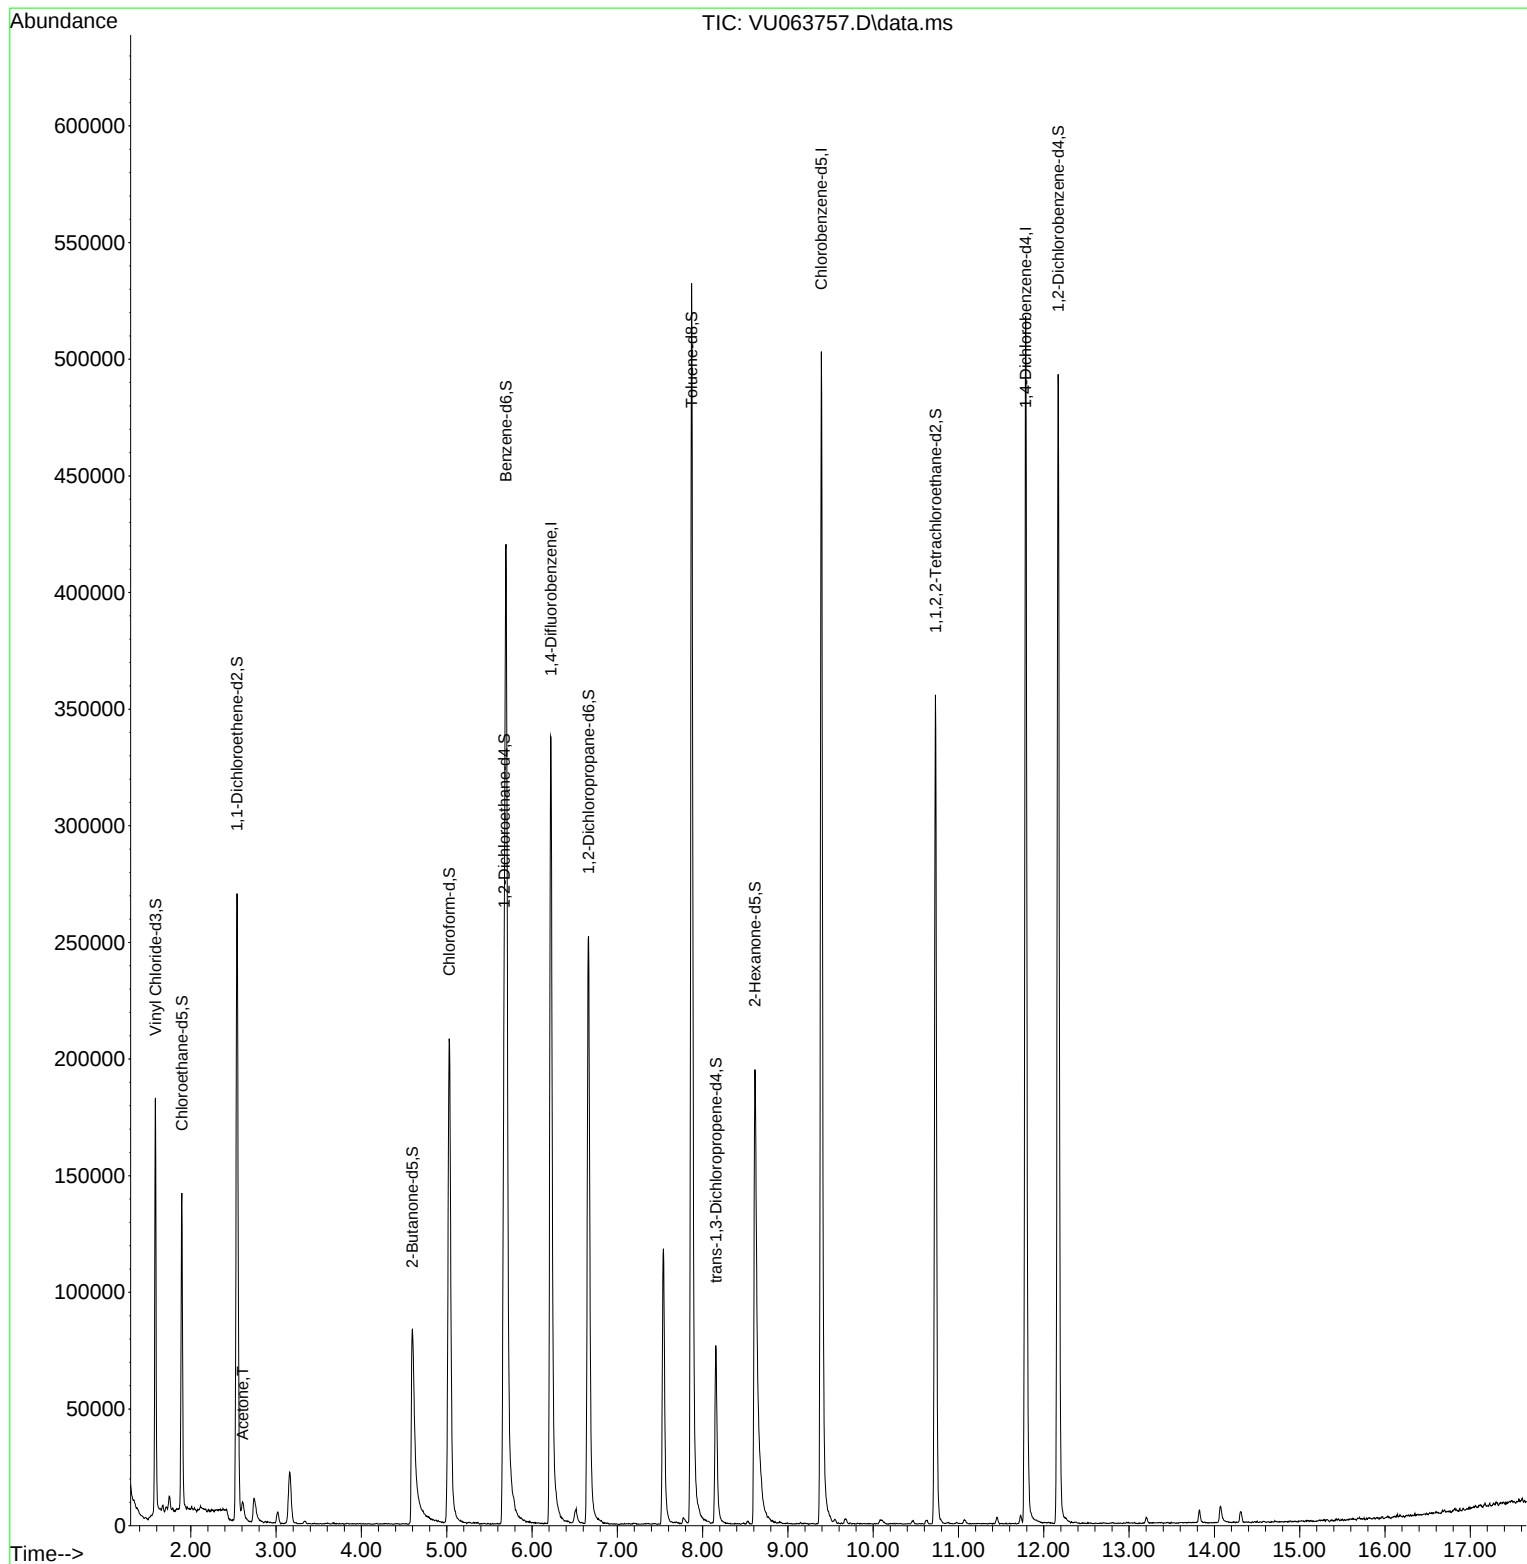


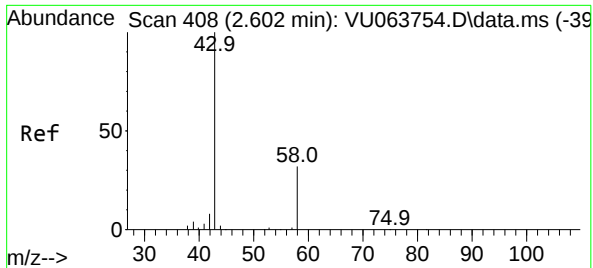

#13  
 Acetone  
 Concen: 4.057 ug/L  
 RT: 2.608 min Scan# 410  
 Delta R.T. 0.006 min  
 Lab File: VU063757.D  
 Acq: 21 Nov 2025 10:05

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 RBGW-20251119

Tgt Ion: 43 Resp: 8175  
 Ion Ratio Lower Upper  
 43 100  
 58 27.9 0.0 63.4

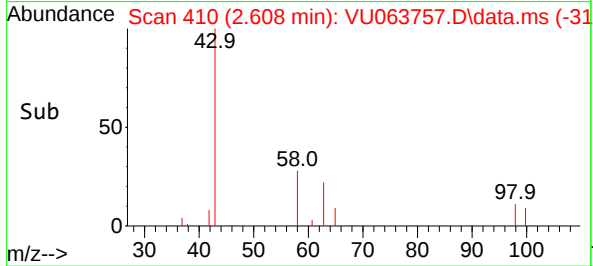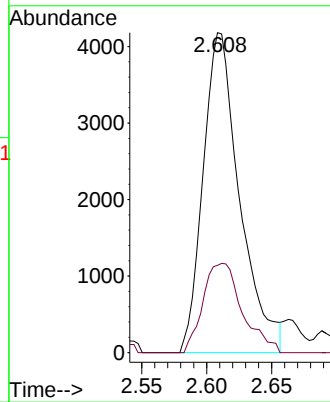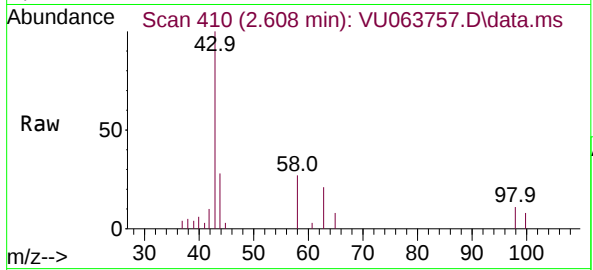

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU112125\  
 Data File : VU063757.D  
 Acq On : 21 Nov 2025 10:05  
 Operator : MD/SY  
 Sample : Q3688-04  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 RBGW-20251119

Quant Time: Nov 21 22:29:09 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMULM111725WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Nov 21 22:28:08 2025  
 Response via : Initial Calibration

| Compound                      | R.T.           | QIon | Response   | Conc     | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|----------|--------|----------|
| -----                         |                |      |            |          |        |          |
| Internal Standards            |                |      |            |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.222          | 114  | 302476     | 50.000   | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 9.393          | 117  | 284569     | 50.000   | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.788         | 152  | 139308     | 50.000   | ug/L   | 0.00     |
|                               |                |      |            |          |        |          |
| System Monitoring Compounds   |                |      |            |          |        |          |
| 4) Vinyl Chloride-d3          | 1.586          | 65   | 118999     | 45.559   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 135 |      | Recovery = | 91.120%  |        |          |
| 7) Chloroethane-d5            | 1.894          | 69   | 94620      | 47.020   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 130 |      | Recovery = | 94.040%  |        |          |
| 11) 1,1-Dichloroethene-d2     | 2.541          | 63   | 166818     | 36.845   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = | 73.680%  |        |          |
| 21) 2-Butanone-d5             | 4.595          | 46   | 133380     | 89.572   | ug/L   | 0.00     |
| Spiked Amount 100.000         | Range 40 - 130 |      | Recovery = | 89.570%  |        |          |
| 24) Chloroform-d              | 5.029          | 84   | 202607     | 46.232   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 92.460%  |        |          |
| 26) 1,2-Dichloroethane-d4     | 5.672          | 65   | 137914     | 47.858   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 95.720%  |        |          |
| 32) Benzene-d6                | 5.695          | 84   | 399098     | 47.846   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 95.700%  |        |          |
| 36) 1,2-Dichloropropane-d6    | 6.663          | 67   | 119896     | 48.963   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 120 |      | Recovery = | 97.920%  |        |          |
| 41) Toluene-d8                | 7.872          | 98   | 375460     | 47.408   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = | 94.820%  |        |          |
| 43) trans-1,3-Dichloroprop... | 8.155          | 79   | 43498      | 42.985   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = | 85.980%  |        |          |
| 47) 2-Hexanone-d5             | 8.614          | 63   | 76272      | 85.668   | ug/L   | 0.00     |
| Spiked Amount 100.000         | Range 45 - 130 |      | Recovery = | 85.670%  |        |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.730         | 84   | 171896     | 48.002   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 65 - 120 |      | Recovery = | 96.000%  |        |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.167         | 152  | 131804     | 50.120   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = | 100.240% |        |          |
|                               |                |      |            |          |        |          |
| Target Compounds              |                |      |            |          | Qvalue |          |
| 13) Acetone                   | 2.608          | 43   | 8175       | 4.057    | ug/L   | 93       |
| -----                         |                |      |            |          |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed