

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063759.D
 Acq On : 21 Nov 2025 10:54
 Operator : MD/SY
 Sample : Q3688-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-32I

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M

Title : VOC Analysis

Signal : TIC: VU063759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.512	64	69	71	rBV4	1358	1399	0.10%	0.013%
2	1.586	84	92	108	rBV	197979	220816	15.86%	2.085%
3	1.895	179	188	201	rBV	152599	195068	14.01%	1.842%
4	2.541	378	389	404	rBV	298121	493679	35.46%	4.661%
5	2.740	442	451	475	rBV	15848	39203	2.82%	0.370%
6	2.978	523	525	529	rBV4	435	281	0.02%	0.003%
7	3.017	529	537	544	rBV4	2517	4073	0.29%	0.038%
8	3.158	564	581	596	rBV	30930	71897	5.16%	0.679%
9	3.313	625	629	630	rBV2	582	274	0.02%	0.003%
10	3.329	632	634	635	rBV2	485	265	0.02%	0.003%
11	3.428	659	665	667	rBV	356	343	0.02%	0.003%
12	3.473	673	679	682	rBV2	379	372	0.03%	0.004%
13	3.544	699	701	705	rBV	354	333	0.02%	0.003%
14	3.666	735	739	747	rBV2	479	575	0.04%	0.005%
15	3.850	793	796	802	rVV2	320	391	0.03%	0.004%
16	3.891	805	809	813	rVB	417	322	0.02%	0.003%
17	3.956	825	829	835	rBV2	298	361	0.03%	0.003%
18	4.107	870	876	880	rBV2	233	302	0.02%	0.003%
19	4.187	895	901	905	rBV	381	454	0.03%	0.004%
20	4.428	972	976	980	rBV2	375	385	0.03%	0.004%
21	4.596	1016	1028	1065	rBV	92127	276937	19.89%	2.615%
22	4.872	1112	1114	1118	rBV4	629	424	0.03%	0.004%
23	5.030	1146	1163	1202	rBV	234133	553424	39.75%	5.225%
24	5.271	1234	1238	1243	rVB5	446	377	0.03%	0.004%
25	5.329	1253	1256	1258	rBV	391	282	0.02%	0.003%
26	5.354	1258	1264	1265	rBV4	350	343	0.02%	0.003%
27	5.432	1284	1288	1295	rVB3	592	725	0.05%	0.007%
28	5.692	1350	1369	1413	rBV2	464976	1392158	100.00%	13.144%
29	6.107	1496	1498	1502	rVB3	487	279	0.02%	0.003%
30	6.155	1509	1513	1517	rBV3	392	295	0.02%	0.003%
31	6.219	1521	1533	1573	rBV	391145	830640	59.67%	7.842%
32	6.512	1614	1624	1637	rBV10	5006	10950	0.79%	0.103%
33	6.660	1657	1670	1702	rBV	283936	600329	43.12%	5.668%
34	7.068	1793	1797	1800	rVB2	366	271	0.02%	0.003%
35	7.190	1828	1835	1837	rVV4	459	458	0.03%	0.004%
36	7.219	1841	1844	1851	rVB3	401	389	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063759.D
 Acq On : 21 Nov 2025 10:54
 Operator : MD/SY
 Sample : Q3688-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-32I

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.541	1930	1944	1967	rBV	135889	257658	18.51%	2.433%
38	7.718	1996	1999	2004	rVB3	566	503	0.04%	0.005%
39	7.785	2012	2020	2024	rBV7	856	1426	0.10%	0.013%
40	7.872	2034	2047	2091	rBV	592377	1140299	81.91%	10.766%
41	8.155	2124	2135	2156	rBV	84484	152843	10.98%	1.443%
42	8.316	2180	2185	2187	rBV2	430	421	0.03%	0.004%
43	8.374	2200	2203	2207	rVB	765	539	0.04%	0.005%
44	8.528	2247	2251	2256	rVB3	1197	1207	0.09%	0.011%
45	8.615	2266	2278	2311	rBV3	217502	571111	41.02%	5.392%
46	8.869	2355	2357	2360	rVB3	479	287	0.02%	0.003%
47	8.904	2365	2368	2372	rVB5	755	555	0.04%	0.005%
48	9.145	2439	2443	2450	rBV3	472	476	0.03%	0.004%
49	9.338	2497	2503	2507	rBV2	274	347	0.02%	0.003%
50	9.393	2507	2520	2560	rBV	579312	1064381	76.46%	10.049%
51	9.544	2565	2567	2569	rBV3	810	399	0.03%	0.004%
52	9.673	2601	2607	2608	rBV3	1215	936	0.07%	0.009%
53	9.737	2623	2627	2633	rBV3	415	412	0.03%	0.004%
54	9.798	2641	2646	2649	rVB	329	295	0.02%	0.003%
55	9.872	2664	2669	2671	rBV2	266	288	0.02%	0.003%
56	9.965	2695	2698	2702	rBV2	263	268	0.02%	0.003%
57	10.010	2707	2712	2717	rVB	239	269	0.02%	0.003%
58	10.074	2728	2732	2734	rBV3	638	522	0.04%	0.005%
59	10.091	2735	2737	2739	rVV3	491	264	0.02%	0.002%
60	10.203	2766	2772	2775	rBV2	272	279	0.02%	0.003%
61	10.232	2775	2781	2783	rVV2	319	370	0.03%	0.003%
62	10.316	2801	2807	2811	rBV2	339	402	0.03%	0.004%
63	10.380	2824	2827	2836	rVB2	427	438	0.03%	0.004%
64	10.460	2845	2852	2864	rVB6	1137	2088	0.15%	0.020%
65	10.547	2876	2879	2882	rVB	418	273	0.02%	0.003%
66	10.573	2882	2887	2890	rBV	310	313	0.02%	0.003%
67	10.621	2896	2902	2912	rVB5	1098	2108	0.15%	0.020%
68	10.660	2912	2914	2920	rBV2	355	347	0.02%	0.003%
69	10.730	2923	2936	2955	rBV	400136	666589	47.88%	6.294%
70	10.972	3008	3011	3016	rBV2	487	361	0.03%	0.003%
71	11.013	3021	3024	3029	rBV2	427	434	0.03%	0.004%
72	11.065	3036	3040	3042	rBV2	904	712	0.05%	0.007%
73	11.242	3089	3095	3099	rBV	293	278	0.02%	0.003%
74	11.283	3105	3108	3111	rBV	350	285	0.02%	0.003%
75	11.451	3152	3160	3163	rBV3	1450	1671	0.12%	0.016%
76	11.730	3237	3247	3252	rBV4	2564	3900	0.28%	0.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063759.D
 Acq On : 21 Nov 2025 10:54
 Operator : MD/SY
 Sample : Q3688-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-32I

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	11.788	3252	3265	3292	rBV	607662	1022167	73.42%	9.651%
78	12.071	3350	3353	3355	rVB3	446	281	0.02%	0.003%
79	12.087	3355	3358	3360	rBV3	429	289	0.02%	0.003%
80	12.168	3370	3383	3406	rBV	576746	968582	69.57%	9.145%
81	12.367	3441	3445	3448	rBV3	425	363	0.03%	0.003%
82	12.406	3453	3457	3460	rVV2	342	313	0.02%	0.003%
83	12.502	3481	3487	3490	rBV2	509	409	0.03%	0.004%
84	12.602	3513	3518	3520	rBV2	320	263	0.02%	0.002%
85	12.753	3559	3565	3568	rVB3	492	450	0.03%	0.004%
86	12.846	3590	3594	3597	rBV2	364	346	0.02%	0.003%
87	13.129	3677	3682	3686	rBV	381	375	0.03%	0.004%
88	13.206	3699	3706	3714	rBV4	1748	2822	0.20%	0.027%
89	13.267	3722	3725	3732	rVB3	325	351	0.03%	0.003%
90	13.405	3764	3768	3772	rBV2	395	360	0.03%	0.003%
91	13.463	3783	3786	3790	rBV	334	328	0.02%	0.003%
92	13.827	3891	3899	3907	rBV6	3591	5510	0.40%	0.052%
93	13.872	3910	3913	3916	rBV	387	343	0.02%	0.003%
94	14.074	3970	3976	3983	rVV2	3105	4350	0.31%	0.041%
95	14.306	4042	4048	4061	rBV6	3523	5769	0.41%	0.054%
96	14.618	4140	4145	4151	rBV3	494	682	0.05%	0.006%
97	14.669	4159	4161	4165	rVB	617	313	0.02%	0.003%
98	14.881	4225	4227	4230	rVB2	628	312	0.02%	0.003%
99	15.190	4321	4323	4329	rBV4	570	492	0.04%	0.005%
100	15.235	4334	4337	4339	rBV	607	476	0.03%	0.004%




Sum of corrected areas: 10591574

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063759.D
Acq On : 21 Nov 2025 10:54
Operator : MD/SY
Sample : Q3688-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-32I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

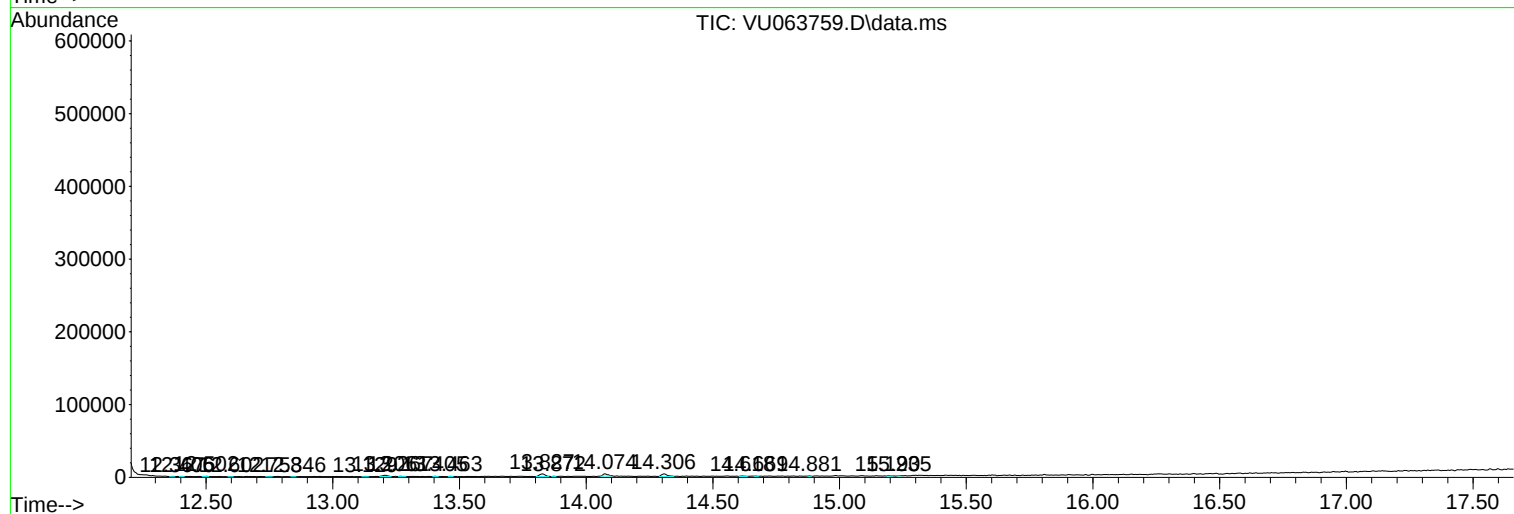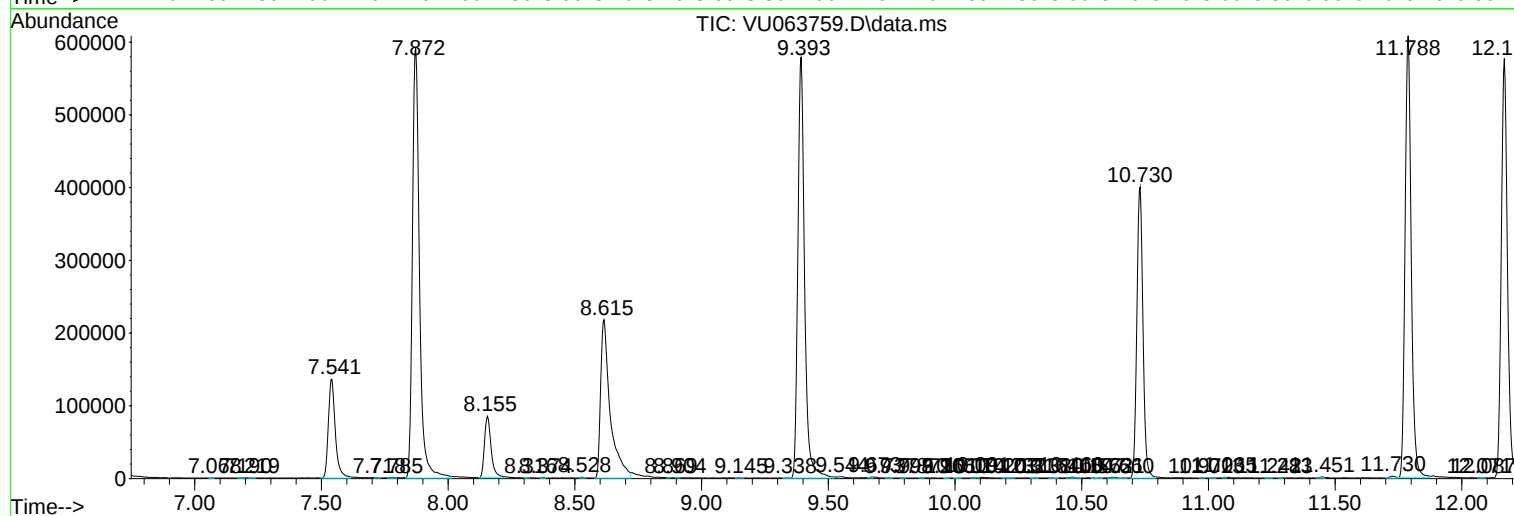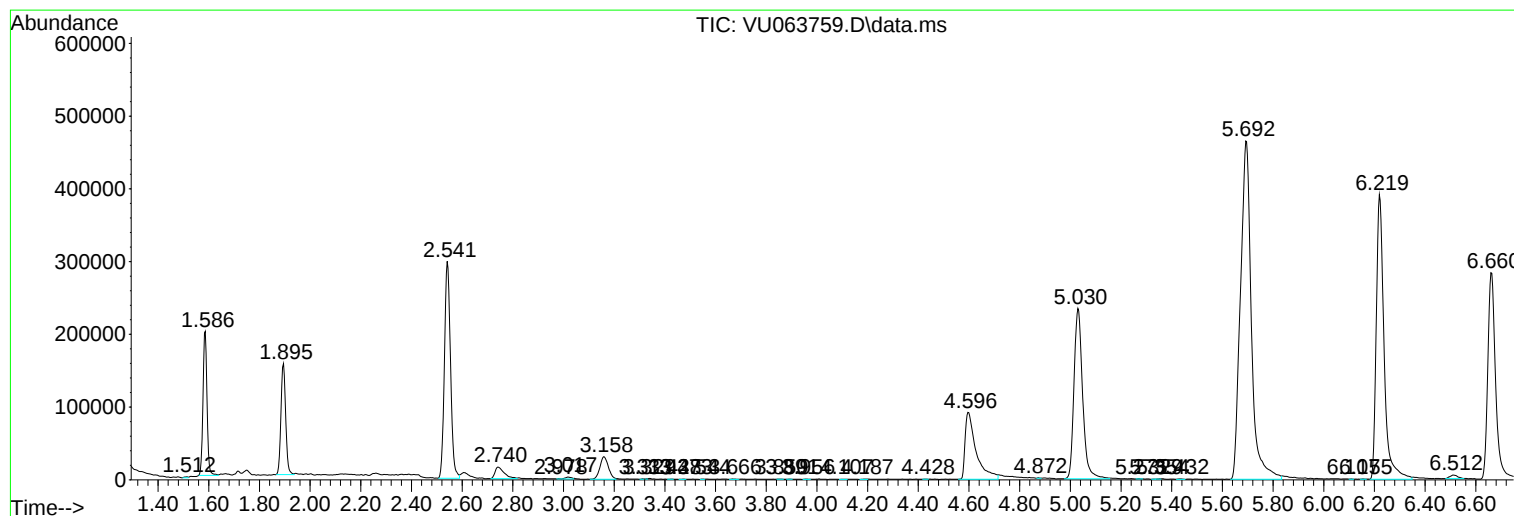

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063759.D
Acq On : 21 Nov 2025 10:54
Operator : MD/SY
Sample : Q3688-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-32I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063759.D
Acq On : 21 Nov 2025 10:54
Operator : MD/SY
Sample : Q3688-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-32I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc