

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063760.D
 Acq On : 21 Nov 2025 11:18
 Operator : MD/SY
 Sample : Q3688-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 RBGW-20251120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M

Title : VOC Analysis

Signal : TIC: VU063760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.583	84	91	106	rBV	199243	220541	15.82%	2.084%
2	1.895	179	188	202	rBV	150898	198249	14.22%	1.874%
3	2.541	376	389	405	rBV	302274	499384	35.82%	4.720%
4	2.747	444	453	469	rBV5	4538	11191	0.80%	0.106%
5	3.017	528	537	547	rBV3	3000	5095	0.37%	0.048%
6	3.158	566	581	607	rBV2	29800	71127	5.10%	0.672%
7	3.342	631	638	641	rBV4	912	1142	0.08%	0.011%
8	3.509	685	690	693	rVB2	342	243	0.02%	0.002%
9	3.602	713	719	725	rVB3	402	412	0.03%	0.004%
10	3.637	725	730	733	rBV	271	241	0.02%	0.002%
11	3.692	741	747	750	rVB2	308	256	0.02%	0.002%
12	3.737	757	761	766	rBV2	239	253	0.02%	0.002%
13	3.843	786	794	798	rBV2	443	656	0.05%	0.006%
14	3.904	810	813	818	rVB	420	359	0.03%	0.003%
15	4.126	878	882	886	rVB2	284	250	0.02%	0.002%
16	4.232	911	915	919	rBV2	299	340	0.02%	0.003%
17	4.319	938	942	947	rVB2	283	272	0.02%	0.003%
18	4.358	947	954	957	rBV2	285	293	0.02%	0.003%
19	4.390	961	964	970	rVB2	423	468	0.03%	0.004%
20	4.425	970	975	979	rBV	315	309	0.02%	0.003%
21	4.599	1016	1029	1060	rBV	95041	276609	19.84%	2.614%
22	5.030	1148	1163	1196	rBV	239574	553886	39.73%	5.235%
23	5.341	1256	1260	1263	rBV2	628	435	0.03%	0.004%
24	5.361	1263	1266	1269	rVB2	594	411	0.03%	0.004%
25	5.412	1279	1282	1286	rVB2	547	453	0.03%	0.004%
26	5.444	1286	1292	1295	rBV3	489	482	0.03%	0.005%
27	5.624	1341	1348	1350	rBV2	341	317	0.02%	0.003%
28	5.692	1350	1369	1412	rBV2	477121	1394111	100.00%	13.175%
29	6.219	1521	1533	1574	rBV	391575	817367	58.63%	7.725%
30	6.509	1613	1623	1632	rBV6	6565	12506	0.90%	0.118%
31	6.563	1638	1640	1644	rVB3	690	393	0.03%	0.004%
32	6.660	1657	1670	1699	rBV	297171	614221	44.06%	5.805%
33	6.853	1727	1730	1734	rVB4	634	435	0.03%	0.004%
34	6.917	1746	1750	1753	rBV2	419	330	0.02%	0.003%
35	7.068	1794	1797	1801	rBV2	457	315	0.02%	0.003%
36	7.126	1812	1815	1821	rVB2	389	351	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063760.D
 Acq On : 21 Nov 2025 11:18
 Operator : MD/SY
 Sample : Q3688-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 RBGW-20251120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.425	1903	1908	1916	rVB2	373	360	0.03%	0.003%
38	7.537	1929	1943	1974	rBV	135774	259877	18.64%	2.456%
39	7.721	1998	2000	2004	rVB2	578	360	0.03%	0.003%
40	7.775	2016	2017	2019	rVV2	660	322	0.02%	0.003%
41	7.785	2019	2020	2026	rVB4	781	548	0.04%	0.005%
42	7.872	2034	2047	2077	rBV	606706	1139676	81.75%	10.771%
43	8.155	2124	2135	2156	rBV2	86259	158840	11.39%	1.501%
44	8.373	2199	2203	2204	rBV	510	258	0.02%	0.002%
45	8.492	2238	2240	2243	rBV2	319	245	0.02%	0.002%
46	8.534	2246	2253	2259	rVB3	781	1089	0.08%	0.010%
47	8.615	2264	2278	2325	rBV3	222910	592834	42.52%	5.603%
48	8.833	2344	2346	2351	rVB5	689	323	0.02%	0.003%
49	9.322	2493	2498	2500	rBV2	419	262	0.02%	0.002%
50	9.393	2507	2520	2557	rBV	579276	1051432	75.42%	9.937%
51	9.579	2577	2578	2584	rVB3	361	275	0.02%	0.003%
52	9.624	2590	2592	2596	rBV2	521	354	0.03%	0.003%
53	9.672	2601	2607	2608	rBV4	860	761	0.05%	0.007%
54	9.904	2675	2679	2683	rVV2	336	317	0.02%	0.003%
55	9.930	2683	2687	2689	rVV	500	358	0.03%	0.003%
56	9.943	2689	2691	2694	rVV	422	284	0.02%	0.003%
57	9.959	2694	2696	2703	rVB2	333	284	0.02%	0.003%
58	9.994	2703	2707	2711	rBV	264	245	0.02%	0.002%
59	10.081	2730	2734	2737	rBV3	729	734	0.05%	0.007%
60	10.116	2741	2745	2753	rVB3	792	835	0.06%	0.008%
61	10.328	2805	2811	2817	rBV2	255	364	0.03%	0.003%
62	10.380	2821	2827	2831	rBV2	287	306	0.02%	0.003%
63	10.463	2847	2853	2861	rVV	861	1041	0.07%	0.010%
64	10.550	2877	2880	2886	rVB2	364	289	0.02%	0.003%
65	10.595	2891	2894	2897	rVV2	358	324	0.02%	0.003%
66	10.624	2897	2903	2912	rVB4	950	1440	0.10%	0.014%
67	10.730	2923	2936	2958	rBV	403923	668546	47.96%	6.318%
68	10.872	2978	2980	2984	rVB2	448	244	0.02%	0.002%
69	10.968	3005	3010	3012	rBV2	275	246	0.02%	0.002%
70	11.071	3038	3042	3051	rVB4	1047	1501	0.11%	0.014%
71	11.200	3079	3082	3086	rVV2	347	260	0.02%	0.002%
72	11.393	3135	3142	3149	rVB2	200	376	0.03%	0.004%
73	11.451	3153	3160	3170	rVV	974	1668	0.12%	0.016%
74	11.621	3211	3213	3219	rBV2	334	391	0.03%	0.004%
75	11.653	3220	3223	3227	rVB	359	276	0.02%	0.003%
76	11.685	3229	3233	3239	rVB2	389	403	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063760.D
 Acq On : 21 Nov 2025 11:18
 Operator : MD/SY
 Sample : Q3688-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 RBGW-20251120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M

Title : VOC Analysis

77	11.730	3239	3247	3251	rBV4	2334	3068	0.22%	0.029%
78	11.788	3252	3265	3290	rBV	590228	1012791	72.65%	9.572%
79	12.042	3340	3344	3349	rBB2	323	299	0.02%	0.003%
80	12.103	3359	3363	3366	rBV2	456	432	0.03%	0.004%
81	12.168	3370	3383	3406	rBV	564109	973058	69.80%	9.196%
82	12.364	3441	3444	3449	rVB4	373	277	0.02%	0.003%
83	12.946	3621	3625	3629	rBV3	338	342	0.02%	0.003%
84	13.139	3682	3685	3688	rBV2	418	285	0.02%	0.003%
85	13.203	3697	3705	3713	rVB6	1955	3024	0.22%	0.029%
86	13.254	3717	3721	3726	rBV2	387	416	0.03%	0.004%
87	13.611	3829	3832	3836	rBV2	322	253	0.02%	0.002%
88	13.669	3846	3850	3852	rBV	477	367	0.03%	0.003%
89	13.695	3853	3858	3863	rVV3	396	532	0.04%	0.005%
90	13.830	3893	3900	3910	rVB5	2662	4775	0.34%	0.045%
91	14.010	3953	3956	3959	rVB2	436	291	0.02%	0.003%
92	14.032	3959	3963	3965	rBV2	307	281	0.02%	0.003%
93	14.077	3972	3977	3989	rVB3	2874	4457	0.32%	0.042%
94	14.306	4043	4048	4049	rBV2	2118	1401	0.10%	0.013%
95	14.637	4148	4151	4156	rBV2	516	456	0.03%	0.004%
96	14.907	4232	4235	4237	rBV3	584	354	0.03%	0.003%
97	14.974	4253	4256	4258	rBV	579	327	0.02%	0.003%
98	15.061	4280	4283	4287	rVB3	707	528	0.04%	0.005%
99	15.357	4373	4375	4377	rBV2	544	323	0.02%	0.003%
100	15.701	4479	4482	4484	rBV3	1010	697	0.05%	0.007%




Sum of corrected areas: 10581285

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063760.D
Acq On : 21 Nov 2025 11:18
Operator : MD/SY
Sample : Q3688-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RBGW-20251120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

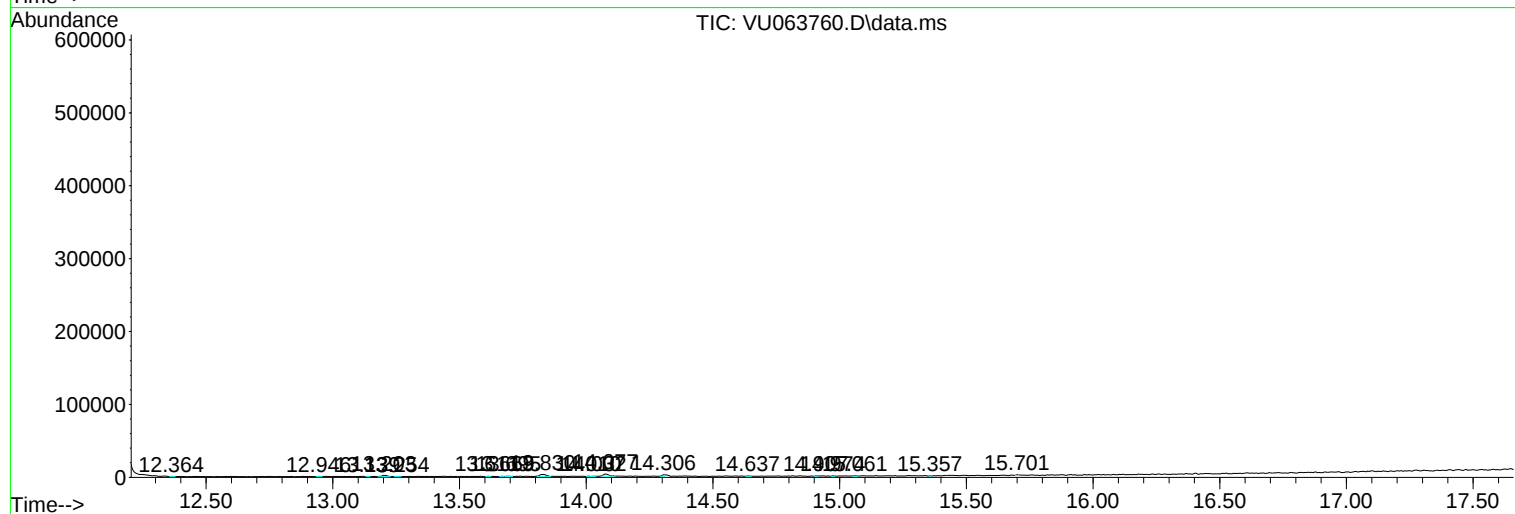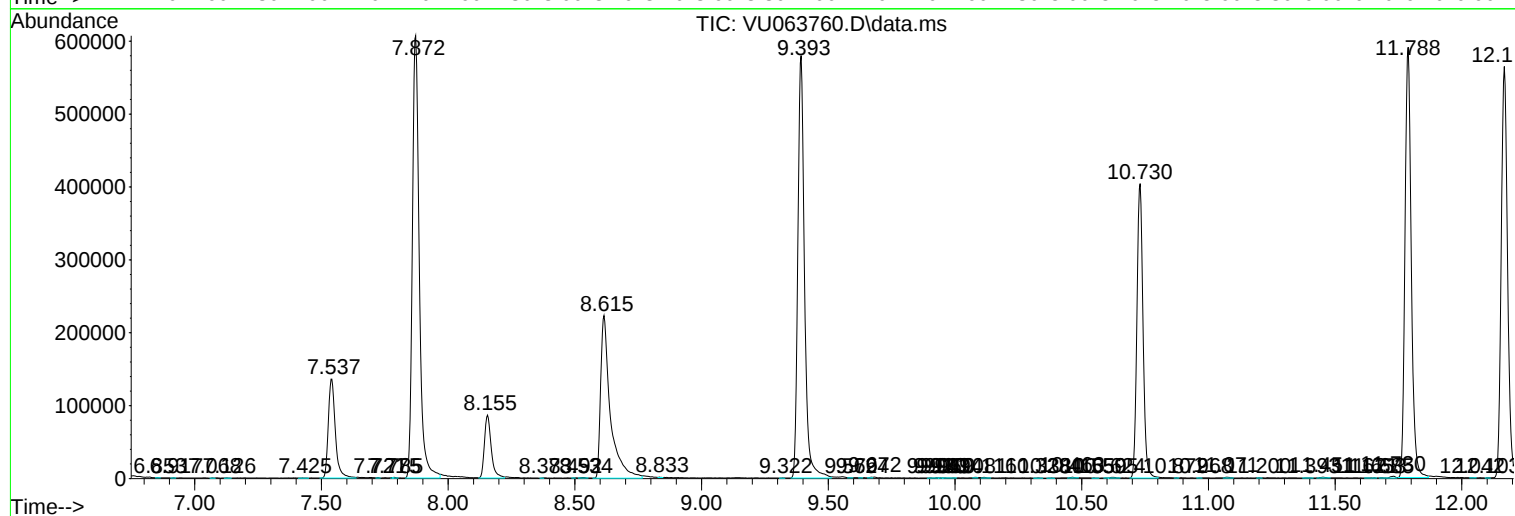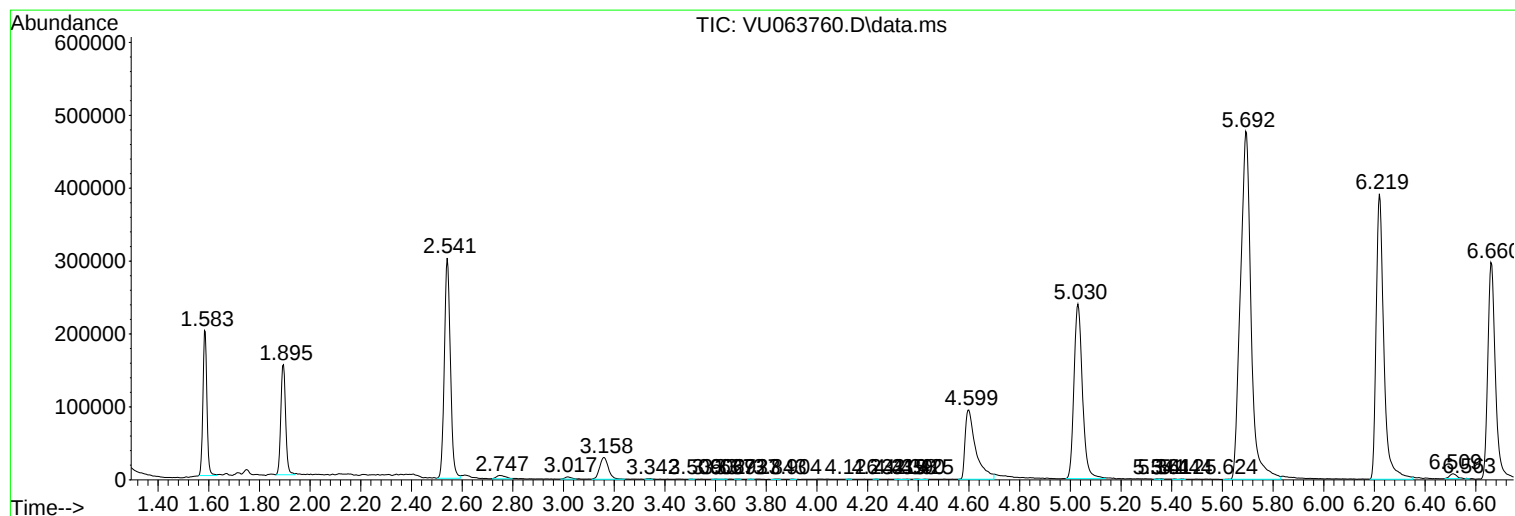

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063760.D
Acq On : 21 Nov 2025 11:18
Operator : MD/SY
Sample : Q3688-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RBGW-20251120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063760.D
Acq On : 21 Nov 2025 11:18
Operator : MD/SY
Sample : Q3688-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RBGW-20251120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
