

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063780.D
 Acq On : 24 Nov 2025 16:15
 Operator : MD/SY
 Sample : Q3688-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TBGW-20251124

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M

Title : VOC Analysis

Signal : TIC: VU063780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.586	84	92	101	rBV	172527	187787	14.56%	1.907%
2	1.895	180	188	205	rVB	133673	172542	13.38%	1.752%
3	2.541	378	389	407	rBV	262664	438429	34.00%	4.452%
4	2.743	441	452	468	rBV	11887	28069	2.18%	0.285%
5	2.949	510	516	520	rBV3	403	581	0.05%	0.006%
6	2.969	520	522	525	rVV	381	260	0.02%	0.003%
7	3.017	529	537	548	rVB4	3272	5981	0.46%	0.061%
8	3.161	564	582	599	rBV	29748	68770	5.33%	0.698%
9	3.332	631	635	645	rVB5	1271	1885	0.15%	0.019%
10	3.621	721	725	730	rVB2	379	260	0.02%	0.003%
11	3.833	787	791	797	rBV2	313	384	0.03%	0.004%
12	3.940	813	824	830	rBV2	361	603	0.05%	0.006%
13	4.065	858	863	868	rBV2	273	285	0.02%	0.003%
14	4.168	892	895	898	rVV	340	238	0.02%	0.002%
15	4.370	956	958	963	rVB	416	283	0.02%	0.003%
16	4.596	1016	1028	1057	rBV	90516	257145	19.94%	2.611%
17	5.030	1147	1163	1199	rVV	219274	511460	39.66%	5.193%
18	5.242	1226	1229	1230	rBV3	438	255	0.02%	0.003%
19	5.274	1236	1239	1241	rBV3	406	246	0.02%	0.002%
20	5.348	1255	1262	1264	rBV4	740	779	0.06%	0.008%
21	5.361	1264	1266	1269	rVB3	646	339	0.03%	0.003%
22	5.528	1314	1318	1320	rBV2	264	241	0.02%	0.002%
23	5.695	1350	1370	1420	rBV2	429218	1289549	100.00%	13.094%
24	6.023	1466	1472	1475	rVV4	685	704	0.05%	0.007%
25	6.219	1521	1533	1563	rBV	380067	787057	61.03%	7.992%
26	6.509	1613	1623	1636	rVB9	5226	11903	0.92%	0.121%
27	6.660	1657	1670	1699	rBV	268483	562049	43.58%	5.707%
28	6.911	1744	1748	1754	rVB2	478	411	0.03%	0.004%
29	7.058	1788	1794	1797	rBV2	403	442	0.03%	0.004%
30	7.132	1814	1817	1821	rVB2	433	241	0.02%	0.002%
31	7.155	1821	1824	1828	rBV	346	286	0.02%	0.003%
32	7.181	1828	1832	1833	rBV	382	262	0.02%	0.003%
33	7.190	1833	1835	1838	rVV2	480	292	0.02%	0.003%
34	7.210	1838	1841	1848	rVV3	324	342	0.03%	0.003%
35	7.251	1852	1854	1860	rVB2	333	247	0.02%	0.003%
36	7.396	1895	1899	1900	rBV	366	297	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063780.D
 Acq On : 24 Nov 2025 16:15
 Operator : MD/SY
 Sample : Q3688-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TBGW-20251124

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.541	1931	1944	1970	rBV	125410	239200	18.55%	2.429%
38	7.656	1976	1980	1988	rVB5	722	809	0.06%	0.008%
39	7.747	2006	2008	2013	rVB2	426	353	0.03%	0.004%
40	7.779	2013	2018	2020	rBV3	630	597	0.05%	0.006%
41	7.872	2034	2047	2081	rBV	546541	1034648	80.23%	10.506%
42	8.155	2125	2135	2160	rVV	80652	147192	11.41%	1.495%
43	8.447	2222	2226	2229	rBV3	359	304	0.02%	0.003%
44	8.470	2229	2233	2238	rBV2	271	298	0.02%	0.003%
45	8.531	2245	2252	2261	rVB6	1200	1893	0.15%	0.019%
46	8.615	2265	2278	2334	rBV3	204634	558515	43.31%	5.671%
47	8.898	2363	2366	2370	rVB3	853	619	0.05%	0.006%
48	8.920	2370	2373	2377	rBV2	457	308	0.02%	0.003%
49	8.975	2387	2390	2395	rVB3	327	271	0.02%	0.003%
50	9.110	2427	2432	2436	rBV2	299	307	0.02%	0.003%
51	9.206	2458	2462	2467	rVB2	326	254	0.02%	0.003%
52	9.232	2467	2470	2473	rBV2	319	249	0.02%	0.003%
53	9.283	2483	2486	2492	rVB2	326	273	0.02%	0.003%
54	9.393	2507	2520	2561	rBV	555089	1012443	78.51%	10.280%
55	9.602	2580	2585	2589	rVB2	318	322	0.02%	0.003%
56	9.624	2589	2592	2597	rBV3	423	339	0.03%	0.003%
57	9.647	2597	2599	2602	rVB2	615	310	0.02%	0.003%
58	9.666	2602	2605	2606	rBV	794	389	0.03%	0.004%
59	9.939	2686	2690	2694	rBV	281	255	0.02%	0.003%
60	10.007	2704	2711	2712	rBV	269	280	0.02%	0.003%
61	10.078	2729	2733	2736	rBV3	714	718	0.06%	0.007%
62	10.107	2740	2742	2750	rVB3	1121	1225	0.09%	0.012%
63	10.187	2764	2767	2773	rVB2	204	258	0.02%	0.003%
64	10.232	2775	2781	2785	rBV2	276	340	0.03%	0.003%
65	10.271	2790	2793	2796	rVB2	400	253	0.02%	0.003%
66	10.357	2817	2820	2824	rBV2	234	261	0.02%	0.003%
67	10.467	2845	2854	2860	rBV4	1300	1974	0.15%	0.020%
68	10.566	2879	2885	2890	rBV2	368	371	0.03%	0.004%
69	10.624	2898	2903	2908	rBV4	861	991	0.08%	0.010%
70	10.730	2923	2936	2960	rBV	382395	635442	49.28%	6.452%
71	10.968	3007	3010	3014	rVB2	405	277	0.02%	0.003%
72	11.071	3038	3042	3052	rVB5	1038	1425	0.11%	0.014%
73	11.139	3057	3063	3067	rBV2	334	316	0.02%	0.003%
74	11.319	3115	3119	3122	rBV	429	353	0.03%	0.004%
75	11.396	3134	3143	3147	rBV2	403	465	0.04%	0.005%
76	11.669	3225	3228	3232	rVB	419	271	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063780.D
 Acq On : 24 Nov 2025 16:15
 Operator : MD/SY
 Sample : Q3688-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TBGW-20251124

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	11.730	3235	3247	3253	rBV7	2241	3806	0.30%	0.039%
78	11.788	3253	3265	3293	rBV	564235	958429	74.32%	9.732%
79	12.087	3355	3358	3361	rVB2	449	276	0.02%	0.003%
80	12.168	3370	3383	3402	rBV	524682	891430	69.13%	9.051%
81	12.341	3435	3437	3443	rVB2	517	470	0.04%	0.005%
82	12.396	3451	3454	3457	rBV	383	246	0.02%	0.002%
83	12.444	3467	3469	3475	rVB2	282	258	0.02%	0.003%
84	12.550	3498	3502	3507	rVB	439	424	0.03%	0.004%
85	12.579	3507	3511	3518	rBV2	489	596	0.05%	0.006%
86	12.740	3559	3561	3567	rVB2	489	345	0.03%	0.004%
87	12.775	3567	3572	3575	rBV2	433	388	0.03%	0.004%
88	12.827	3584	3588	3591	rBV	448	332	0.03%	0.003%
89	13.004	3639	3643	3646	rVB2	489	394	0.03%	0.004%
90	13.042	3651	3655	3662	rVB3	512	674	0.05%	0.007%
91	13.106	3672	3675	3679	rBV	387	307	0.02%	0.003%
92	13.200	3698	3704	3709	rVV6	1134	1611	0.12%	0.016%
93	13.830	3893	3900	3905	rBV4	2494	3496	0.27%	0.035%
94	14.077	3972	3977	3987	rVB4	2434	2832	0.22%	0.029%
95	14.312	4040	4050	4059	rBV4	2429	4154	0.32%	0.042%
96	14.441	4086	4090	4094	rBV2	674	523	0.04%	0.005%
97	14.512	4109	4112	4114	rBV2	313	236	0.02%	0.002%
98	14.618	4140	4145	4146	rBV2	439	291	0.02%	0.003%
99	14.714	4172	4175	4178	rBV	535	423	0.03%	0.004%
100	14.807	4202	4204	4207	rVB3	551	257	0.02%	0.003%




Sum of corrected areas: 9848470

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063780.D
Acq On : 24 Nov 2025 16:15
Operator : MD/SY
Sample : Q3688-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TBGW-20251124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

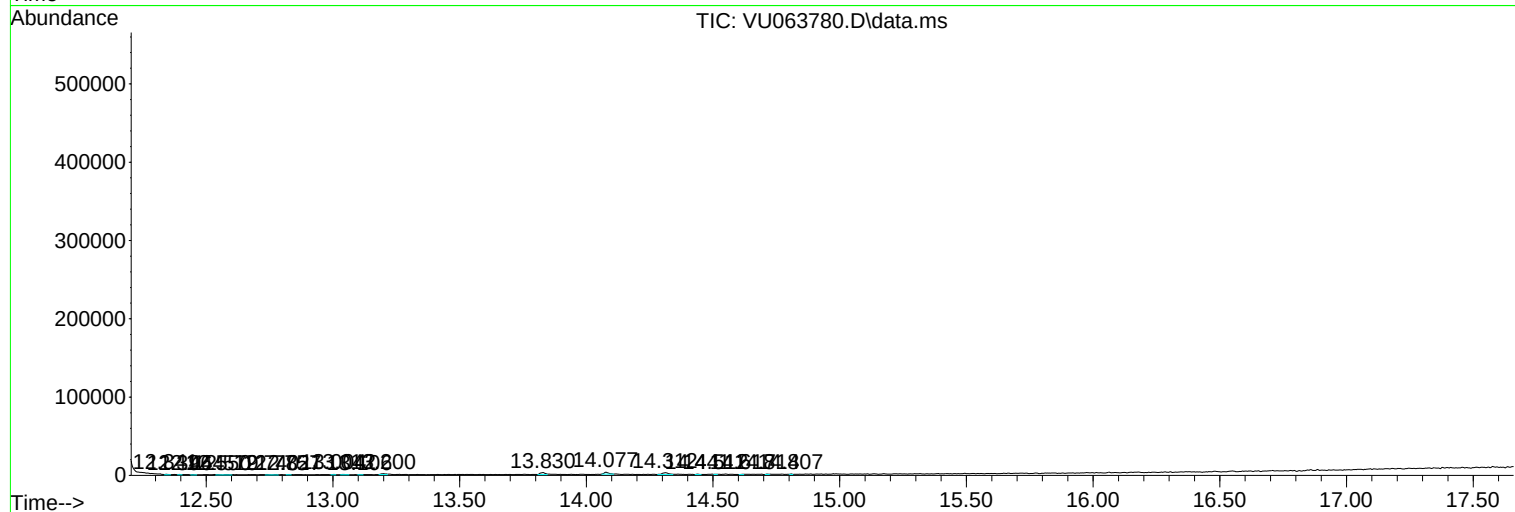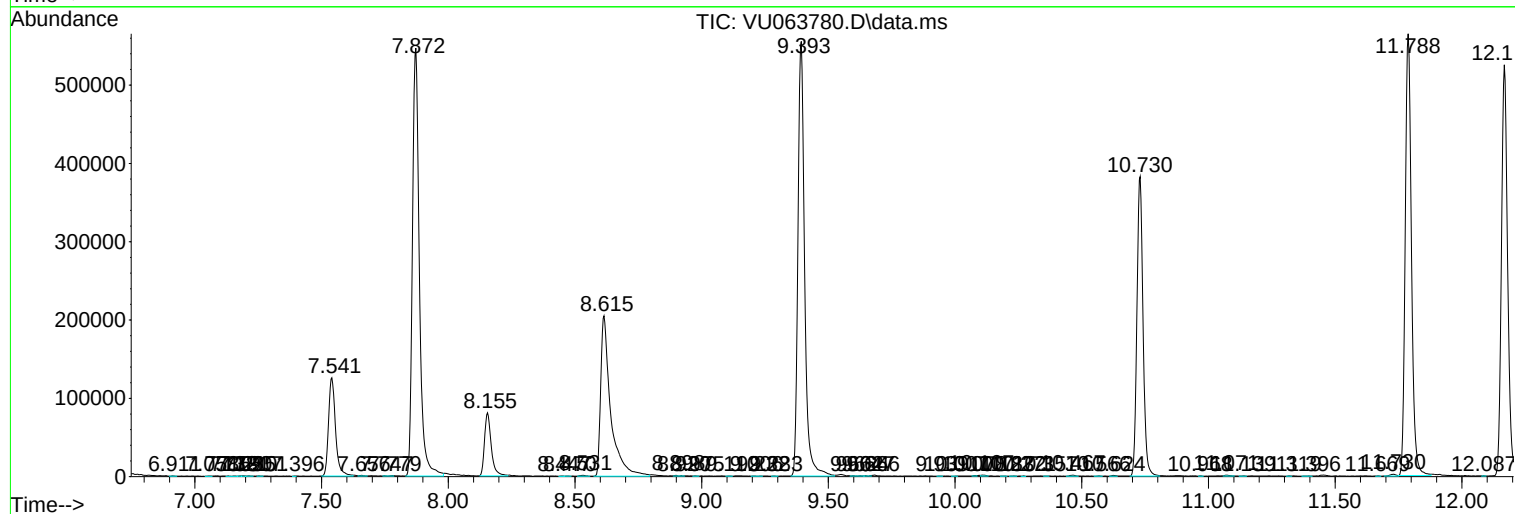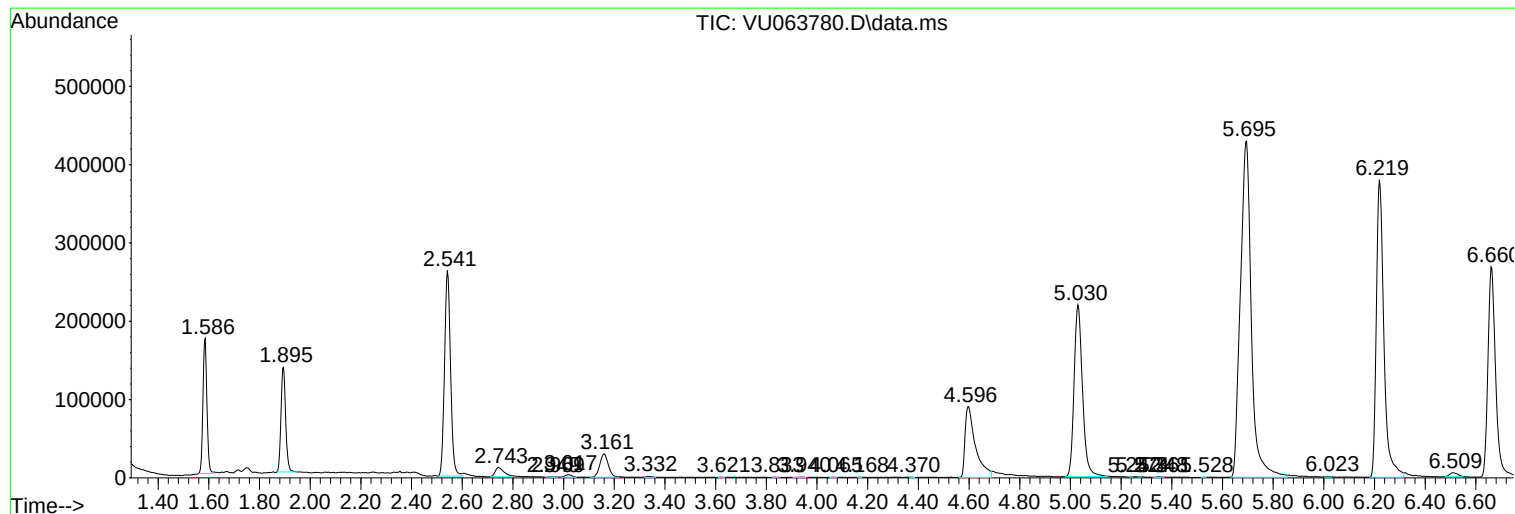

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063780.D
Acq On : 24 Nov 2025 16:15
Operator : MD/SY
Sample : Q3688-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TBGW-20251124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063780.D
Acq On : 24 Nov 2025 16:15
Operator : MD/SY
Sample : Q3688-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TBGW-20251124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
