

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063783.D
 Acq On : 24 Nov 2025 17:28
 Operator : MD/SY
 Sample : Q3688-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-28I

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

Signal : TIC: VU063783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.586	83	92	108	rBV	172292	190372	15.07%	2.005%
2	1.894	180	188	202	rVB	128910	165757	13.12%	1.746%
3	2.541	377	389	405	rBV	255273	424721	33.62%	4.474%
4	2.743	442	452	470	rBV2	14998	35027	2.77%	0.369%
5	2.891	496	498	500	rBV2	442	237	0.02%	0.002%
6	3.020	529	538	540	rBV3	1893	2655	0.21%	0.028%
7	3.058	548	550	555	rVB	368	227	0.02%	0.002%
8	3.100	560	563	566	rBV2	449	332	0.03%	0.003%
9	3.161	567	582	599	rVV	35488	83911	6.64%	0.884%
10	3.335	629	636	647	rVB6	1447	2780	0.22%	0.029%
11	3.505	686	689	694	rVB3	302	274	0.02%	0.003%
12	3.592	713	716	718	rBV2	335	189	0.01%	0.002%
13	3.737	757	761	765	rVB2	322	323	0.03%	0.003%
14	3.804	778	782	785	rBV2	349	295	0.02%	0.003%
15	3.952	824	828	832	rVB2	349	288	0.02%	0.003%
16	3.972	832	834	838	rBV	260	190	0.02%	0.002%
17	4.094	869	872	875	rVB	408	273	0.02%	0.003%
18	4.226	909	913	916	rBV2	309	261	0.02%	0.003%
19	4.264	921	925	927	rBV	268	210	0.02%	0.002%
20	4.447	979	982	987	rVV	293	336	0.03%	0.004%
21	4.473	988	990	996	rVB	356	199	0.02%	0.002%
22	4.502	996	999	1004	rBV	289	186	0.01%	0.002%
23	4.599	1019	1029	1077	rBV	88587	278456	22.04%	2.933%
24	5.029	1147	1163	1191	rBV	221058	510848	40.44%	5.382%
25	5.248	1229	1231	1232	rBV	621	234	0.02%	0.002%
26	5.357	1260	1265	1270	rBV5	684	613	0.05%	0.006%
27	5.431	1285	1288	1290	rBV	494	296	0.02%	0.003%
28	5.537	1319	1321	1326	rVB2	349	221	0.02%	0.002%
29	5.570	1327	1331	1334	rBV	257	211	0.02%	0.002%
30	5.586	1334	1336	1343	rVB2	362	382	0.03%	0.004%
31	5.618	1343	1346	1350	rBV2	468	320	0.03%	0.003%
32	5.692	1350	1369	1412	rBV2	427989	1263126	100.00%	13.306%
33	5.981	1457	1459	1462	rBV4	354	197	0.02%	0.002%
34	6.004	1464	1466	1470	rVB	440	223	0.02%	0.002%
35	6.065	1482	1485	1489	rVB3	442	323	0.03%	0.003%
36	6.087	1489	1492	1495	rBV2	368	215	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063783.D
 Acq On : 24 Nov 2025 17:28
 Operator : MD/SY
 Sample : Q3688-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-28I

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	6.219	1520	1533	1573	rBV	338613	717705	56.82%	7.561%
38	6.512	1612	1624	1634	rBV9	5751	12422	0.98%	0.131%
39	6.660	1657	1670	1703	rBV	265825	553924	43.85%	5.835%
40	7.052	1789	1792	1797	rBV2	198	223	0.02%	0.002%
41	7.081	1797	1801	1804	rVB2	248	222	0.02%	0.002%
42	7.123	1810	1814	1815	rBV	279	205	0.02%	0.002%
43	7.164	1823	1827	1829	rBV2	278	219	0.02%	0.002%
44	7.193	1833	1836	1840	rVV3	359	259	0.02%	0.003%
45	7.447	1909	1915	1917	rVB2	431	409	0.03%	0.004%
46	7.463	1917	1920	1922	rBV	254	193	0.02%	0.002%
47	7.541	1930	1944	1966	rBV	121329	233163	18.46%	2.456%
48	7.692	1989	1991	1993	rBV	430	224	0.02%	0.002%
49	7.772	2013	2016	2017	rBV2	751	422	0.03%	0.004%
50	7.872	2033	2047	2080	rBV	534112	1010692	80.02%	10.647%
51	8.155	2124	2135	2155	rBV	76694	139125	11.01%	1.466%
52	8.473	2229	2234	2236	rBV2	293	199	0.02%	0.002%
53	8.515	2242	2247	2248	rBV	358	311	0.02%	0.003%
54	8.524	2248	2250	2256	rBV3	749	626	0.05%	0.007%
55	8.614	2267	2278	2337	rBV3	195865	553266	43.80%	5.828%
56	8.904	2365	2368	2373	rVB4	1034	854	0.07%	0.009%
57	8.926	2373	2375	2379	rVB3	495	374	0.03%	0.004%
58	8.955	2379	2384	2388	rBV2	618	637	0.05%	0.007%
59	9.100	2427	2429	2435	rVB2	543	452	0.04%	0.005%
60	9.139	2435	2441	2446	rBV3	748	927	0.07%	0.010%
61	9.261	2476	2479	2485	rVB2	394	372	0.03%	0.004%
62	9.393	2507	2520	2563	rVV	494617	913081	72.29%	9.619%
63	9.547	2564	2568	2575	rVB5	1468	2098	0.17%	0.022%
64	9.640	2595	2597	2602	rVB2	589	336	0.03%	0.004%
65	9.679	2602	2609	2621	rBV4	1585	2718	0.22%	0.029%
66	9.753	2627	2632	2635	rBV	294	276	0.02%	0.003%
67	9.888	2671	2674	2677	rBV	299	201	0.02%	0.002%
68	10.087	2727	2736	2737	rBV3	969	1114	0.09%	0.012%
69	10.180	2763	2765	2768	rVB2	409	202	0.02%	0.002%
70	10.241	2781	2784	2788	rVB	316	220	0.02%	0.002%
71	10.460	2848	2852	2855	rBV4	837	736	0.06%	0.008%
72	10.544	2872	2878	2882	rBV2	404	427	0.03%	0.004%
73	10.621	2900	2902	2907	rVB3	677	496	0.04%	0.005%
74	10.647	2907	2910	2914	rBV2	303	229	0.02%	0.002%
75	10.730	2919	2936	2955	rBV	376291	623549	49.37%	6.569%
76	11.071	3026	3042	3047	rBV3	908	1881	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063783.D
 Acq On : 24 Nov 2025 17:28
 Operator : MD/SY
 Sample : Q3688-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-28I

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	11.447	3153	3159	3169	rVV4	1095	1822	0.14%	0.019%
78	11.492	3170	3173	3178	rVB2	512	407	0.03%	0.004%
79	11.730	3241	3247	3253	rVB5	1900	2391	0.19%	0.025%
80	11.788	3253	3265	3288	rBV	506447	861575	68.21%	9.076%
81	11.952	3314	3316	3317	rBV2	491	208	0.02%	0.002%
82	12.167	3370	3383	3406	rBV	511786	878798	69.57%	9.258%
83	12.354	3439	3441	3442	rBV	466	240	0.02%	0.003%
84	12.617	3520	3523	3528	rBV2	239	191	0.02%	0.002%
85	13.019	3643	3648	3653	rBV2	255	341	0.03%	0.004%
86	13.097	3669	3672	3674	rBV	402	280	0.02%	0.003%
87	13.209	3699	3707	3713	rBV4	946	1507	0.12%	0.016%
88	13.261	3720	3723	3724	rBV	358	227	0.02%	0.002%
89	13.344	3746	3749	3753	rBV2	576	457	0.04%	0.005%
90	13.486	3789	3793	3795	rBV	427	334	0.03%	0.004%
91	13.685	3853	3855	3861	rBV3	298	242	0.02%	0.003%
92	13.830	3896	3900	3905	rVB5	1141	1074	0.09%	0.011%
93	13.961	3938	3941	3943	rBV2	317	229	0.02%	0.002%
94	14.312	4045	4050	4052	rBV2	1254	1159	0.09%	0.012%
95	14.640	4150	4152	4154	rBV2	328	193	0.02%	0.002%
96	14.682	4162	4165	4168	rBV2	427	324	0.03%	0.003%
97	14.781	4194	4196	4198	rBV	355	195	0.02%	0.002%
98	14.817	4205	4207	4209	rBV	485	263	0.02%	0.003%
99	14.974	4253	4256	4258	rBV3	446	318	0.03%	0.003%
100	15.203	4325	4327	4328	rBV	455	194	0.02%	0.002%




Sum of corrected areas: 9492666

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063783.D
Acq On : 24 Nov 2025 17:28
Operator : MD/SY
Sample : Q3688-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-28I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

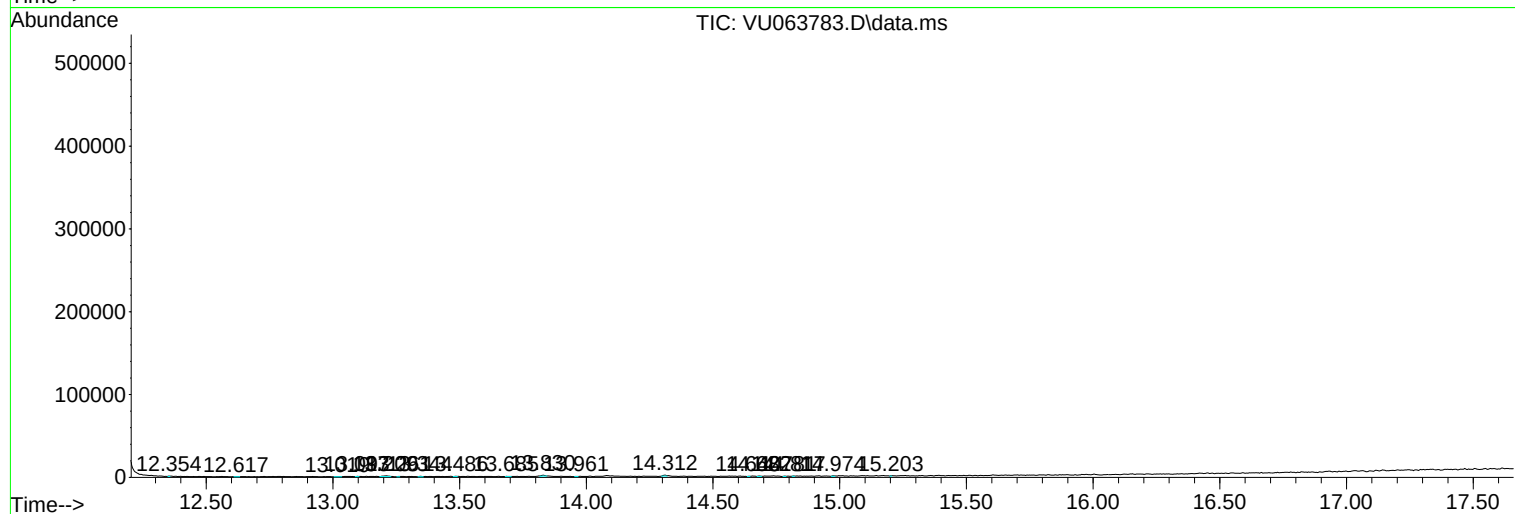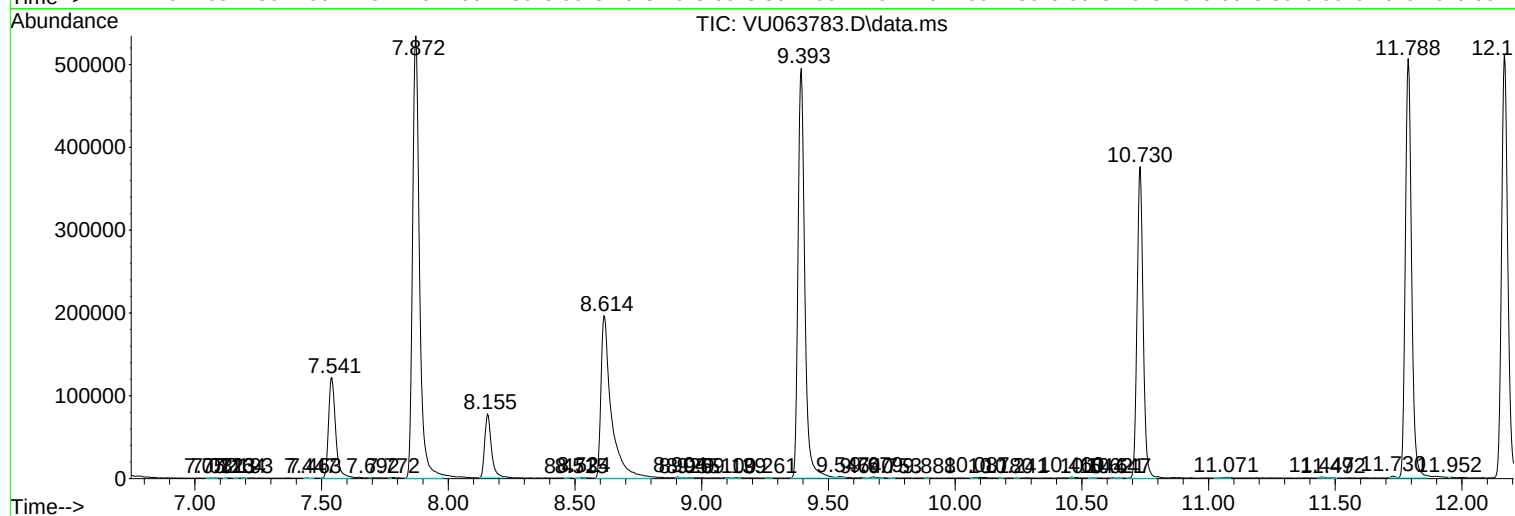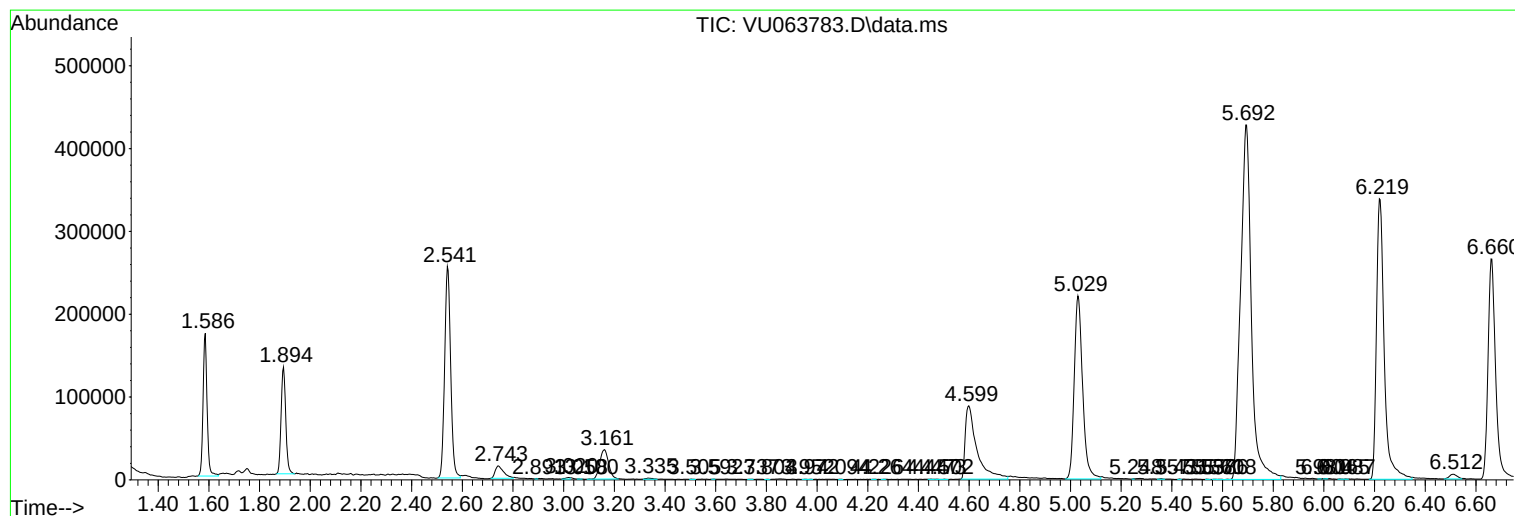

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063783.D
Acq On : 24 Nov 2025 17:28
Operator : MD/SY
Sample : Q3688-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-28I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063783.D
Acq On : 24 Nov 2025 17:28
Operator : MD/SY
Sample : Q3688-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-28I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
