


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112025\
Data File : VN088316.D
Acq On : 20 Nov 2025 08:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N111325W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Nov 14 00:49:21 2025

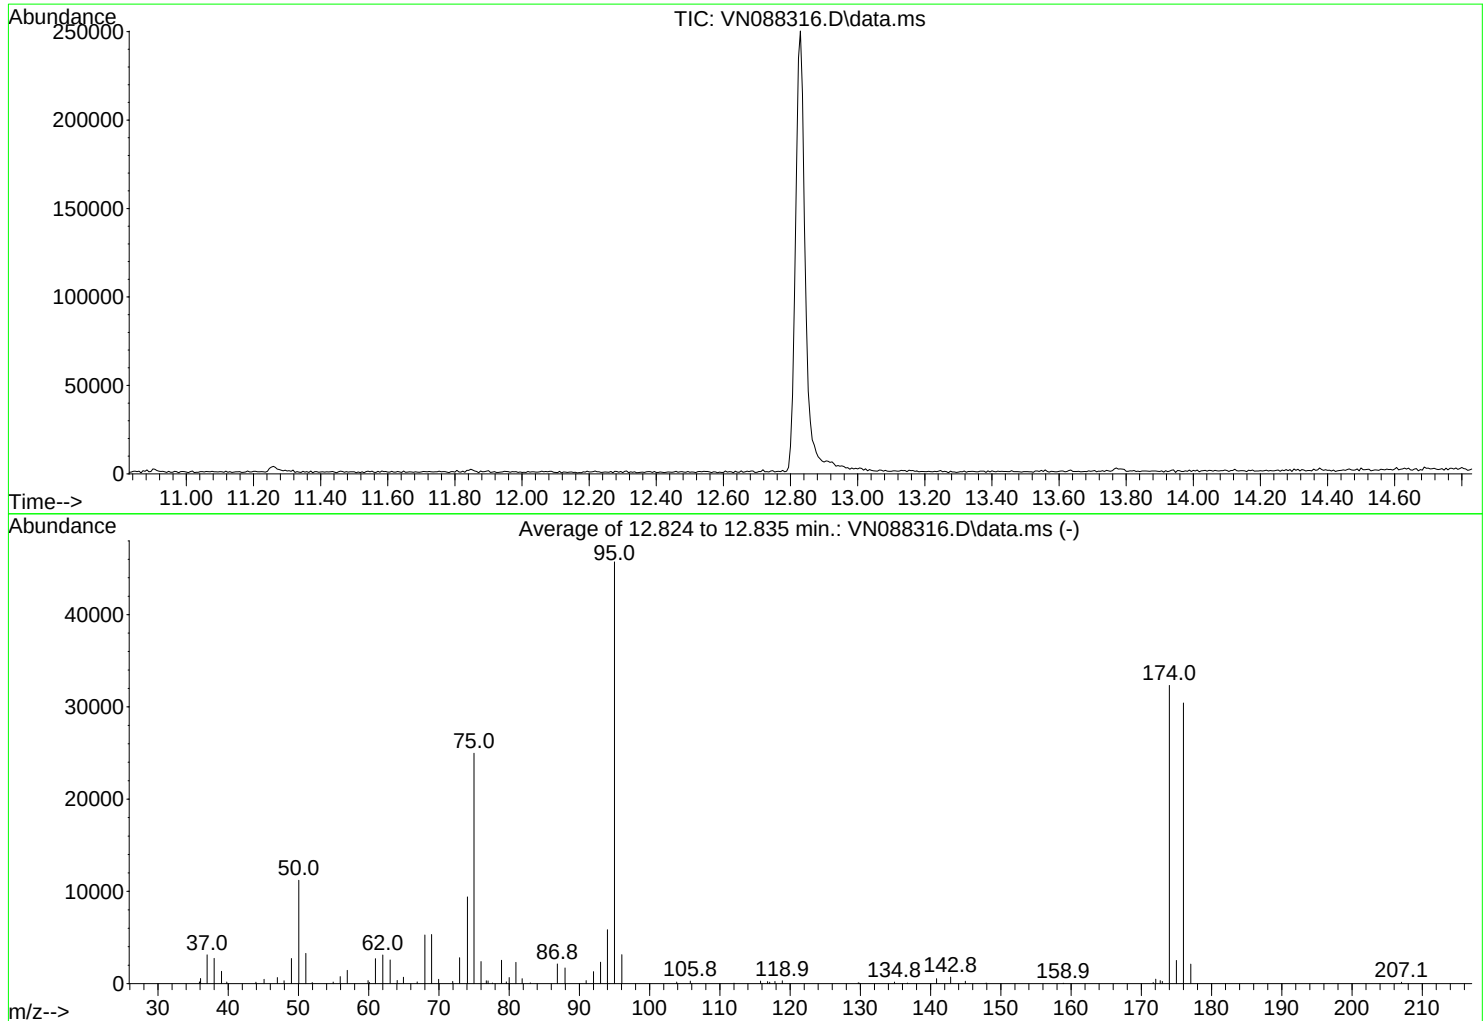

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1841

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.5	11202	PASS
75	95	30	60	54.6	24976	PASS
95	95	100	100	100.0	45725	PASS
96	95	5	9	6.9	3138	PASS
173	174	0.00	2	1.0	331	PASS
174	95	50	100	70.7	32339	PASS
175	174	5	9	7.8	2518	PASS
176	174	95	101	94.1	30429	FAIL*
177	176	5	9	7.0	2121	PASS