


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112725\
Data File : BN038211.D
Acq On : 26 Nov 2025 19:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 28 21:04:10 2025

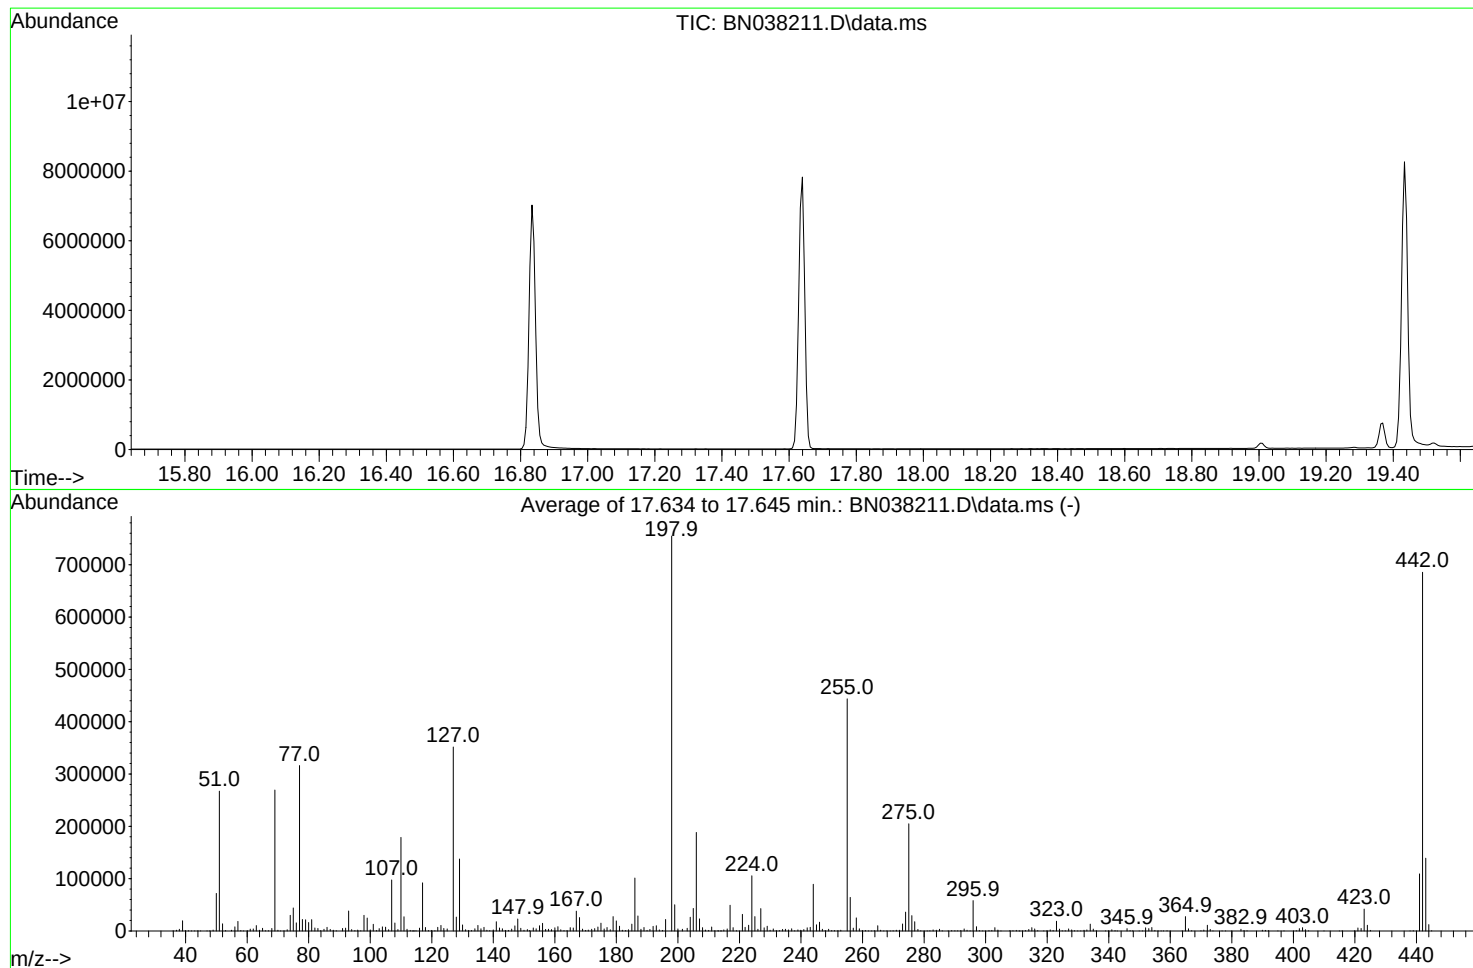




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2465

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	4865	PASS
69	69	100	100	100.0	269184	PASS
70	69	0.00	2	0.5	1321	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	754667	PASS
199	198	5	9	6.6	49939	PASS
365	198	1	100	3.6	27373	PASS
441	443	0.01	150	78.5	109085	PASS
442	442	100	100	100.0	685653	PASS
443	442	15	24	20.3	139035	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112725\
Data File : BN038211.D
Acq On : 26 Nov 2025 19:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 01 17:45:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 10:15:10 2025
Response via : Initial Calibration

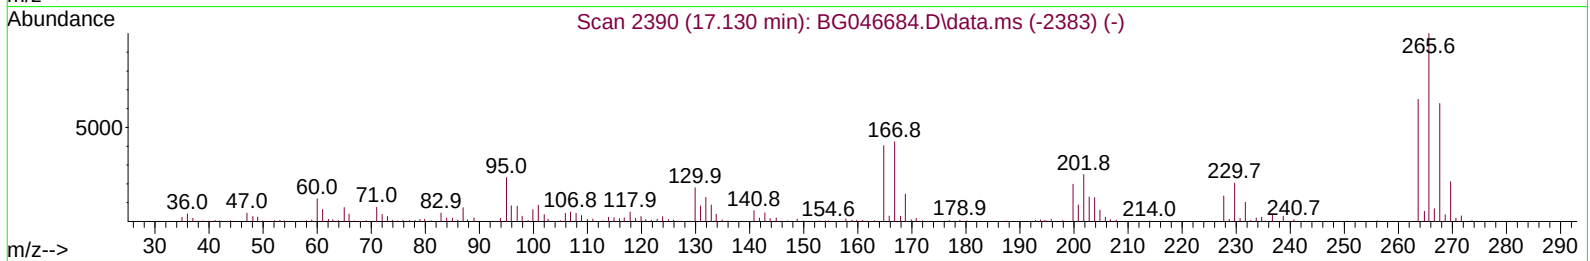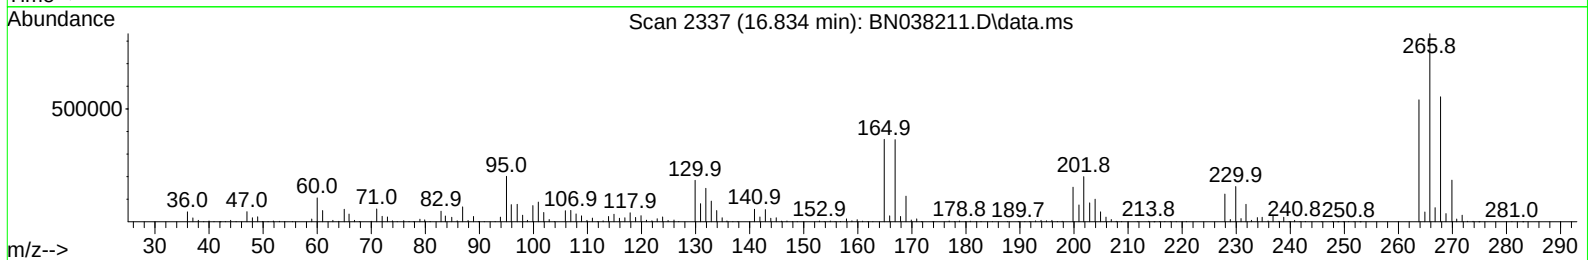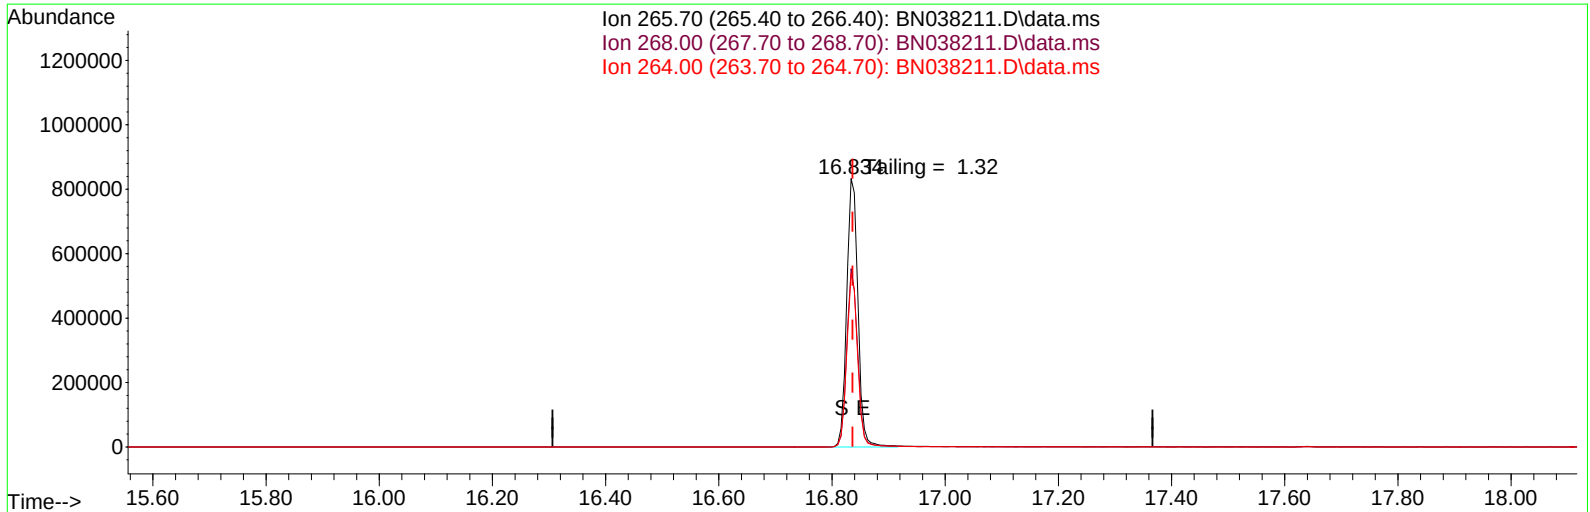

TIC: BN038211.D\data.ms

(70) Pentachlorophenol (C)

16.834min (-0.002) 31780.36 ng




response 1154991

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.41
264.00	61.60	64.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112725\
Data File : BN038211.D
Acq On : 26 Nov 2025 19:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 01 17:45:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 10:15:10 2025
Response via : Initial Calibration

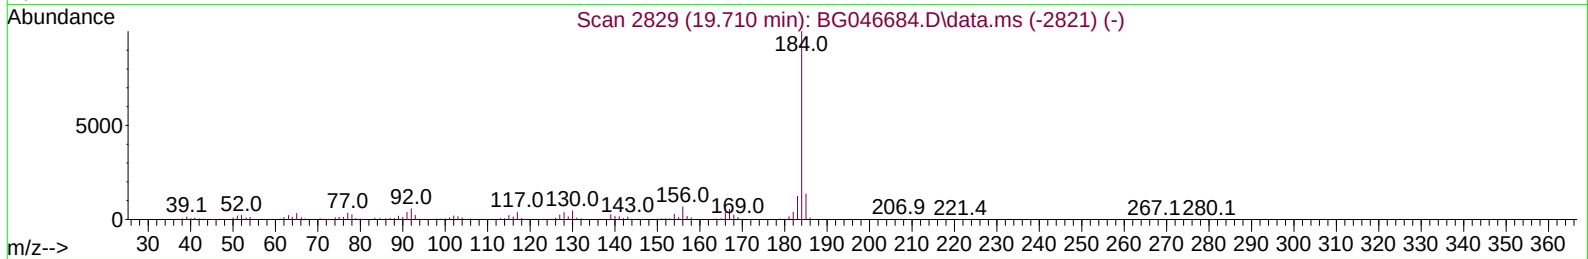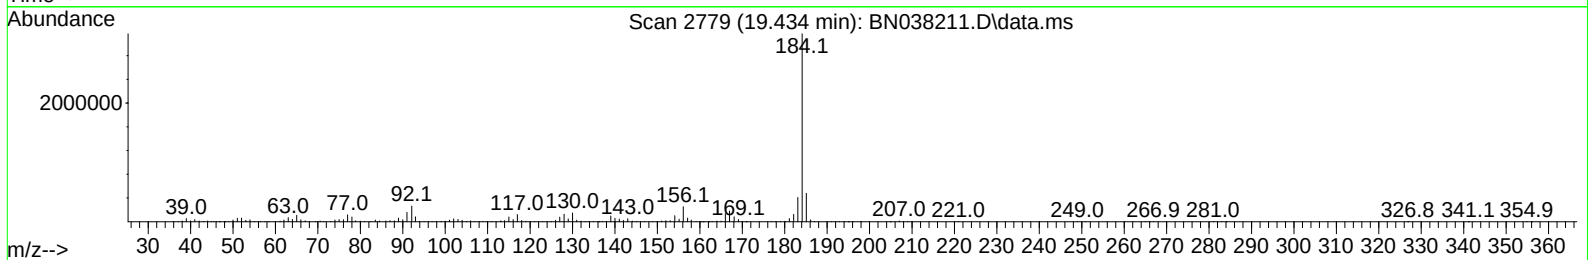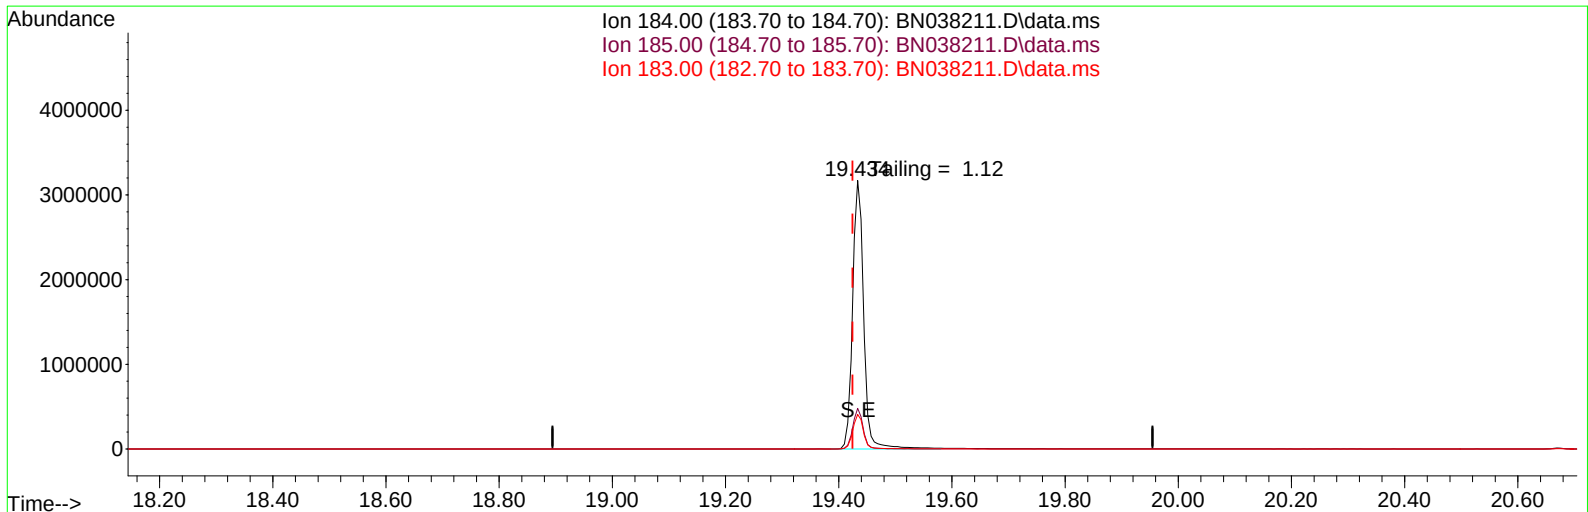

TIC: BN038211.D\data.ms

(77) Benzidine

19.434min (+ 0.009) 0.00 ng

response 4344162

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.12
183.00	13.20	12.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/27/2025	BNA_N	<u>BN038211.D</u>
Compound Name	Response	Retention Time
DDT	2721200	20.675
DDD	25337	20.233
DDE	5413	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30750	2751950	1.12

Instrument :
BNA_N
ClientSampleId :
DFTPP